

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU059000.D
 Acq On : 25 May 2024 15:45
 Operator : MD/SY
 Sample : P2566-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHS0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M

Title : VOC Analysis

Signal : TIC: VU059000.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	88	94	110	rVB	76931	90711	13.74%	1.946%
2	1.888	179	186	203	rVB	62371	90034	13.64%	1.932%
3	2.554	381	393	407	rBV	120063	194297	29.43%	4.168%
4	2.750	453	454	456	rBV	264	109	0.02%	0.002%
5	3.030	536	541	542	rBV2	1372	1123	0.17%	0.024%
6	3.174	573	586	599	rBV	5495	11703	1.77%	0.251%
7	3.512	687	691	694	rBV2	190	172	0.03%	0.004%
8	3.557	701	705	708	rBV2	188	195	0.03%	0.004%
9	3.843	790	794	796	rBV	174	165	0.02%	0.004%
10	3.927	817	820	826	rBV2	81	95	0.01%	0.002%
11	3.959	826	830	833	rBV	255	251	0.04%	0.005%
12	4.004	840	844	847	rBV2	254	193	0.03%	0.004%
13	4.081	866	868	870	rBV	89	41	0.01%	0.001%
14	4.100	870	874	879	rVV2	236	242	0.04%	0.005%
15	4.149	883	889	892	rBV	232	257	0.04%	0.006%
16	4.274	925	928	930	rBV	149	99	0.01%	0.002%
17	4.313	937	940	941	rBV	160	92	0.01%	0.002%
18	4.448	976	982	983	rBV2	160	149	0.02%	0.003%
19	4.518	999	1004	1008	rBV2	189	172	0.03%	0.004%
20	4.608	1022	1032	1059	rBV	69727	172565	26.14%	3.702%
21	5.052	1155	1170	1194	rBV	119455	267539	40.52%	5.740%
22	5.174	1206	1208	1210	rBV	142	71	0.01%	0.002%
23	5.216	1218	1221	1226	rVB	257	218	0.03%	0.005%
24	5.245	1226	1230	1233	rBV2	252	184	0.03%	0.004%
25	5.264	1233	1236	1240	rBV2	321	219	0.03%	0.005%
26	5.444	1288	1292	1294	rBV	181	144	0.02%	0.003%
27	5.457	1294	1296	1301	rVB2	202	128	0.02%	0.003%
28	5.499	1306	1309	1310	rBV	110	66	0.01%	0.001%
29	5.602	1337	1341	1345	rBV	295	284	0.04%	0.006%
30	5.631	1345	1350	1353	rBV	215	186	0.03%	0.004%
31	5.714	1356	1376	1400	rBV2	239737	660201	100.00%	14.164%
32	5.975	1454	1457	1458	rBV	293	140	0.02%	0.003%
33	6.017	1468	1470	1472	rVB	182	74	0.01%	0.002%
34	6.030	1472	1474	1480	rBV2	204	189	0.03%	0.004%
35	6.136	1504	1507	1511	rVB2	331	245	0.04%	0.005%
36	6.158	1511	1514	1516	rBV	133	81	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU059000.D
 Acq On : 25 May 2024 15:45
 Operator : MD/SY
 Sample : P2566-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHS0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	6.242	1527	1540	1561	rBV	172087	329511	49.91%	7.069%
38	6.390	1580	1586	1590	rBV2	431	532	0.08%	0.011%
39	6.457	1605	1607	1608	rBV	150	79	0.01%	0.002%
40	6.531	1620	1630	1638	rVB7	3221	6634	1.00%	0.142%
41	6.583	1643	1646	1647	rBV	233	96	0.01%	0.002%
42	6.602	1647	1652	1656	rVB2	233	274	0.04%	0.006%
43	6.682	1664	1677	1695	rBV	157433	304137	46.07%	6.525%
44	6.808	1714	1716	1719	rVB2	164	52	0.01%	0.001%
45	6.827	1719	1722	1723	rBV	141	67	0.01%	0.001%
46	6.939	1755	1757	1759	rBV	183	107	0.02%	0.002%
47	7.004	1773	1777	1782	rBV	276	263	0.04%	0.006%
48	7.094	1802	1805	1807	rBV	132	95	0.01%	0.002%
49	7.277	1859	1862	1865	rBV2	196	147	0.02%	0.003%
50	7.316	1870	1874	1878	rBV	232	233	0.04%	0.005%
51	7.435	1910	1911	1912	rBV	147	37	0.01%	0.001%
52	7.560	1938	1950	1968	rBV	76628	133949	20.29%	2.874%
53	7.669	1982	1984	1986	rVB2	244	124	0.02%	0.003%
54	7.685	1986	1989	1991	rBV2	272	176	0.03%	0.004%
55	7.756	2008	2011	2014	rBV2	170	114	0.02%	0.002%
56	7.775	2014	2017	2019	rBV2	231	159	0.02%	0.003%
57	7.804	2024	2026	2029	rVV2	186	61	0.01%	0.001%
58	7.891	2041	2053	2069	rBV	262722	461825	69.95%	9.908%
59	8.049	2100	2102	2107	rVB2	367	241	0.04%	0.005%
60	8.174	2130	2141	2161	rBV	52684	89676	13.58%	1.924%
61	8.348	2191	2195	2196	rBV2	253	182	0.03%	0.004%
62	8.470	2223	2233	2243	rBV3	3314	5991	0.91%	0.129%
63	8.582	2263	2268	2271	rBV	187	215	0.03%	0.005%
64	8.624	2271	2281	2317	rBV	178517	347329	52.61%	7.451%
65	8.946	2378	2381	2384	rBV2	230	195	0.03%	0.004%
66	9.020	2402	2404	2406	rBV	237	100	0.02%	0.002%
67	9.113	2431	2433	2436	rBV	155	94	0.01%	0.002%
68	9.197	2457	2459	2461	rBV2	155	51	0.01%	0.001%
69	9.287	2485	2487	2490	rBV2	185	120	0.02%	0.003%
70	9.412	2514	2526	2552	rBV	246576	410080	62.11%	8.798%
71	9.865	2665	2667	2669	rBV	192	79	0.01%	0.002%
72	10.062	2725	2728	2731	rVB	262	144	0.02%	0.003%
73	10.081	2731	2734	2735	rBV	120	71	0.01%	0.002%
74	10.225	2776	2779	2782	rBV2	243	185	0.03%	0.004%
75	10.367	2821	2823	2827	rBV	447	257	0.04%	0.006%
76	10.476	2854	2857	2859	rBV2	238	163	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU059000.D
Acq On : 25 May 2024 15:45
Operator : MD/SY
Sample : P2566-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M

Title : VOC Analysis

77	10.586	2888	2891	2897	rBV2	314	331	0.05%	0.007%
78	10.750	2930	2942	2964	rBV2	216613	346259	52.45%	7.428%
79	10.888	2978	2985	2996	rVB4	4149	6064	0.92%	0.130%
80	11.090	3045	3048	3051	rBV2	464	312	0.05%	0.007%
81	11.135	3059	3062	3065	rVB	256	154	0.02%	0.003%
82	11.698	3234	3237	3242	rBV3	523	437	0.07%	0.009%
83	11.743	3247	3251	3255	rBV	670	466	0.07%	0.010%
84	11.807	3259	3271	3290	rBV	209312	339172	51.37%	7.276%
85	11.962	3317	3319	3326	rVB3	453	343	0.05%	0.007%
86	12.187	3377	3389	3417	rBV	227654	377687	57.21%	8.103%
87	12.901	3603	3611	3620	rBV6	1750	3529	0.53%	0.076%




Sum of corrected areas: 4661233

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU059000.D
Acq On : 25 May 2024 15:45
Operator : MD/SY
Sample : P2566-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

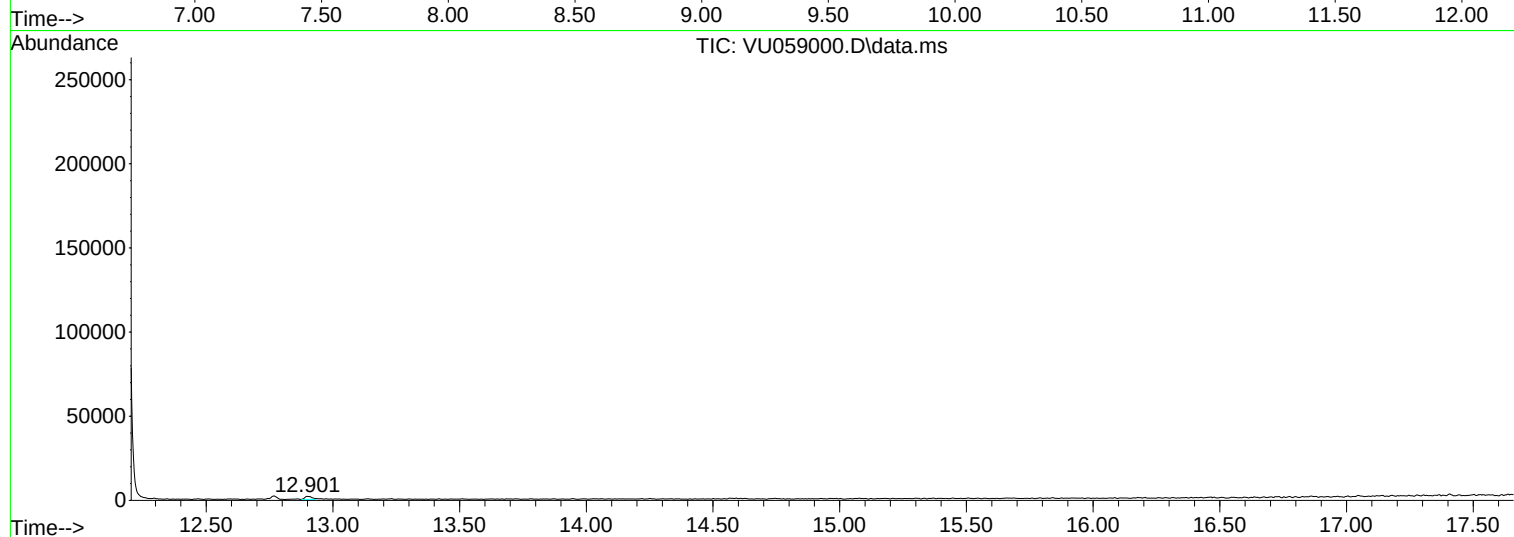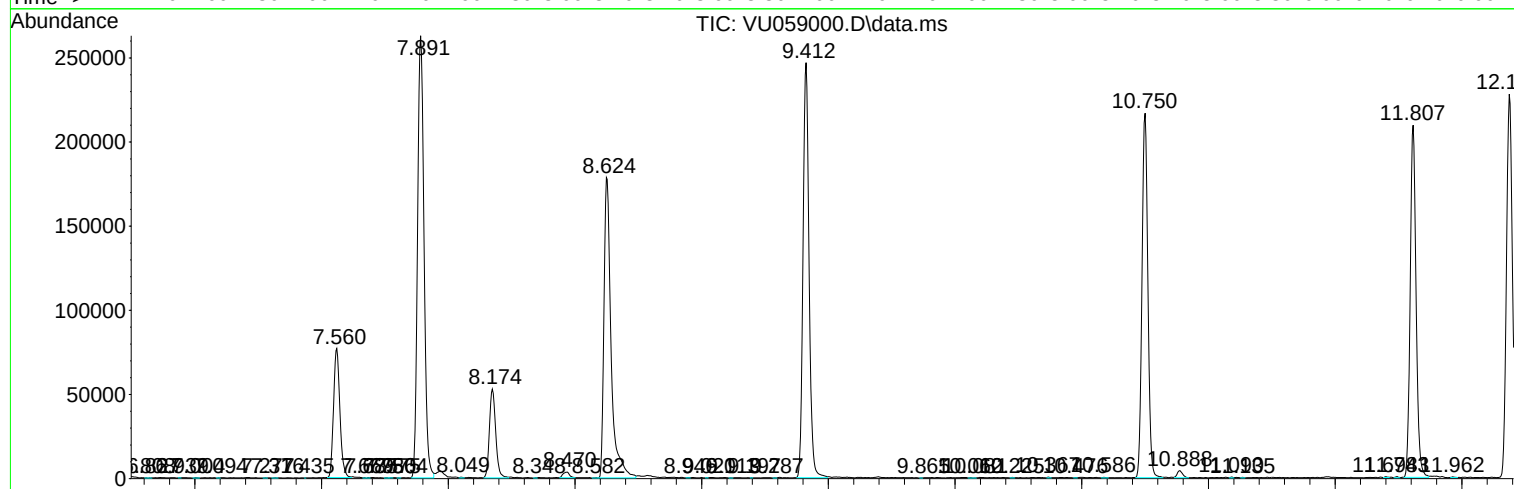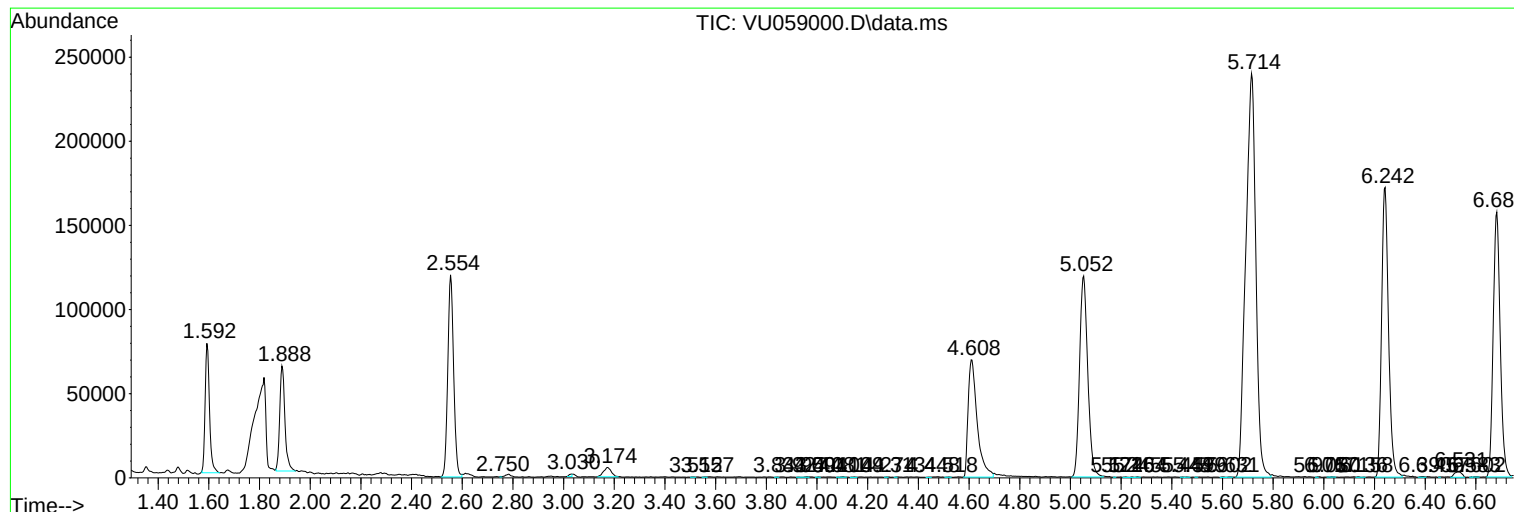

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU059000.D
Acq On : 25 May 2024 15:45
Operator : MD/SY
Sample : P2566-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU059000.D
Acq On : 25 May 2024 15:45
Operator : MD/SY
Sample : P2566-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------