

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU059007.D
 Acq On : 25 May 2024 18:37
 Operator : MD/SY
 Sample : P2596-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

Signal : TIC: VU059007.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.515	67	70	77	rVB3	1784	1497	0.21%	0.029%
2	1.592	86	94	111	rVB	72798	93573	13.29%	1.798%
3	1.872	177	181	200	rVB2	146565	233874	33.20%	4.494%
4	2.489	371	373	376	rVB3	401	204	0.03%	0.004%
5	2.547	379	391	406	rVV	128252	207475	29.46%	3.987%
6	2.624	407	415	428	rVB2	2960	5730	0.81%	0.110%
7	2.724	443	446	450	rVB2	237	204	0.03%	0.004%
8	2.772	453	461	477	rVB	1822	3119	0.44%	0.060%
9	2.846	481	484	487	rVB	335	200	0.03%	0.004%
10	2.869	487	491	495	rVB3	262	231	0.03%	0.004%
11	3.030	532	541	553	rBV4	2078	3873	0.55%	0.074%
12	3.113	561	567	572	rBV4	957	1289	0.18%	0.025%
13	3.178	574	587	601	rVV2	5628	12856	1.83%	0.247%
14	3.361	641	644	647	rVV2	237	183	0.03%	0.004%
15	3.383	647	651	657	rVV2	342	416	0.06%	0.008%
16	3.618	721	724	727	rBV	273	194	0.03%	0.004%
17	3.917	814	817	820	rBV	233	180	0.03%	0.003%
18	3.965	829	832	836	rVB2	346	164	0.02%	0.003%
19	3.994	836	841	847	rVB2	322	387	0.05%	0.007%
20	4.126	878	882	885	rBV2	201	197	0.03%	0.004%
21	4.197	899	904	906	rBV2	228	179	0.03%	0.003%
22	4.615	1023	1034	1074	rBV2	69620	194602	27.63%	3.740%
23	4.827	1098	1100	1107	rVB3	355	352	0.05%	0.007%
24	4.917	1124	1128	1134	rBV3	316	318	0.05%	0.006%
25	4.975	1140	1146	1149	rVB2	349	313	0.04%	0.006%
26	5.049	1154	1169	1195	rBV	124594	277963	39.46%	5.342%
27	5.714	1356	1376	1401	rBV2	260863	704335	100.00%	13.535%
28	5.843	1414	1416	1420	rVB2	308	164	0.02%	0.003%
29	5.936	1440	1445	1449	rBV3	221	204	0.03%	0.004%
30	5.975	1454	1457	1465	rVB3	482	539	0.08%	0.010%
31	6.026	1469	1473	1477	rBV2	179	195	0.03%	0.004%
32	6.171	1515	1518	1522	rVB	451	370	0.05%	0.007%
33	6.238	1522	1539	1562	rBV	185162	360252	51.15%	6.923%
34	6.399	1586	1589	1592	rBV	237	207	0.03%	0.004%
35	6.464	1606	1609	1613	rBV3	186	167	0.02%	0.003%
36	6.531	1620	1630	1637	rVV7	3701	6307	0.90%	0.121%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU059007.D
 Acq On : 25 May 2024 18:37
 Operator : MD/SY
 Sample : P2596-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	6.595	1646	1650	1652	rBV	369	304	0.04%	0.006%
38	6.679	1663	1676	1699	rBV	168638	328853	46.69%	6.320%
39	7.013	1775	1780	1783	rBV	163	172	0.02%	0.003%
40	7.046	1787	1790	1798	rBB2	217	209	0.03%	0.004%
41	7.197	1834	1837	1840	rVB3	379	228	0.03%	0.004%
42	7.213	1840	1842	1845	rBV3	196	168	0.02%	0.003%
43	7.361	1885	1888	1891	rVB	302	191	0.03%	0.004%
44	7.444	1911	1914	1919	rVB2	241	173	0.02%	0.003%
45	7.560	1936	1950	1971	rBV	80769	143583	20.39%	2.759%
46	7.705	1991	1995	1999	rBV2	226	246	0.03%	0.005%
47	7.727	1999	2002	2008	rVB2	348	218	0.03%	0.004%
48	7.785	2013	2020	2022	rBV2	207	264	0.04%	0.005%
49	7.891	2036	2053	2074	rBV	288242	498265	70.74%	9.575%
50	8.081	2109	2112	2122	rVB3	405	492	0.07%	0.009%
51	8.174	2129	2141	2158	rBV	55611	94190	13.37%	1.810%
52	8.467	2222	2232	2242	rVB3	3243	5278	0.75%	0.101%
53	8.631	2272	2283	2319	rBV	194617	399494	56.72%	7.677%
54	8.808	2336	2338	2344	rVV2	272	250	0.04%	0.005%
55	8.840	2345	2348	2353	rVB3	404	312	0.04%	0.006%
56	8.891	2362	2364	2367	rBV	345	163	0.02%	0.003%
57	8.923	2368	2374	2377	rVB3	418	377	0.05%	0.007%
58	8.949	2377	2382	2383	rBV	316	194	0.03%	0.004%
59	8.997	2393	2397	2399	rBV	343	231	0.03%	0.004%
60	9.158	2443	2447	2448	rBV	230	168	0.02%	0.003%
61	9.412	2514	2526	2550	rBV	265119	436964	62.04%	8.397%
62	9.663	2600	2604	2607	rBV	289	277	0.04%	0.005%
63	9.695	2607	2614	2625	rVB4	1135	1643	0.23%	0.032%
64	9.971	2692	2700	2703	rBV2	218	315	0.04%	0.006%
65	10.103	2738	2741	2745	rVB2	384	310	0.04%	0.006%
66	10.441	2842	2846	2853	rVB2	185	184	0.03%	0.004%
67	10.566	2882	2885	2889	rBV2	165	169	0.02%	0.003%
68	10.750	2930	2942	2965	rVV	239398	393718	55.90%	7.566%
69	10.833	2965	2968	2972	rVB2	367	270	0.04%	0.005%
70	10.885	2977	2984	2996	rVB4	3496	5491	0.78%	0.106%
71	10.997	3017	3019	3025	rVB2	222	190	0.03%	0.004%
72	11.097	3048	3050	3055	rVB	260	168	0.02%	0.003%
73	11.190	3076	3079	3085	rVB2	332	330	0.05%	0.006%
74	11.418	3147	3150	3154	rVB	250	194	0.03%	0.004%
75	11.479	3166	3169	3179	rVB2	415	282	0.04%	0.005%
76	11.560	3188	3194	3201	rVB2	368	451	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU059007.D
 Acq On : 25 May 2024 18:37
 Operator : MD/SY
 Sample : P2596-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

77	11.592	3201	3204	3208	rBV	244	180	0.03%	0.003%
78	11.807	3260	3271	3293	rBV	225089	368076	52.26%	7.073%
79	12.087	3355	3358	3363	rVB	413	254	0.04%	0.005%
80	12.190	3378	3390	3413	rBV	238782	399903	56.78%	7.685%
81	12.672	3537	3540	3545	rBV2	232	235	0.03%	0.005%
82	12.766	3564	3569	3577	rVB3	1428	2272	0.32%	0.044%
83	12.843	3590	3593	3596	rBV	356	245	0.03%	0.005%
84	13.241	3713	3717	3719	rBV2	218	192	0.03%	0.004%
85	13.280	3726	3729	3732	rBV2	208	167	0.02%	0.003%
86	13.788	3885	3887	3891	rBV	322	192	0.03%	0.004%
87	13.852	3905	3907	3914	rVB2	257	227	0.03%	0.004%
88	13.884	3914	3917	3922	rBV	266	170	0.02%	0.003%
89	14.097	3977	3983	3984	rBV2	315	284	0.04%	0.005%
90	14.187	4008	4011	4014	rBV	337	226	0.03%	0.004%
91	14.425	4082	4085	4089	rBV2	332	272	0.04%	0.005%
92	14.547	4121	4123	4126	rBV2	350	166	0.02%	0.003%
93	14.566	4126	4129	4139	rVB2	410	640	0.09%	0.012%
94	14.788	4196	4198	4202	rVB	646	401	0.06%	0.008%
95	14.817	4202	4207	4210	rBV3	518	558	0.08%	0.011%
96	14.971	4250	4255	4257	rBV3	378	370	0.05%	0.007%
97	15.206	4325	4328	4332	rBV	310	298	0.04%	0.006%
98	15.280	4348	4351	4354	rBV2	396	295	0.04%	0.006%
99	15.515	4421	4424	4429	rBV3	331	285	0.04%	0.005%
100	16.691	4787	4790	4792	rBV3	653	429	0.06%	0.008%




Sum of corrected areas: 5203629

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU059007.D
Acq On : 25 May 2024 18:37
Operator : MD/SY
Sample : P2596-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

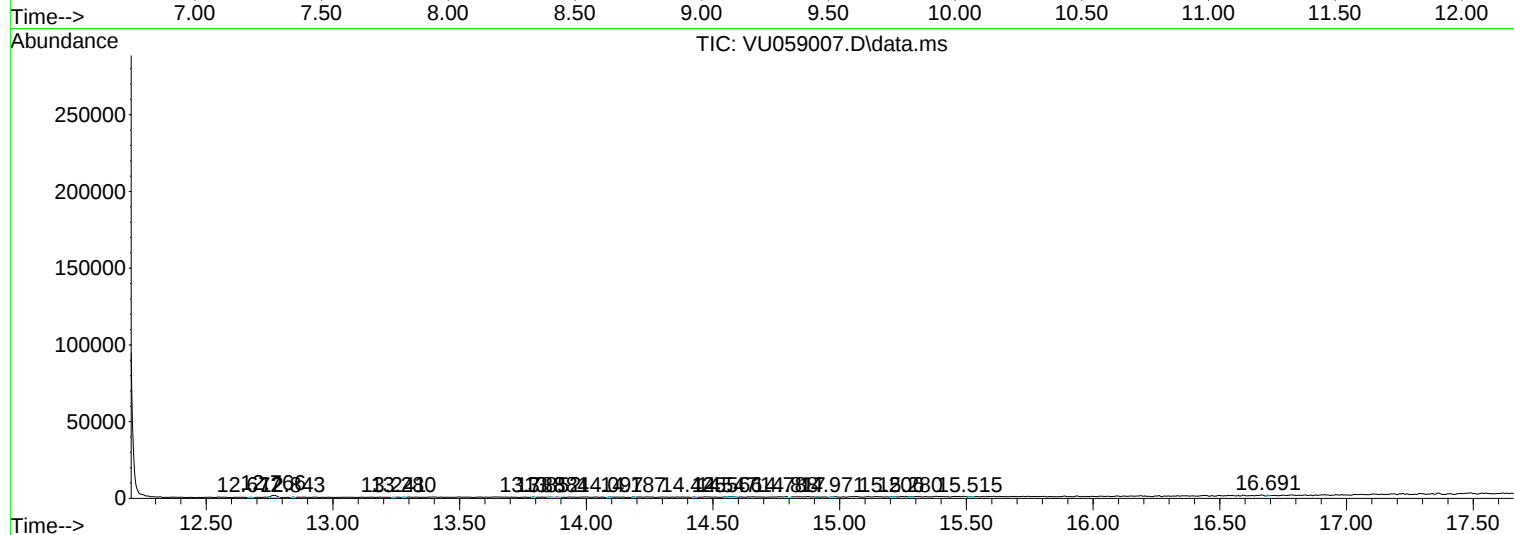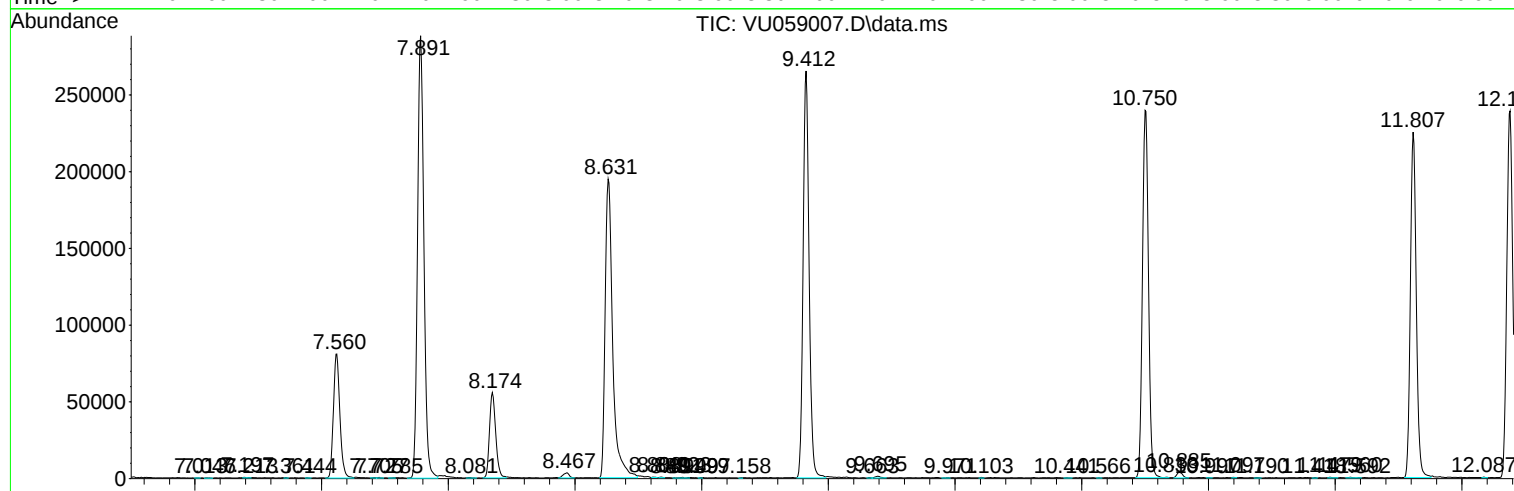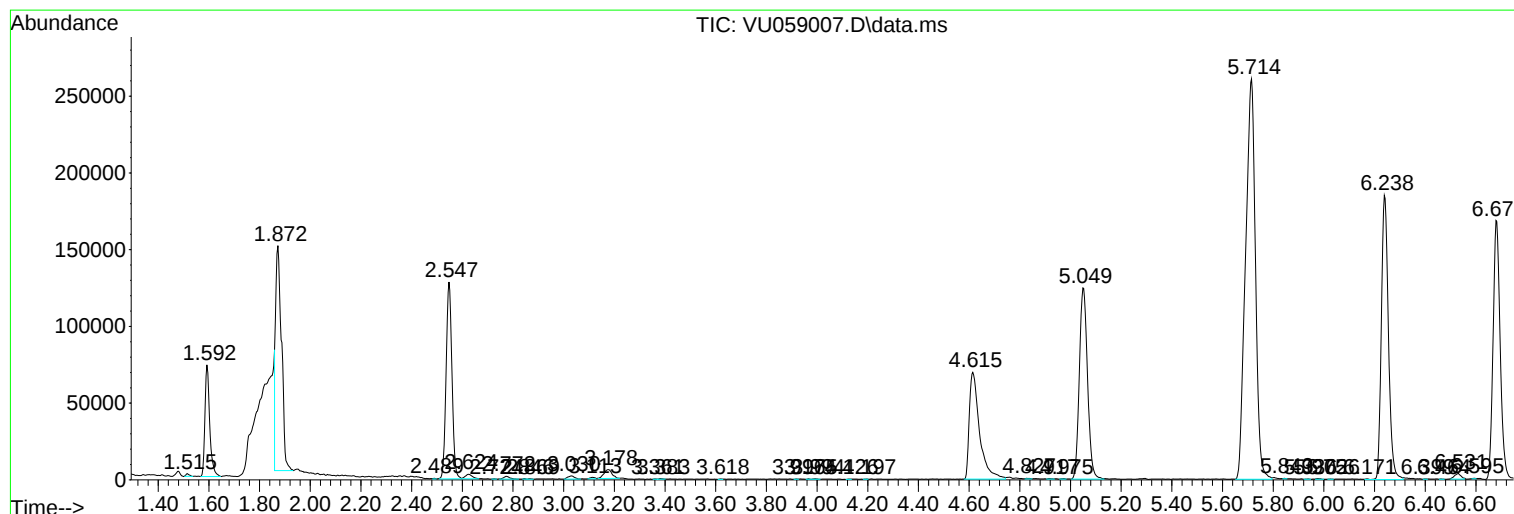

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU059007.D
Acq On : 25 May 2024 18:37
Operator : MD/SY
Sample : P2596-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU059007.D
Acq On : 25 May 2024 18:37
Operator : MD/SY
Sample : P2596-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc