

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU059009.D
 Acq On : 25 May 2024 19:26
 Operator : MD/SY
 Sample : P2596-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M

Title : VOC Analysis

Signal : TIC: VU059009.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.351	15	19	29	rVB	15610	16295	2.31%	0.332%
2	1.592	85	94	110	rBV	81390	106287	15.09%	2.163%
3	2.551	380	392	406	rBV	127665	207229	29.41%	4.216%
4	2.731	444	448	453	rBV2	299	359	0.05%	0.007%
5	2.843	477	483	488	rBV4	800	1159	0.16%	0.024%
6	2.994	528	530	532	rBV2	97	56	0.01%	0.001%
7	3.033	533	542	554	rVB4	1859	3417	0.48%	0.070%
8	3.174	574	586	601	rVB2	4171	9163	1.30%	0.186%
9	3.367	645	646	647	rBV	192	47	0.01%	0.001%
10	3.380	647	650	653	rVV	207	145	0.02%	0.003%
11	3.679	741	743	752	rVB3	274	326	0.05%	0.007%
12	3.750	762	765	769	rVB2	143	121	0.02%	0.002%
13	3.795	771	779	782	rBV2	284	359	0.05%	0.007%
14	3.862	797	800	803	rBV	209	145	0.02%	0.003%
15	3.965	830	832	834	rVB	116	49	0.01%	0.001%
16	3.981	834	837	839	rBV2	161	88	0.01%	0.002%
17	4.020	846	849	853	rBV	141	111	0.02%	0.002%
18	4.071	862	865	869	rBV	201	155	0.02%	0.003%
19	4.094	869	872	878	rVV2	158	149	0.02%	0.003%
20	4.242	913	918	923	rBV2	328	426	0.06%	0.009%
21	4.303	933	937	940	rBV	192	170	0.02%	0.003%
22	4.441	976	980	984	rVB2	249	175	0.02%	0.004%
23	4.464	984	987	990	rBV	148	136	0.02%	0.003%
24	4.502	997	999	1002	rBV	223	130	0.02%	0.003%
25	4.573	1017	1021	1023	rBV	237	160	0.02%	0.003%
26	4.612	1023	1033	1060	rBV	73890	186217	26.43%	3.789%
27	5.052	1154	1170	1191	rBV	126594	284113	40.32%	5.781%
28	5.271	1233	1238	1240	rBV2	430	369	0.05%	0.008%
29	5.383	1270	1273	1276	rVB2	158	117	0.02%	0.002%
30	5.409	1276	1281	1284	rBV2	233	200	0.03%	0.004%
31	5.422	1284	1285	1287	rVB	136	48	0.01%	0.001%
32	5.435	1287	1289	1292	rBV2	215	121	0.02%	0.002%
33	5.499	1307	1309	1312	rVB	188	106	0.02%	0.002%
34	5.550	1323	1325	1326	rBV	134	63	0.01%	0.001%
35	5.576	1330	1333	1336	rVV2	218	146	0.02%	0.003%
36	5.618	1345	1346	1349	rVB	192	56	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU059009.D
 Acq On : 25 May 2024 19:26
 Operator : MD/SY
 Sample : P2596-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	5.634	1349	1351	1353	rBV	73	43	0.01%	0.001%
38	5.714	1355	1376	1401	rBV2	258377	704580	100.00%	14.336%
39	5.946	1446	1448	1449	rBV	185	62	0.01%	0.001%
40	5.968	1453	1455	1458	rVB2	334	158	0.02%	0.003%
41	6.017	1465	1470	1474	rVB2	278	250	0.04%	0.005%
42	6.039	1474	1477	1478	rBV2	101	64	0.01%	0.001%
43	6.052	1478	1481	1485	rVV2	242	156	0.02%	0.003%
44	6.238	1527	1539	1569	rBV	179033	345761	49.07%	7.035%
45	6.431	1597	1599	1601	rBV	214	115	0.02%	0.002%
46	6.467	1609	1610	1612	rBV	252	80	0.01%	0.002%
47	6.528	1619	1629	1641	rVB9	3701	7822	1.11%	0.159%
48	6.579	1643	1645	1647	rBV3	371	177	0.03%	0.004%
49	6.682	1663	1677	1701	rBV2	165167	324147	46.01%	6.595%
50	6.804	1711	1715	1716	rBV	522	338	0.05%	0.007%
51	6.872	1734	1736	1737	rVB	196	48	0.01%	0.001%
52	6.885	1737	1740	1745	rVB	276	203	0.03%	0.004%
53	6.910	1745	1748	1750	rBV	176	131	0.02%	0.003%
54	7.029	1781	1785	1789	rVB2	254	208	0.03%	0.004%
55	7.100	1804	1807	1813	rBV2	187	169	0.02%	0.003%
56	7.274	1859	1861	1863	rBV	80	45	0.01%	0.001%
57	7.390	1894	1897	1900	rBV	207	118	0.02%	0.002%
58	7.476	1921	1924	1931	rBV2	206	238	0.03%	0.005%
59	7.557	1938	1949	1966	rBV	78279	138842	19.71%	2.825%
60	7.705	1987	1995	1998	rBV2	214	311	0.04%	0.006%
61	7.795	2021	2023	2026	rVB2	214	99	0.01%	0.002%
62	7.814	2027	2029	2031	rVB	132	49	0.01%	0.001%
63	7.891	2041	2053	2070	rBV	284415	493546	70.05%	10.042%
64	8.094	2114	2116	2118	rBV3	255	151	0.02%	0.003%
65	8.174	2128	2141	2160	rBV2	53730	93299	13.24%	1.898%
66	8.467	2221	2232	2242	rVB4	2585	4568	0.65%	0.093%
67	8.550	2252	2258	2262	rVB4	956	849	0.12%	0.017%
68	8.627	2272	2282	2314	rBV	199045	392988	55.78%	7.996%
69	9.200	2457	2460	2462	rBV	201	130	0.02%	0.003%
70	9.412	2514	2526	2551	rBV	253253	425736	60.42%	8.662%
71	9.541	2562	2566	2570	rBV3	282	273	0.04%	0.006%
72	9.701	2606	2616	2624	rBV3	865	1388	0.20%	0.028%
73	9.785	2637	2642	2643	rBV2	255	215	0.03%	0.004%
74	9.811	2648	2650	2656	rVB	271	197	0.03%	0.004%
75	10.750	2930	2942	2958	rBV	238013	389526	55.28%	7.926%
76	10.891	2976	2986	2996	rVB4	3429	5695	0.81%	0.116%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU059009.D
Acq On : 25 May 2024 19:26
Operator : MD/SY
Sample : P2596-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Title : VOC Analysis

77	10.936	2997	3000	3002	rBV	281	175	0.02%	0.004%
78	11.209	3082	3085	3088	rBV	251	163	0.02%	0.003%
79	11.627	3212	3215	3220	rVB2	377	249	0.04%	0.005%
80	11.807	3259	3271	3293	rBV	218969	357306	50.71%	7.270%
81	12.187	3377	3389	3413	rBV	241156	405275	57.52%	8.246%
82	12.605	3516	3519	3522	rBV2	273	154	0.02%	0.003%
83	12.688	3542	3545	3549	rBV2	310	288	0.04%	0.006%




Sum of corrected areas: 4914798

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU059009.D
Acq On : 25 May 2024 19:26
Operator : MD/SY
Sample : P2596-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

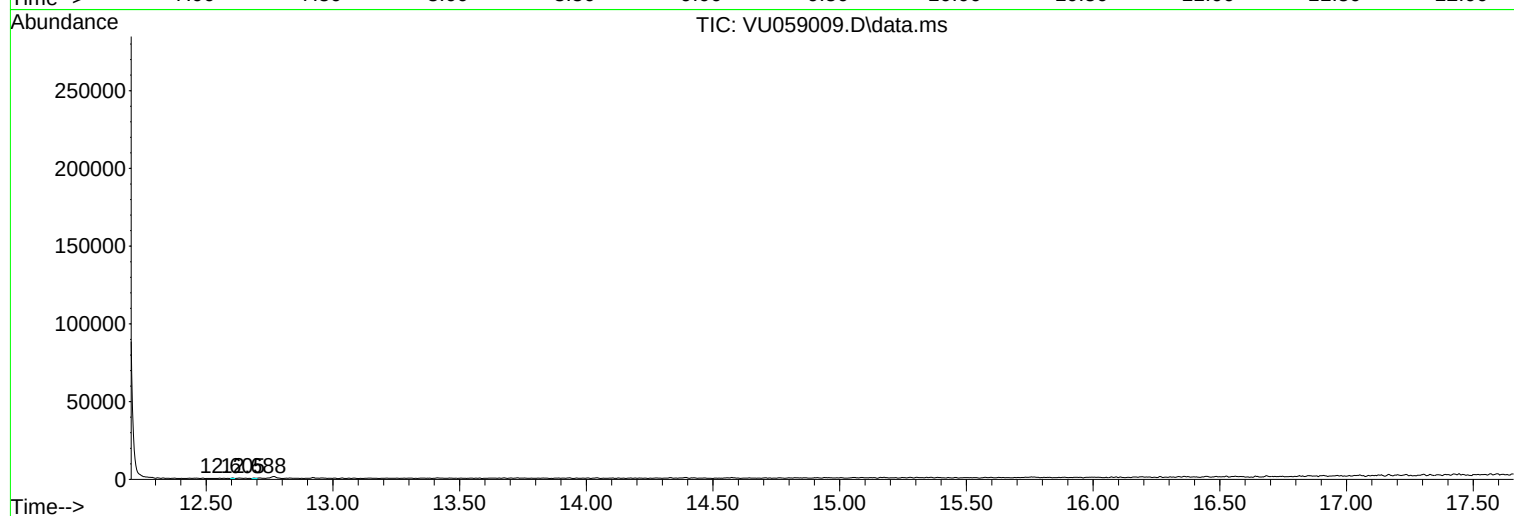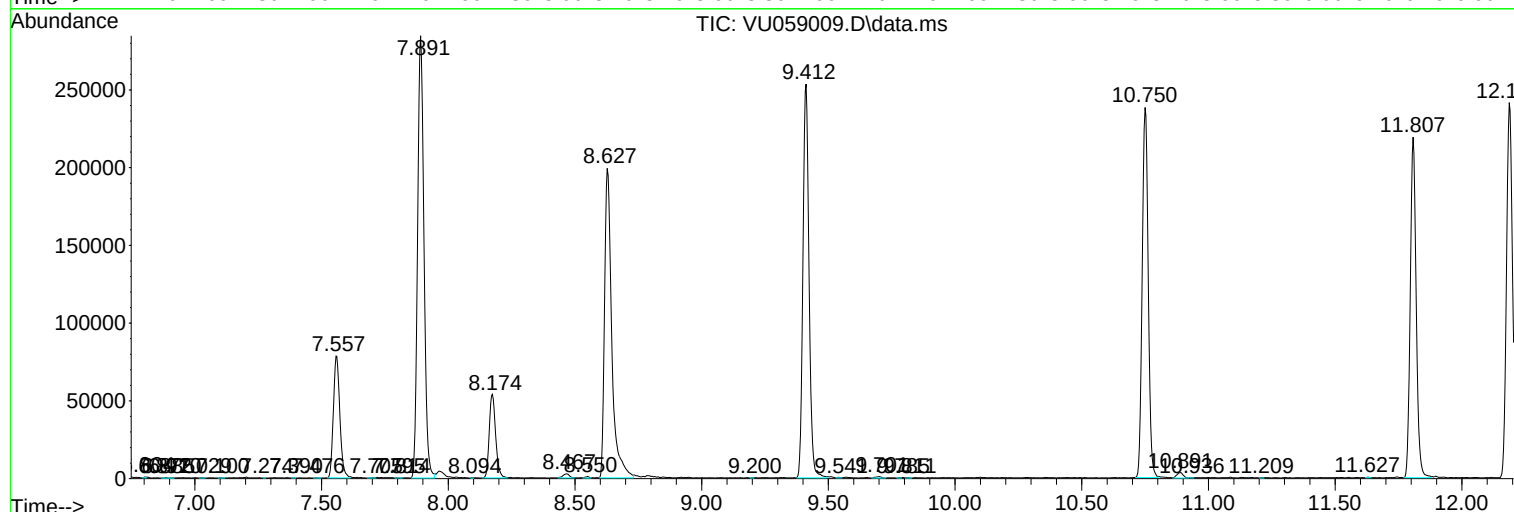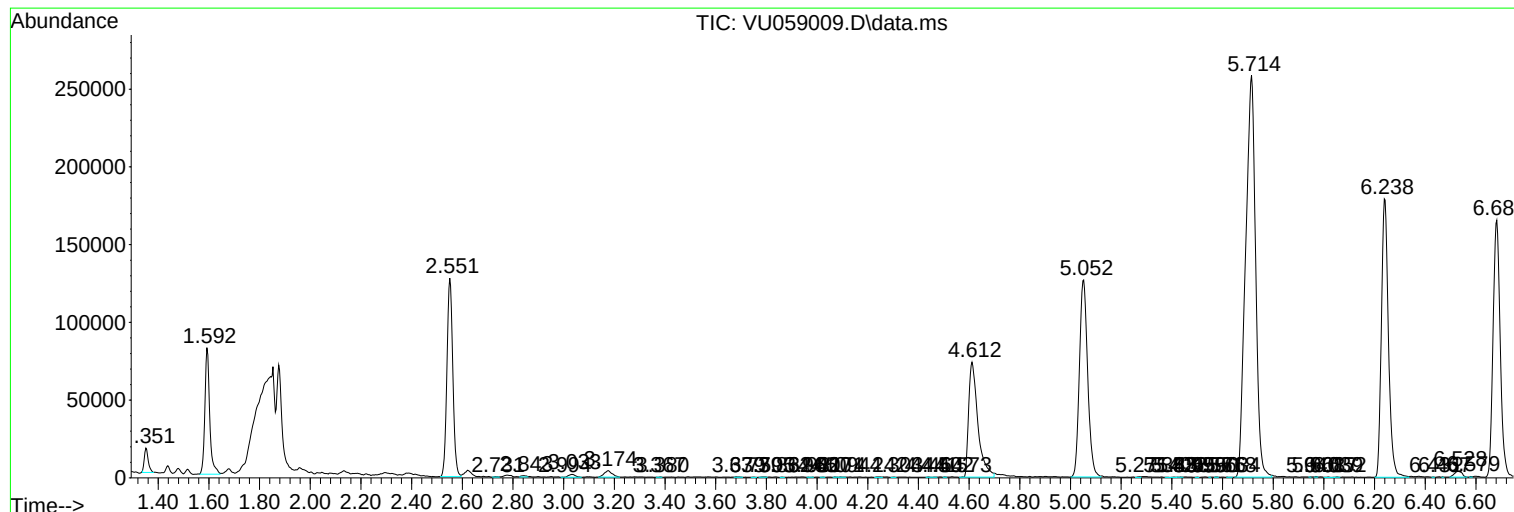

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU059009.D
Acq On : 25 May 2024 19:26
Operator : MD/SY
Sample : P2596-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU059009.D
Acq On : 25 May 2024 19:26
Operator : MD/SY
Sample : P2596-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------