

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU059014.D
 Acq On : 25 May 2024 21:29
 Operator : MD/SY
 Sample : P2566-03 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

Signal : TIC: VU059014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	87	94	111	rBV	82011	100582	5.67%	1.596%
2	1.888	179	186	201	rVB	68992	99261	5.59%	1.575%
3	2.554	381	393	407	rBV	129748	209043	11.78%	3.318%
4	2.734	448	449	450	rBV	380	85	0.00%	0.001%
5	2.866	483	490	494	rBV2	432	521	0.03%	0.008%
6	2.917	502	506	508	rBV	232	163	0.01%	0.003%
7	3.033	534	542	552	rVB	2779	4941	0.28%	0.078%
8	3.075	553	555	558	rBV2	262	113	0.01%	0.002%
9	3.088	558	559	560	rBV2	130	39	0.00%	0.001%
10	3.171	568	585	604	rBV2	8741	20707	1.17%	0.329%
11	3.345	636	639	640	rBV	120	72	0.00%	0.001%
12	3.377	646	649	652	rBV	308	204	0.01%	0.003%
13	3.419	657	662	665	rBV2	249	234	0.01%	0.004%
14	3.438	665	668	671	rVB	207	112	0.01%	0.002%
15	3.480	678	681	685	rVB2	320	286	0.02%	0.005%
16	3.509	685	690	692	rBV2	186	182	0.01%	0.003%
17	3.525	692	695	697	rVV2	237	127	0.01%	0.002%
18	3.602	716	719	723	rBV	199	168	0.01%	0.003%
19	3.663	734	738	741	rBV2	229	193	0.01%	0.003%
20	3.779	771	774	777	rBV2	173	115	0.01%	0.002%
21	3.808	782	783	786	rVB2	78	34	0.00%	0.001%
22	3.824	786	788	790	rBV	102	55	0.00%	0.001%
23	4.065	858	863	865	rBV2	200	178	0.01%	0.003%
24	4.313	937	940	943	rBV	228	184	0.01%	0.003%
25	4.374	954	959	965	rBV	232	289	0.02%	0.005%
26	4.483	990	993	997	rVB2	214	146	0.01%	0.002%
27	4.528	1004	1007	1012	rBV2	143	124	0.01%	0.002%
28	4.608	1021	1032	1068	rBV	80567	205983	11.60%	3.269%
29	4.956	1137	1140	1144	rBV2	292	227	0.01%	0.004%
30	5.052	1156	1170	1195	rVB	132447	292230	16.46%	4.638%
31	5.232	1224	1226	1230	rBV2	145	127	0.01%	0.002%
32	5.306	1244	1249	1253	rVB2	267	232	0.01%	0.004%
33	5.332	1253	1257	1262	rBV	221	243	0.01%	0.004%
34	5.396	1274	1277	1279	rBV	142	95	0.01%	0.002%
35	5.438	1288	1290	1294	rVB	165	93	0.01%	0.001%
36	5.470	1298	1300	1301	rBV	109	48	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU059014.D
 Acq On : 25 May 2024 21:29
 Operator : MD/SY
 Sample : P2566-03 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	5.502	1308	1310	1312	rBV2	53	28	0.00%	0.000%
38	5.528	1312	1318	1324	rVV	181	209	0.01%	0.003%
39	5.554	1324	1326	1330	rBV2	152	121	0.01%	0.002%
40	5.592	1335	1338	1340	rBV2	177	127	0.01%	0.002%
41	5.634	1347	1351	1354	rBV2	184	150	0.01%	0.002%
42	5.714	1355	1376	1403	rBV2	272182	744941	41.97%	11.823%
43	5.936	1441	1445	1447	rBV2	285	258	0.01%	0.004%
44	5.968	1453	1455	1458	rBV2	320	191	0.01%	0.003%
45	6.004	1461	1466	1469	rBV	280	268	0.02%	0.004%
46	6.097	1492	1495	1499	rBV2	189	177	0.01%	0.003%
47	6.242	1527	1540	1562	rBV	83600	159697	9.00%	2.535%
48	6.370	1577	1580	1582	rVB	380	211	0.01%	0.003%
49	6.386	1582	1585	1589	rBV2	254	217	0.01%	0.003%
50	6.534	1616	1631	1664	rBV	933944	1775137	100.00%	28.173%
51	6.682	1664	1677	1695	rVB	178920	350294	19.73%	5.559%
52	6.808	1714	1716	1720	rBV	638	354	0.02%	0.006%
53	6.830	1720	1723	1725	rVV3	338	191	0.01%	0.003%
54	7.033	1784	1786	1787	rBV	64	34	0.00%	0.001%
55	7.049	1788	1791	1794	rVV2	381	310	0.02%	0.005%
56	7.081	1798	1801	1803	rVV2	178	108	0.01%	0.002%
57	7.100	1804	1807	1809	rVB2	260	160	0.01%	0.003%
58	7.126	1809	1815	1818	rBV2	168	194	0.01%	0.003%
59	7.200	1832	1838	1843	rBV4	738	665	0.04%	0.011%
60	7.229	1843	1847	1852	rVB2	250	200	0.01%	0.003%
61	7.261	1852	1857	1860	rBB3	234	186	0.01%	0.003%
62	7.287	1860	1865	1868	rVB2	274	159	0.01%	0.003%
63	7.306	1868	1871	1873	rBV2	133	88	0.00%	0.001%
64	7.489	1925	1928	1931	rVB3	171	110	0.01%	0.002%
65	7.512	1932	1935	1937	rVB	228	112	0.01%	0.002%
66	7.560	1937	1950	1968	rBV	83453	149177	8.40%	2.368%
67	7.647	1974	1977	1981	rBV3	307	283	0.02%	0.004%
68	7.669	1981	1984	1987	rVB2	272	199	0.01%	0.003%
69	7.689	1987	1990	1992	rBV2	287	179	0.01%	0.003%
70	7.750	2006	2009	2011	rBV	195	152	0.01%	0.002%
71	7.788	2018	2021	2025	rVB	452	293	0.02%	0.005%
72	7.814	2025	2029	2030	rBV3	292	187	0.01%	0.003%
73	7.891	2041	2053	2075	rBV	294380	519230	29.25%	8.241%
74	8.174	2131	2141	2164	rVB	57613	96743	5.45%	1.535%
75	8.280	2171	2174	2178	rVB2	267	166	0.01%	0.003%
76	8.402	2209	2212	2215	rBV2	193	111	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU059014.D
 Acq On : 25 May 2024 21:29
 Operator : MD/SY
 Sample : P2566-03 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M

Title : VOC Analysis

77	8.431	2218	2221	2222	rBV	139	72	0.00%	0.001%
78	8.550	2252	2258	2267	rVB4	1110	1458	0.08%	0.023%
79	8.628	2271	2282	2316	rBV	206405	398175	22.43%	6.319%
80	8.984	2391	2393	2396	rVB	144	42	0.00%	0.001%
81	9.184	2452	2455	2457	rBV2	238	166	0.01%	0.003%
82	9.367	2508	2512	2514	rBV2	137	116	0.01%	0.002%
83	9.412	2514	2526	2553	rVV2	119714	203579	11.47%	3.231%
84	9.605	2582	2586	2588	rBV	302	228	0.01%	0.004%
85	9.724	2621	2623	2626	rBV2	272	164	0.01%	0.003%
86	10.174	2760	2763	2765	rBV	162	100	0.01%	0.002%
87	10.602	2892	2896	2899	rBV	226	190	0.01%	0.003%
88	10.750	2929	2942	2964	rBV	240416	385666	21.73%	6.121%
89	11.193	3077	3080	3082	rBV2	169	135	0.01%	0.002%
90	11.367	3130	3134	3136	rBV2	401	286	0.02%	0.005%
91	11.807	3260	3271	3292	rBV	97197	161590	9.10%	2.565%
92	12.084	3354	3357	3360	rBV2	222	148	0.01%	0.002%
93	12.187	3377	3389	3410	rBV	239151	409101	23.05%	6.493%
94	12.312	3425	3428	3431	rBV3	643	410	0.02%	0.007%
95	12.492	3482	3484	3489	rBV2	287	232	0.01%	0.004%




Sum of corrected areas: 6300911

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU059014.D
Acq On : 25 May 2024 21:29
Operator : MD/SY
Sample : P2566-03 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

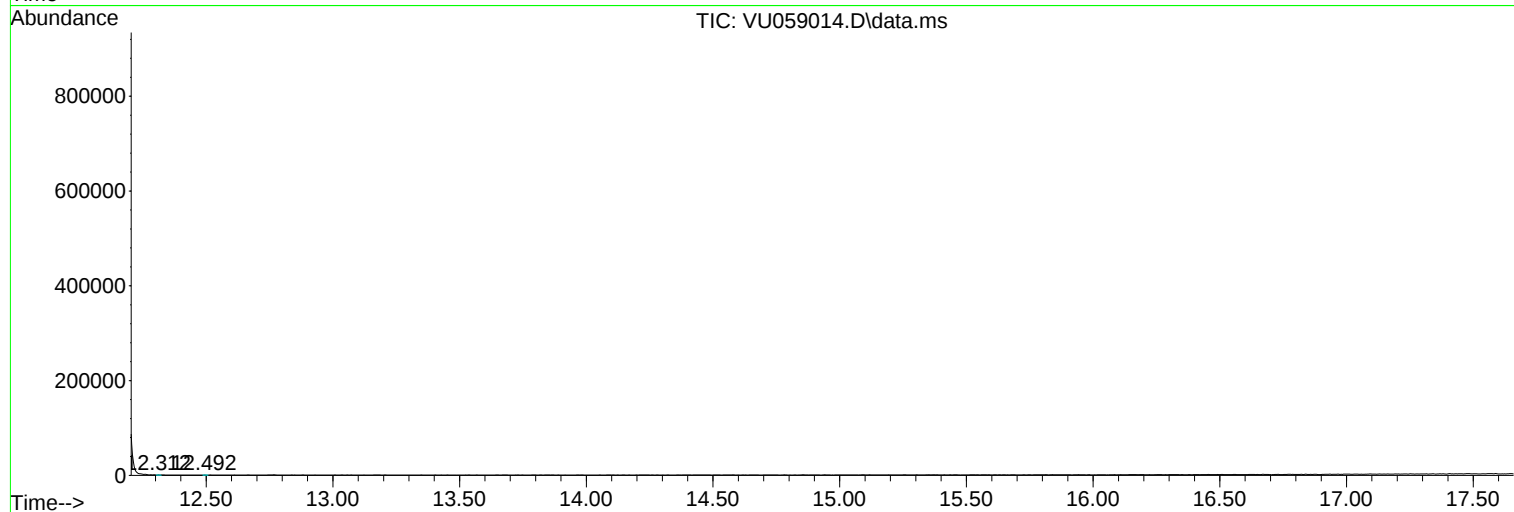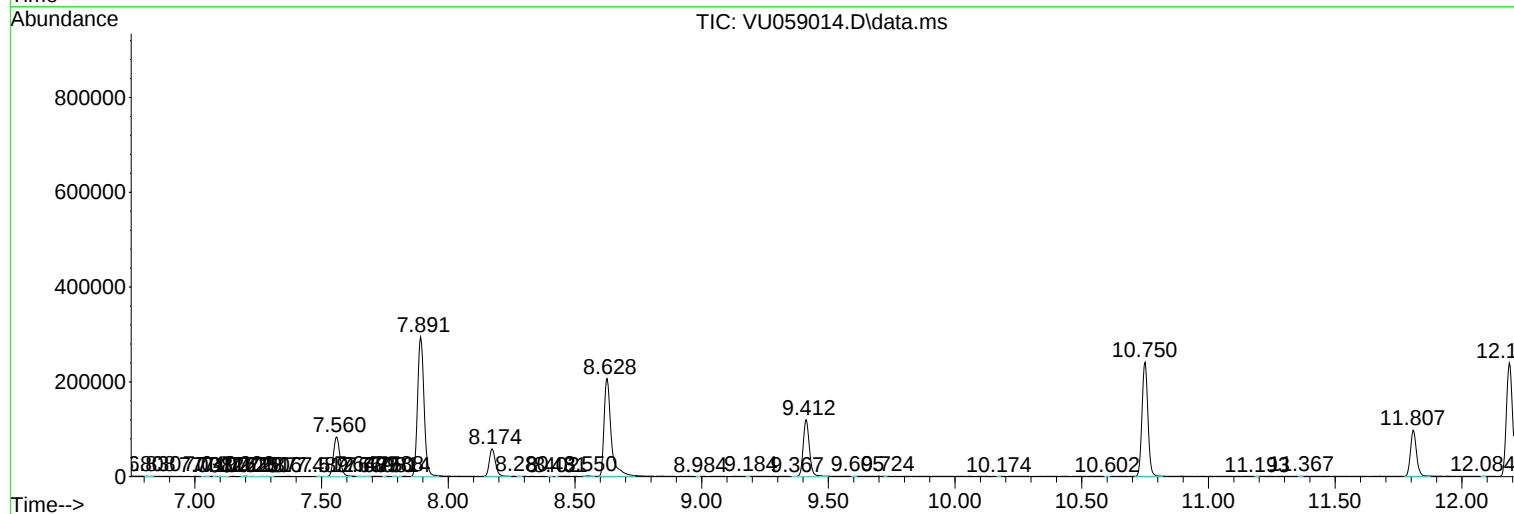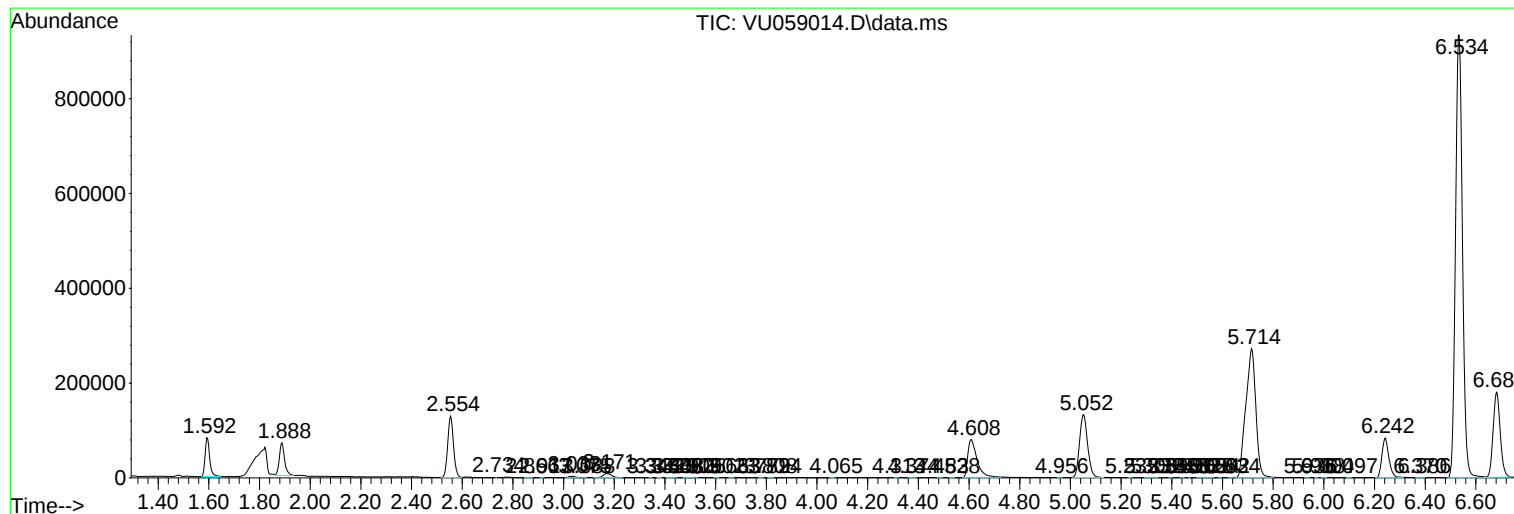

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU059014.D
Acq On : 25 May 2024 21:29
Operator : MD/SY
Sample : P2566-03 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU059014.D
Acq On : 25 May 2024 21:29
Operator : MD/SY
Sample : P2566-03 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------