


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU058988.D
Acq On : 25 May 2024 10:19
Operator : MD/SY
Sample : BFB053
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB053

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Title : VOC Analysis
Last Update : Wed May 29 02:38:59 2024

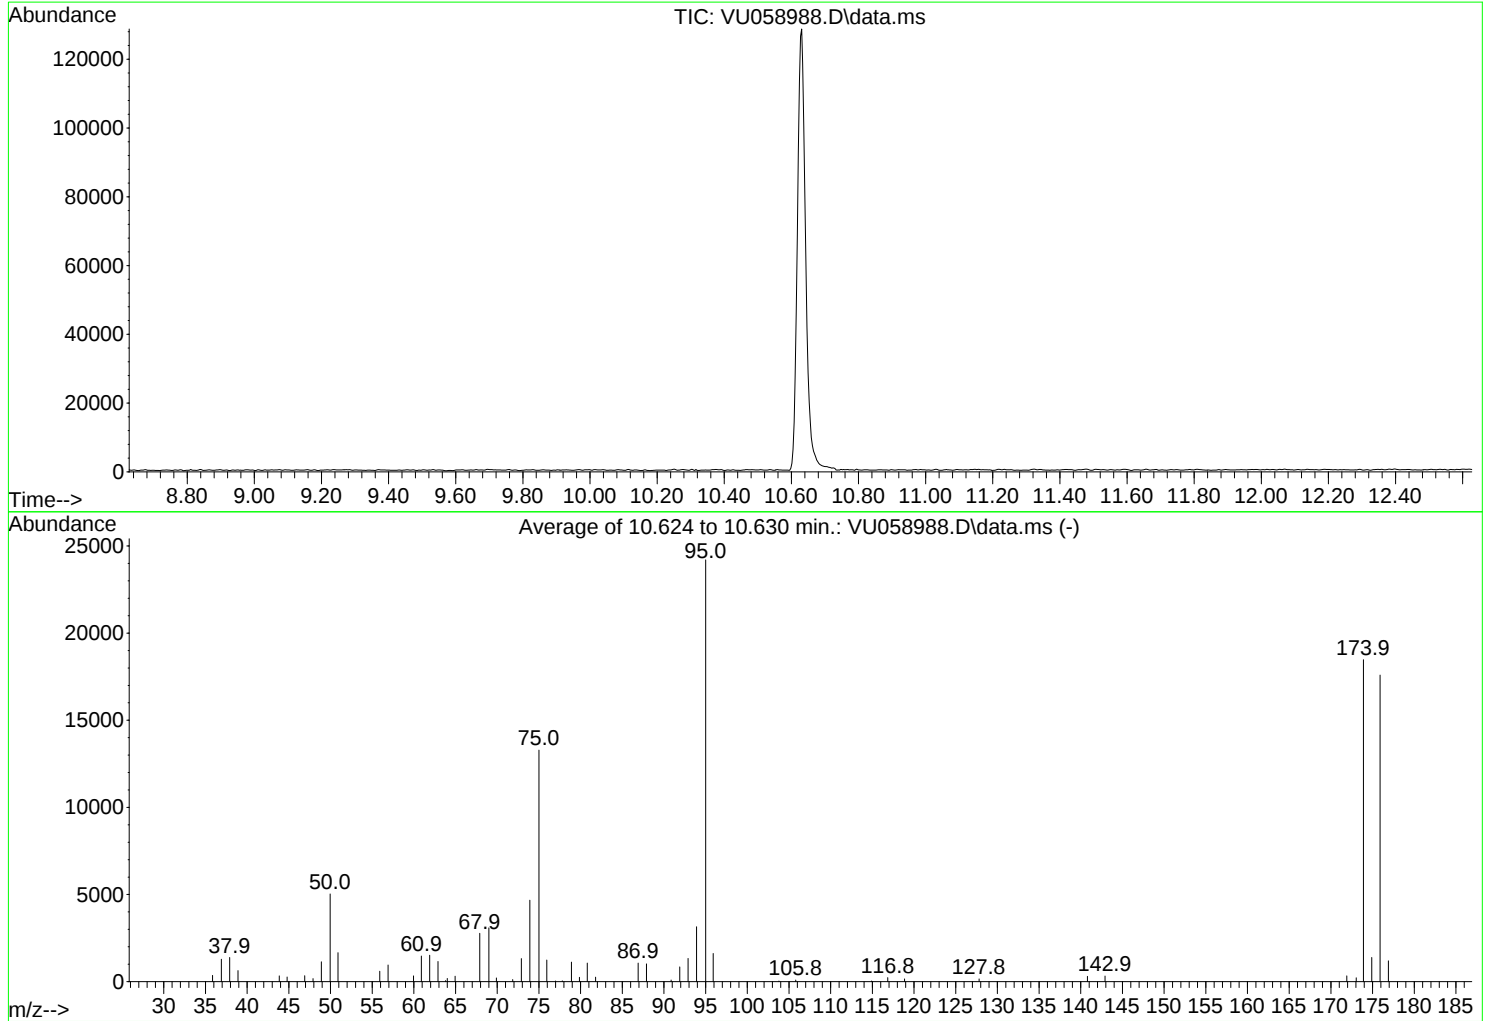

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2893

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	5034	PASS
75	95	30	80	54.9	13286	PASS
95	95	100	100	100.0	24205	PASS
96	95	5	9	6.7	1619	PASS
173	174	0.00	2	1.2	225	PASS
174	95	50	120	76.3	18477	PASS
175	174	5	9	7.5	1383	PASS
176	174	95	101	95.2	17596	PASS
177	176	5	9	6.8	1190	PASS

m/z	Abundance
39.80	257.0
43.80	217.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053

m/z	Abundance
35.80	313.0
36.90	1226.0
37.90	1273.0
38.90	611.0
39.70	207.0
43.90	516.0
44.80	260.0
46.90	310.0
47.90	169.0
48.90	1080.0
49.90	4686.0
50.90	1493.0
55.90	564.0
56.90	970.0
60.00	313.0
60.90	1275.0
61.90	1421.0
62.90	1099.0
63.80	168.0
64.90	376.0
67.90	2562.0
69.00	2966.0
70.00	200.0
71.90	113.0
72.90	1192.0
73.90	4285.0
75.00	12246.0
76.00	1115.0
78.90	1036.0
79.90	241.0
80.80	955.0
81.80	254.0
86.90	1002.0
87.90	903.0
91.90	793.0
92.90	1193.0
93.90	2963.0
95.00	22848.0
95.90	1636.0
116.80	197.0
118.80	190.0
127.80	125.0
140.80	259.0
142.90	315.0
171.90	233.0
173.00	291.0
173.90	16856.0
174.90	1262.0
175.90	15845.0
176.90	1056.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053

m/z	Abundance
35.90	373.0
36.90	1299.0
37.90	1437.0
38.90	661.0
39.70	221.0
43.90	547.0
44.80	278.0
46.90	359.0
47.90	188.0
48.90	1172.0
50.00	5171.0
50.90	1672.0
55.90	627.0
56.90	998.0
60.00	351.0
60.90	1514.0
61.90	1588.0
62.90	1158.0
64.00	236.0
64.90	299.0
67.90	2868.0
69.00	3220.0
69.90	209.0
71.80	113.0
72.90	1353.0
73.90	4748.0
75.00	13735.0
75.90	1285.0
78.90	1133.0
79.90	254.0
80.80	1104.0
81.80	263.0
86.90	1052.0
87.90	1054.0
90.80	128.0
91.90	860.0
92.90	1418.0
93.90	3272.0
95.00	24912.0
95.90	1681.0
105.80	124.0
114.90	102.0
116.90	235.0
118.90	164.0
127.80	163.0
140.80	322.0
142.90	339.0
171.90	337.0
173.90	19240.0
174.90	1385.0
175.90	18216.0
176.90	1217.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053

m/z	Abundance
35.90	382.0
36.90	1339.0
37.90	1450.0
38.90	619.0
39.80	199.0
43.90	572.0
44.80	266.0
46.90	361.0
47.90	176.0
48.90	1167.0
49.90	5246.0
50.90	1833.0
55.90	604.0
56.90	892.0
59.90	329.0
60.90	1608.0
61.90	1546.0
62.90	1202.0
64.00	314.0
65.00	256.0
67.90	2877.0
69.00	3062.0
69.80	214.0
71.80	122.0
72.90	1427.0
73.90	5002.0
75.00	13877.0
75.90	1327.0
77.00	119.0
77.80	128.0
78.90	1205.0
79.80	241.0
80.80	1147.0
81.80	245.0
86.90	1134.0
87.90	1089.0
90.90	160.0
91.90	883.0
92.90	1390.0
93.90	3206.0
95.00	24856.0
95.90	1539.0
103.80	116.0
105.80	155.0
116.90	271.0
118.80	125.0
127.80	171.0
140.80	320.0
142.90	312.0
171.90	429.0
173.10	384.0
173.90	19336.0
174.90	1501.0
175.90	18728.0
176.90	1298.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053