

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053124\
 Data File : VU059110.D
 Acq On : 31 May 2024 13:25
 Operator : MD/SY
 Sample : P2647-06ME
 Misc : 6.78g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jun 01 01:19:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 01 01:17:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	486905	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	490806	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	222932	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	143185	49.115	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	98.220%	
7) Chloroethane-d5	1.875	69	131904	52.819	ug/L	-0.03
Spiked Amount	50.000	Range 70 - 130	Recovery	=	105.640%	
11) 1,1-Dichloroethene-d2	2.544	63	196965	34.228	ug/L	-0.02
Spiked Amount	50.000	Range 60 - 125	Recovery	=	68.460%	
21) 2-Butanone-d5	4.615	46	283359	103.120	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	103.120%	
24) Chloroform-d	5.049	84	296408	51.073	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	102.140%	
26) 1,2-Dichloroethane-d4	5.689	65	197628	55.559	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	111.120%	
32) Benzene-d6	5.714	84	614918	54.588	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	109.180%	
36) 1,2-Dichloropropane-d6	6.679	67	209197	53.860	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	107.720%	
41) Toluene-d8	7.891	98	527815	55.195	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	110.380%	
43) trans-1,3-Dichloroprop...	8.174	79	88995	56.685	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	113.360%	
47) 2-Hexanone-d5	8.634	63	189761	105.652	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	105.650%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	329181	50.077	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	100.160%	
66) 1,2-Dichlorobenzene-d4	12.187	152	194712	58.527	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	117.060%	
Target Compounds						
60) 1,2,3-Trichloropropane	11.807	75	31310	5.050	ug/L	Qvalue # 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053124\
Data File : VU059110.D
Acq On : 31 May 2024 13:25
Operator : MD/SY
Sample : P2647-06ME
Misc : 6.78g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Jun 01 01:19:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 01 01:17:21 2024
Response via : Initial Calibration

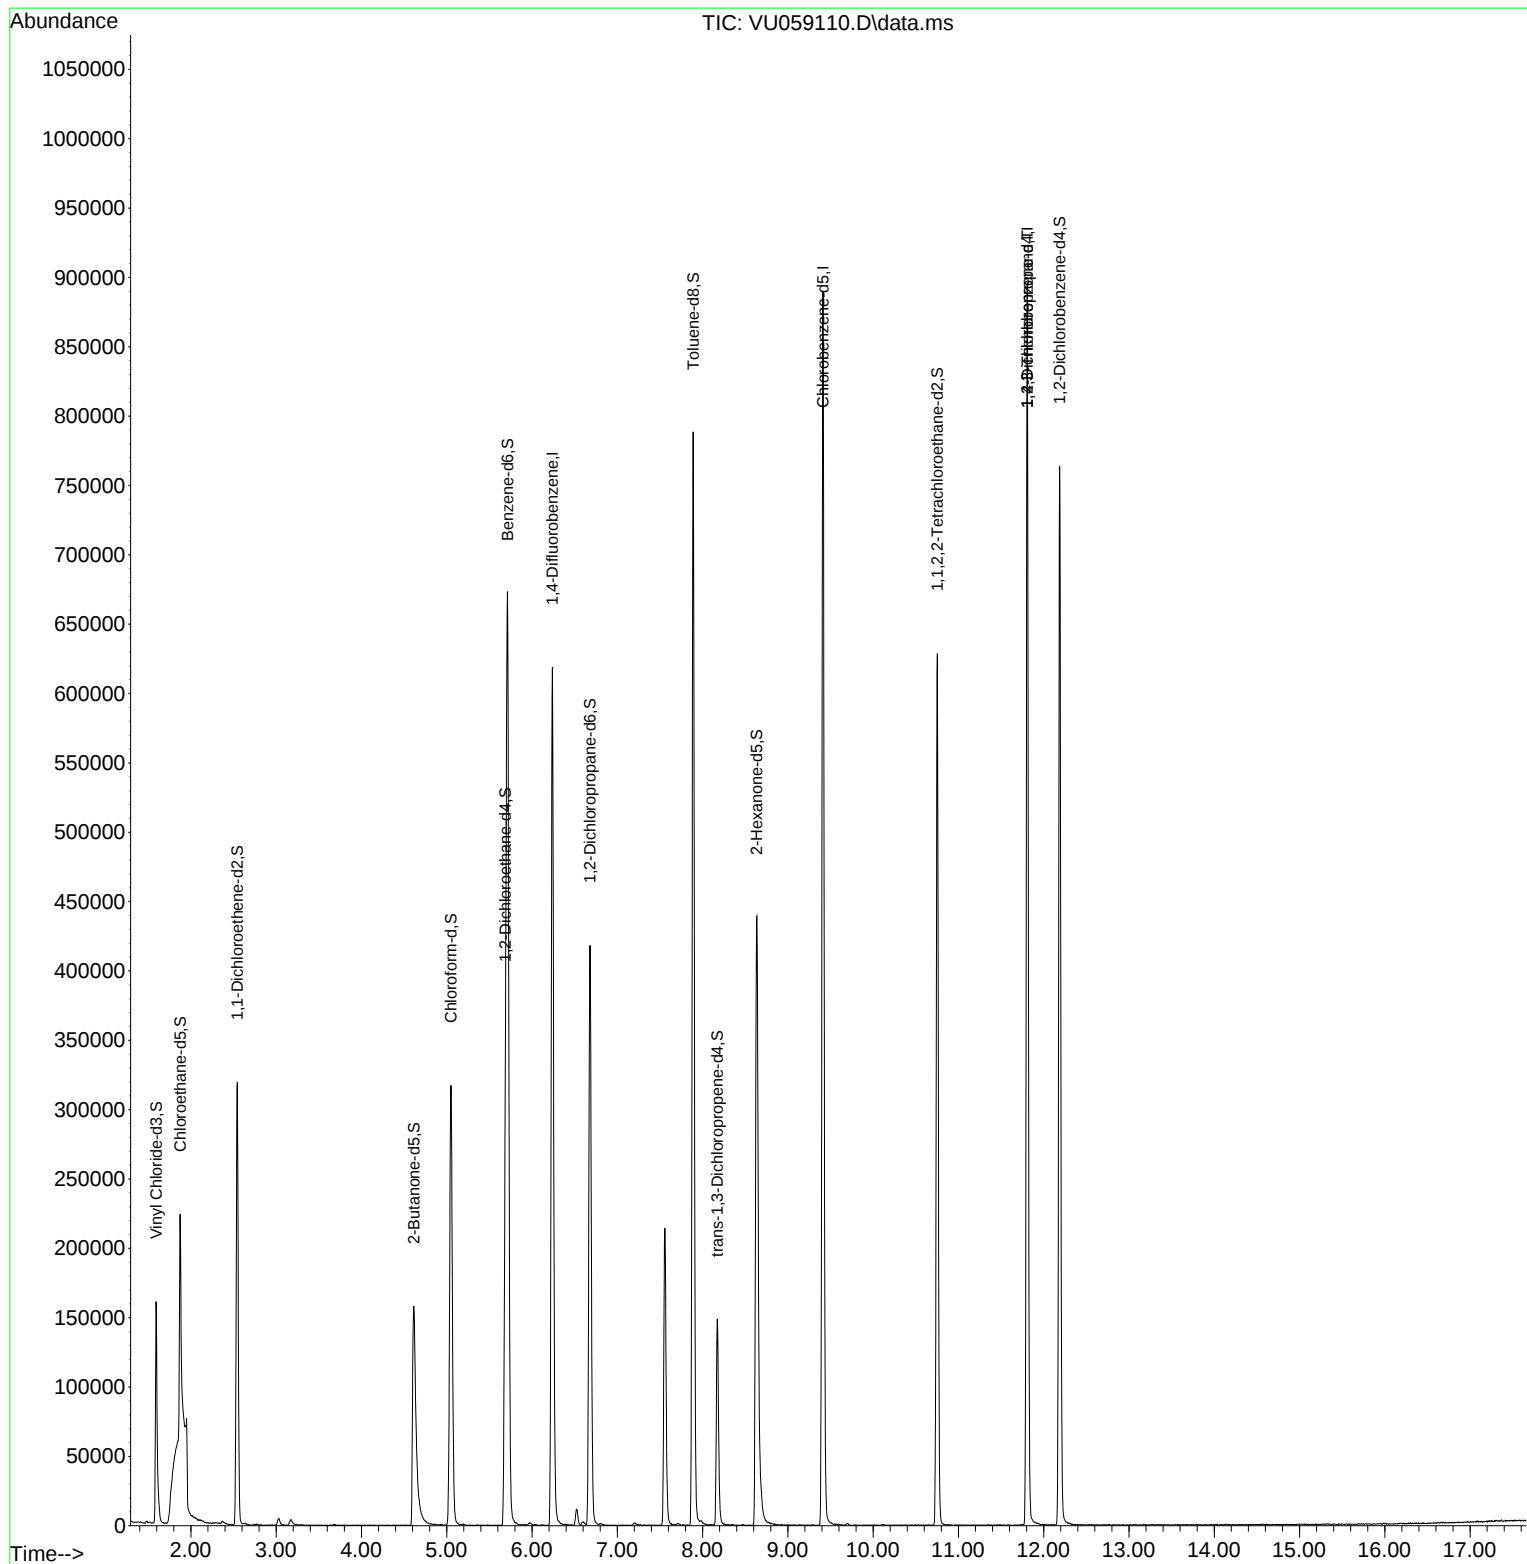

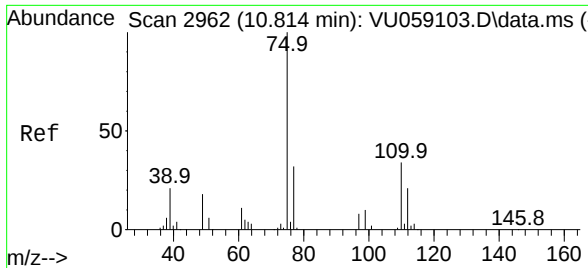

#60
 1,2,3-Trichloropropane
 Concen: 5.050 ug/L
 RT: 11.807 min Scan# 31
 Delta R.T. 0.994 min
 Lab File: VU059110.D
 Acq: 31 May 2024 13:25

Instrument :
 MSVOA_U
 ClientSampleId :

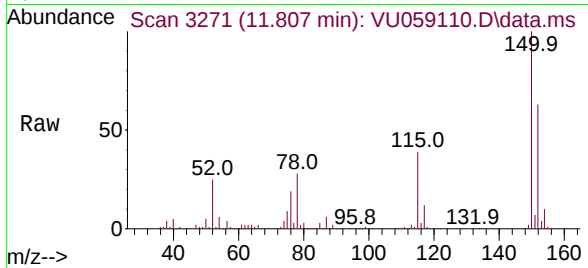

Tgt Ion: 75	Resp:	31310
Ion Ratio	Lower	Upper
75	100	
77	31.0	26.2 39.2
110	2.5	28.4 42.6#

