

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053124\
 Data File : VU059105.D
 Acq On : 31 May 2024 10:19
 Operator : MD/SY
 Sample : VU0531WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059105.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	114	rVB	72068	89184	13.44%	1.651%
2	1.908	184	192	212	rVB	66910	88674	13.36%	1.642%
3	2.490	369	373	376	rBV2	465	325	0.05%	0.006%
4	2.560	384	395	414	rBV	117056	196321	29.58%	3.634%
5	2.702	436	439	443	rVB2	299	212	0.03%	0.004%
6	2.792	458	467	476	rVB2	2249	4120	0.62%	0.076%
7	3.036	533	543	553	rBV2	2667	5055	0.76%	0.094%
8	3.152	574	579	584	rBV2	227	292	0.04%	0.005%
9	3.354	638	642	645	rVV	258	246	0.04%	0.005%
10	3.509	686	690	693	rBV2	191	184	0.03%	0.003%
11	3.528	693	696	699	rBV2	234	177	0.03%	0.003%
12	3.637	724	730	734	rBV2	272	365	0.05%	0.007%
13	3.695	744	748	751	rBV	208	183	0.03%	0.003%
14	3.972	828	834	838	rBV2	240	307	0.05%	0.006%
15	4.075	863	866	872	rVV	303	317	0.05%	0.006%
16	4.136	879	885	887	rBV	238	236	0.04%	0.004%
17	4.274	923	928	933	rBV	268	311	0.05%	0.006%
18	4.544	1009	1012	1015	rBV2	287	272	0.04%	0.005%
19	4.615	1023	1034	1065	rBV2	73231	197216	29.71%	3.651%
20	4.801	1089	1092	1095	rBV2	577	390	0.06%	0.007%
21	4.862	1108	1111	1118	rVB2	499	526	0.08%	0.010%
22	4.969	1141	1144	1146	rBV	289	205	0.03%	0.004%
23	5.055	1155	1171	1191	rBV	123914	276792	41.70%	5.124%
24	5.313	1246	1251	1253	rBV2	250	189	0.03%	0.003%
25	5.341	1256	1260	1262	rBV	239	186	0.03%	0.003%
26	5.425	1281	1286	1291	rBV	285	389	0.06%	0.007%
27	5.554	1319	1326	1328	rVB	279	310	0.05%	0.006%
28	5.718	1357	1377	1398	rBV2	243714	663737	100.00%	12.287%
29	5.927	1438	1442	1445	rBV2	453	339	0.05%	0.006%
30	5.943	1445	1447	1450	rVV	246	189	0.03%	0.003%
31	5.972	1450	1456	1460	rVV2	425	514	0.08%	0.010%
32	6.242	1527	1540	1570	rBV	250918	488345	73.58%	9.040%
33	6.525	1620	1628	1639	rBV6	4319	8604	1.30%	0.159%
34	6.682	1663	1677	1704	rBV	159577	314995	47.46%	5.831%
35	6.843	1724	1727	1730	rBV2	283	198	0.03%	0.004%
36	6.862	1730	1733	1738	rBV	346	287	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053124\
 Data File : VU059105.D
 Acq On : 31 May 2024 10:19
 Operator : MD/SY
 Sample : VU0531WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.911	1746	1748	1753	rVB2	330	207	0.03%	0.004%
38	6.936	1753	1756	1758	rBV	281	212	0.03%	0.004%
39	7.203	1835	1839	1845	rBV2	380	444	0.07%	0.008%
40	7.560	1939	1950	1973	rBV	78902	141094	21.26%	2.612%
41	7.714	1994	1998	2003	rVB3	215	192	0.03%	0.004%
42	7.804	2024	2026	2030	rVB	346	241	0.04%	0.004%
43	7.824	2030	2032	2034	rBV	363	239	0.04%	0.004%
44	7.891	2041	2053	2075	rBV	263561	462897	69.74%	8.569%
45	8.100	2116	2118	2123	rVB3	285	209	0.03%	0.004%
46	8.174	2129	2141	2165	rBV	52780	94977	14.31%	1.758%
47	8.357	2193	2198	2200	rBV	321	308	0.05%	0.006%
48	8.457	2227	2229	2236	rBV2	192	206	0.03%	0.004%
49	8.628	2269	2282	2333	rBV2	184016	384132	57.87%	7.111%
50	8.891	2362	2364	2367	rBV2	274	187	0.03%	0.003%
51	8.939	2375	2379	2382	rBV	226	192	0.03%	0.004%
52	9.026	2400	2406	2414	rBV2	334	570	0.09%	0.011%
53	9.071	2414	2420	2424	rBV2	308	427	0.06%	0.008%
54	9.165	2446	2449	2452	rBV	282	233	0.04%	0.004%
55	9.332	2498	2501	2503	rBV2	300	193	0.03%	0.004%
56	9.412	2514	2526	2550	rBV	359735	619262	93.30%	11.464%
57	9.563	2570	2573	2575	rBV	364	233	0.04%	0.004%
58	9.698	2610	2615	2618	rBV3	494	486	0.07%	0.009%
59	9.753	2628	2632	2633	rBV	251	178	0.03%	0.003%
60	9.840	2656	2659	2664	rBV2	308	258	0.04%	0.005%
61	9.869	2664	2668	2674	rBV2	300	405	0.06%	0.007%
62	9.894	2674	2676	2679	rVB	314	194	0.03%	0.004%
63	9.933	2682	2688	2689	rBV	228	253	0.04%	0.005%
64	9.975	2698	2701	2705	rVB	315	225	0.03%	0.004%
65	10.007	2706	2711	2717	rBV2	233	340	0.05%	0.006%
66	10.091	2733	2737	2740	rBV2	205	223	0.03%	0.004%
67	10.107	2740	2742	2746	rVB2	300	182	0.03%	0.003%
68	10.399	2828	2833	2839	rVB2	308	441	0.07%	0.008%
69	10.428	2839	2842	2843	rBV2	289	194	0.03%	0.004%
70	10.602	2893	2896	2903	rVB2	211	221	0.03%	0.004%
71	10.647	2903	2910	2913	rBV2	1183	1661	0.25%	0.031%
72	10.750	2930	2942	2962	rBV	241667	396993	59.81%	7.349%
73	11.062	3037	3039	3042	rVB2	322	182	0.03%	0.003%
74	11.084	3042	3046	3048	rBV2	309	277	0.04%	0.005%
75	11.206	3080	3084	3088	rBV2	221	228	0.03%	0.004%
76	11.287	3105	3109	3112	rBV2	172	180	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053124\
 Data File : VU059105.D
 Acq On : 31 May 2024 10:19
 Operator : MD/SY
 Sample : VU0531WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.361	3129	3132	3136	rBV	290	232	0.03%	0.004%
78	11.463	3155	3164	3167	rBV2	391	594	0.09%	0.011%
79	11.553	3185	3192	3197	rBV2	365	551	0.08%	0.010%
80	11.750	3249	3253	3257	rVB2	838	746	0.11%	0.014%
81	11.807	3257	3271	3296	rBV	308421	522262	78.69%	9.668%
82	12.187	3377	3389	3415	rBV	247357	418243	63.01%	7.742%
83	12.946	3621	3625	3627	rBV	262	221	0.03%	0.004%
84	13.016	3644	3647	3655	rBV	306	294	0.04%	0.005%
85	13.332	3740	3745	3747	rBV2	296	335	0.05%	0.006%
86	13.476	3786	3790	3795	rVV2	410	385	0.06%	0.007%
87	13.852	3902	3907	3916	rVB3	1153	1451	0.22%	0.027%
88	14.100	3979	3984	3985	rBV3	1764	1282	0.19%	0.024%
89	14.168	4001	4005	4007	rBV	448	384	0.06%	0.007%
90	14.331	4054	4056	4065	rVB5	1244	1415	0.21%	0.026%
91	14.418	4079	4083	4086	rBV2	254	222	0.03%	0.004%
92	14.563	4125	4128	4131	rBV	403	350	0.05%	0.006%
93	14.814	4202	4206	4212	rBV3	300	365	0.05%	0.007%
94	14.881	4225	4227	4230	rBV2	343	212	0.03%	0.004%
95	15.116	4297	4300	4302	rBV	242	202	0.03%	0.004%
96	15.155	4306	4312	4318	rBV3	419	631	0.10%	0.012%
97	15.467	4407	4409	4412	rBV	354	232	0.03%	0.004%
98	15.836	4521	4524	4527	rBV2	582	435	0.07%	0.008%
99	16.431	4707	4709	4712	rBV2	575	430	0.06%	0.008%
100	16.682	4784	4787	4788	rBV2	775	504	0.08%	0.009%




Sum of corrected areas: 5401946

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053124\
Data File : VU059105.D
Acq On : 31 May 2024 10:19
Operator : MD/SY
Sample : VU0531WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK062

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

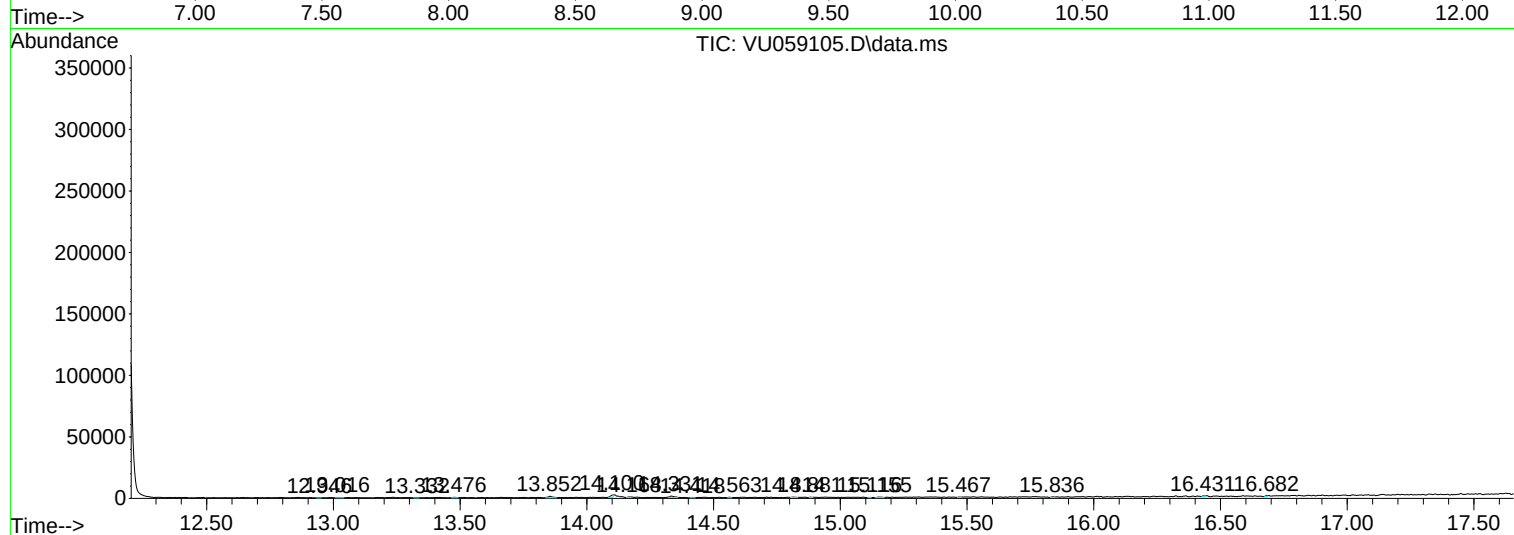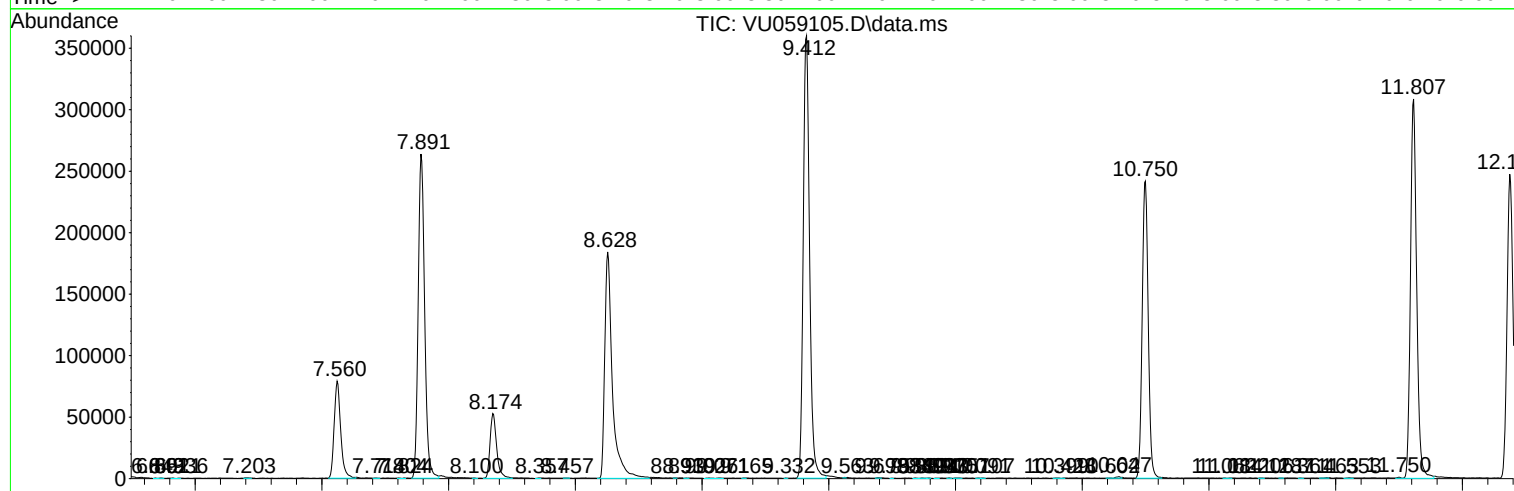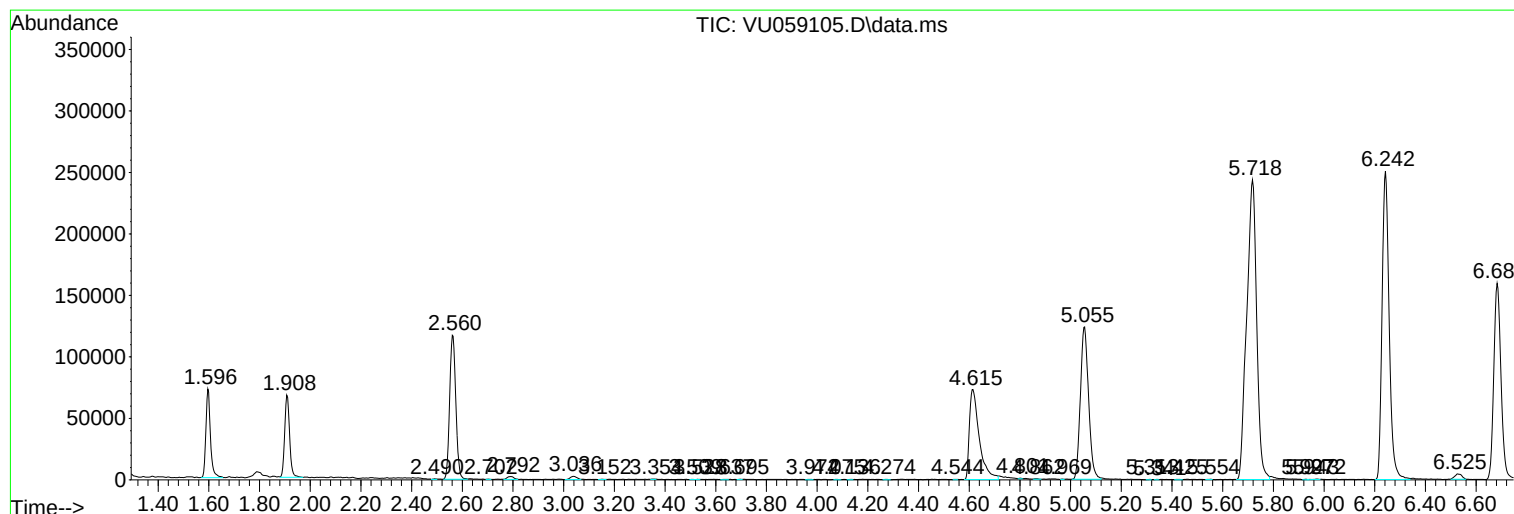

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053124\
Data File : VU059105.D
Acq On : 31 May 2024 10:19
Operator : MD/SY
Sample : VU0531WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK062

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053124\
Data File : VU059105.D
Acq On : 31 May 2024 10:19
Operator : MD/SY
Sample : VU0531WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK062

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------