
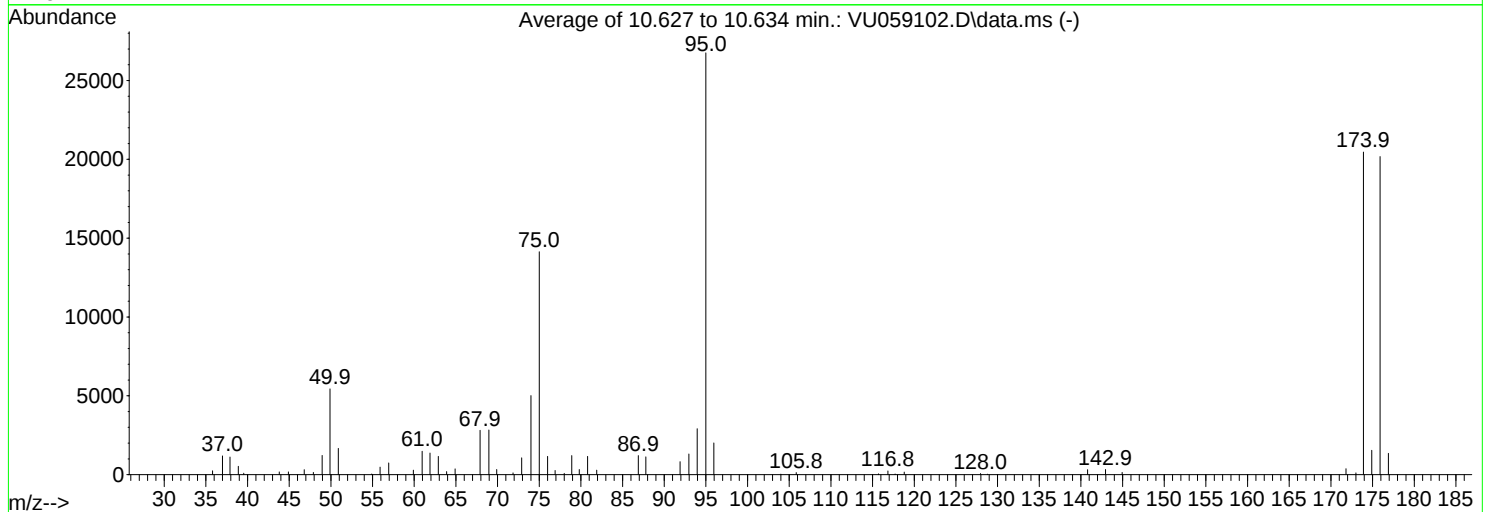


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU053124\
Data File : VU059102.D
Acq On : 31 May 2024 07:56
Operator : MD/SY
Sample : BFB057
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB057

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Title : VOC Analysis
Last Update : Sat Jun 01 01:17:21 2024

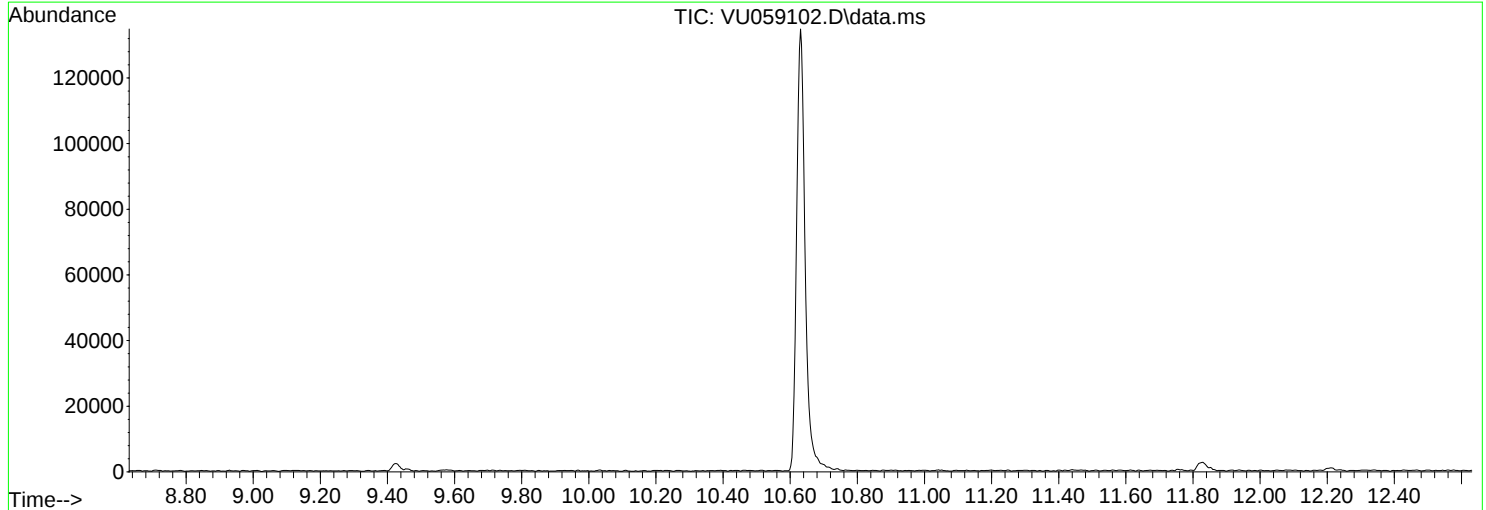

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2893

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	5443	PASS
75	95	30	80	52.8	14140	PASS
95	95	100	100	100.0	26755	PASS
96	95	5	9	7.5	2005	PASS
173	174	0.00	2	0.5	107	PASS
174	95	50	120	76.5	20464	PASS
175	174	5	9	7.5	1545	PASS
176	174	95	101	98.6	20179	PASS
177	176	5	9	6.7	1347	PASS

m/z	Abundance
39.80	105.0
43.80	257.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057

m/z	Abundance
35.80	286.0
37.00	1154.0
37.90	1124.0
38.90	467.0
43.90	431.0
44.90	203.0
46.80	273.0
48.00	143.0
48.90	1134.0
49.90	5284.0
50.90	1642.0
55.90	515.0
56.90	769.0
59.90	275.0
60.90	1517.0
61.90	1498.0
62.90	1233.0
63.90	190.0
64.90	342.0
67.90	2815.0
69.00	2729.0
69.90	345.0
71.80	115.0
72.90	1021.0
74.00	4966.0
75.00	13980.0
76.00	1127.0
76.90	206.0
78.90	1213.0
79.80	297.0
80.80	1038.0
81.90	244.0
86.90	1219.0
87.80	1098.0
91.90	806.0
92.90	1201.0
94.00	3164.0
95.00	26544.0
96.00	1944.0
105.80	137.0
116.80	187.0
118.80	170.0
128.00	107.0
128.80	102.0
140.80	288.0
142.90	371.0
144.90	100.0
171.80	315.0
173.90	20008.0
174.90	1547.0
175.90	19272.0
176.90	1359.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057

m/z	Abundance
35.80	258.0
37.00	1221.0
37.90	1155.0
38.90	540.0
39.50	149.0
43.80	456.0
45.00	181.0
46.80	322.0
47.90	159.0
49.00	1272.0
49.90	5649.0
50.90	1696.0
54.90	115.0
55.90	492.0
56.90	742.0
59.90	315.0
61.00	1553.0
61.90	1410.0
62.90	1182.0
63.90	206.0
64.90	362.0
67.90	2860.0
68.90	2891.0
69.90	337.0
71.90	109.0
72.90	1080.0
74.00	5193.0
75.00	14519.0
76.00	1213.0
76.90	280.0
78.00	118.0
78.90	1280.0
79.80	325.0
80.80	1177.0
81.90	302.0
86.90	1212.0
87.80	1190.0
91.90	828.0
93.00	1363.0
93.90	2944.0
95.00	27488.0
95.90	1997.0
105.80	132.0
116.90	242.0
118.80	156.0
127.90	120.0
140.80	331.0
143.00	318.0
145.00	147.0
171.80	391.0
173.90	20952.0
174.90	1626.0
175.90	20944.0
176.90	1385.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057

m/z	Abundance
35.80	179.0
37.00	1177.0
37.90	1075.0
38.90	577.0
39.60	132.0
43.80	403.0
44.80	147.0
46.80	335.0
47.80	138.0
48.90	1249.0
49.90	5397.0
50.90	1643.0
55.90	423.0
57.00	705.0
59.90	275.0
61.00	1387.0
61.90	1194.0
62.90	1063.0
63.90	183.0
64.90	383.0
67.90	2747.0
68.90	2887.0
69.90	289.0
71.90	121.0
72.90	1094.0
74.00	4878.0
75.00	13921.0
76.00	1127.0
76.90	301.0
78.00	125.0
78.90	1134.0
79.80	346.0
80.80	1256.0
81.90	322.0
86.90	1181.0
87.80	1103.0
91.90	820.0
92.90	1379.0
93.90	2643.0
95.00	26232.0
96.00	2074.0
104.00	100.0
105.90	114.0
115.70	144.0
116.90	262.0
117.70	114.0
118.80	167.0
140.80	330.0
142.90	298.0
145.00	171.0
171.80	418.0
173.00	320.0
173.90	20432.0
174.90	1463.0
175.90	20320.0
176.90	1296.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057