


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060220\
Data File : VU038501.D
Acq On : 02 Jun 2020 18:14
Operator : JC/MD
Sample : L2856-07
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1




Quant Time: Jun 03 02:26:29 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 03 00:48:29 2020
Response via : Initial Calibration

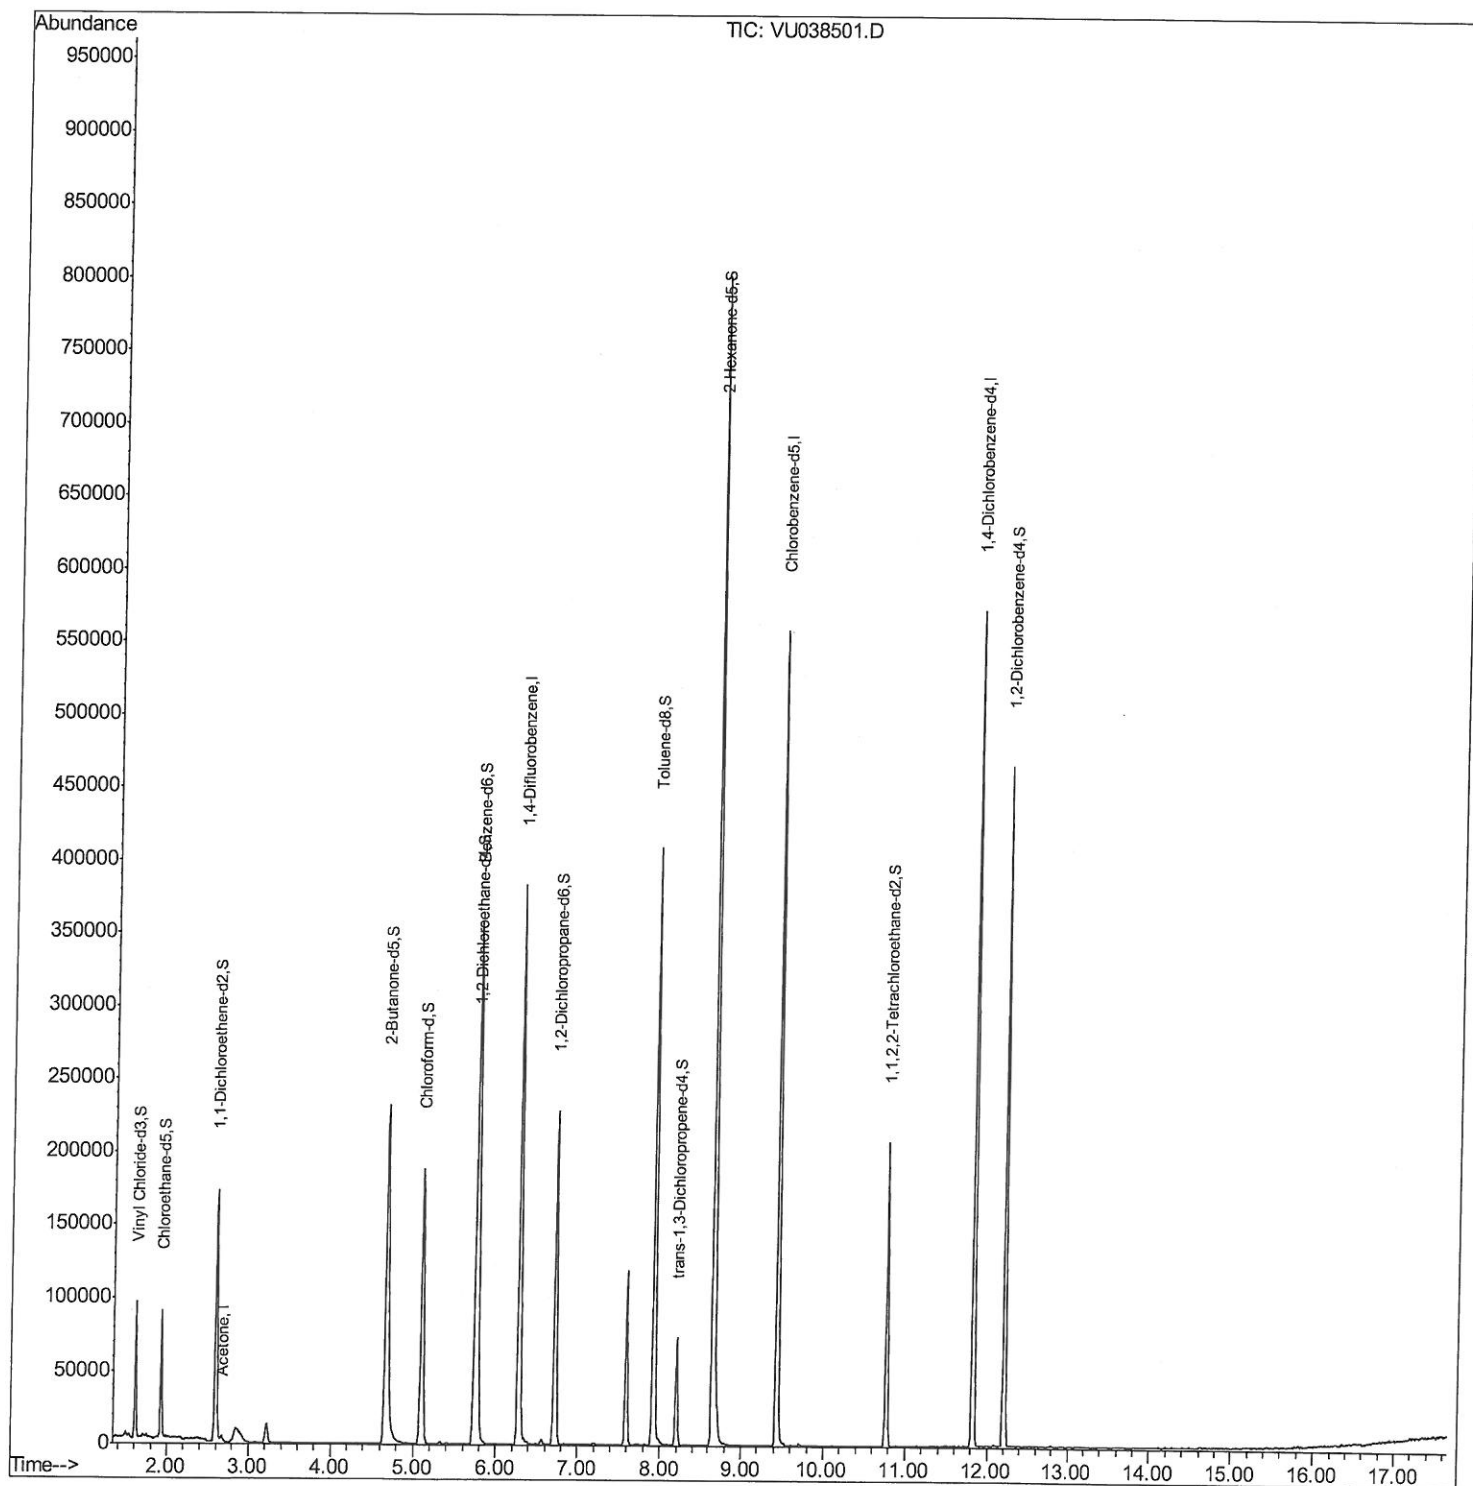

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060220\
Data File : VU038501.D
Acq On : 02 Jun 2020 18:14
Operator : JC/MD
Sample : L2856-07
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 00:51:49 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 03 00:48:29 2020
Response via : Initial Calibration

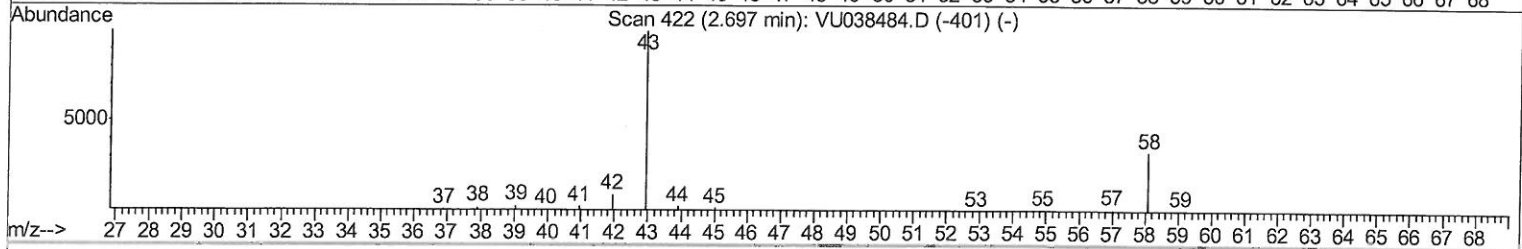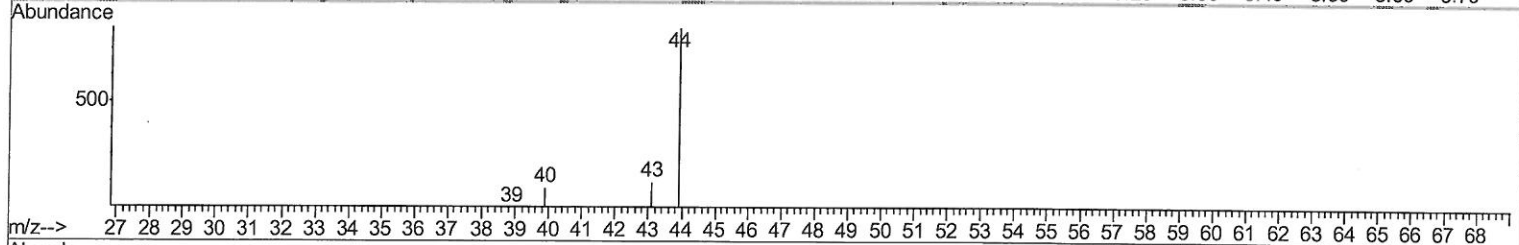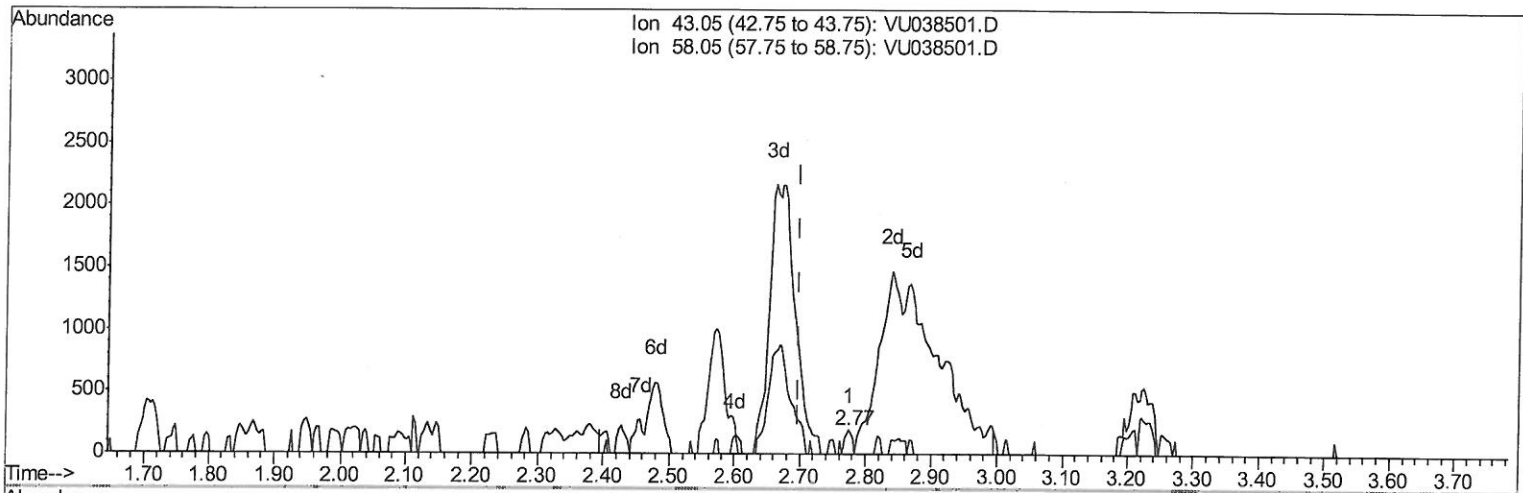

TIC: VU038501.D

(13) Acetone (T)

2.774min (+0.077) 0.04ug/L




response 171

Ion	Exp%	Act%
43.05	100	100
58.05	32.80	43.27
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060220\
 Data File : VU038501.D
 Acq On : 02 Jun 2020 18:14
 Operator : JC/MD
 Sample : L2856-07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 00:51:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 03 00:48:29 2020
 Response via : Initial Calibration

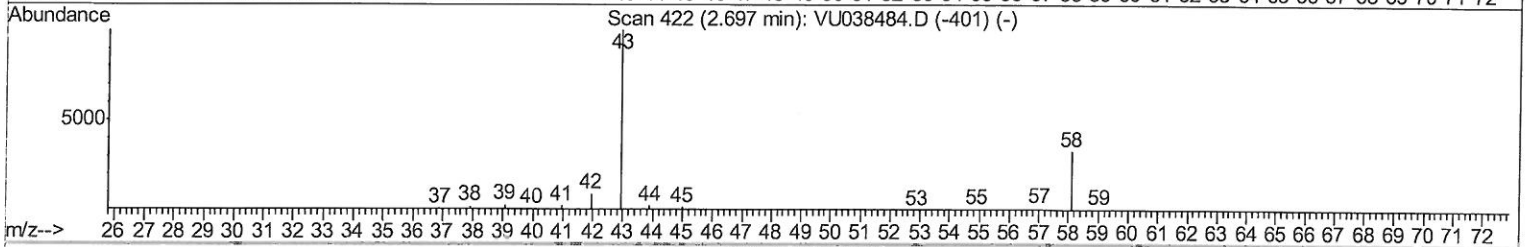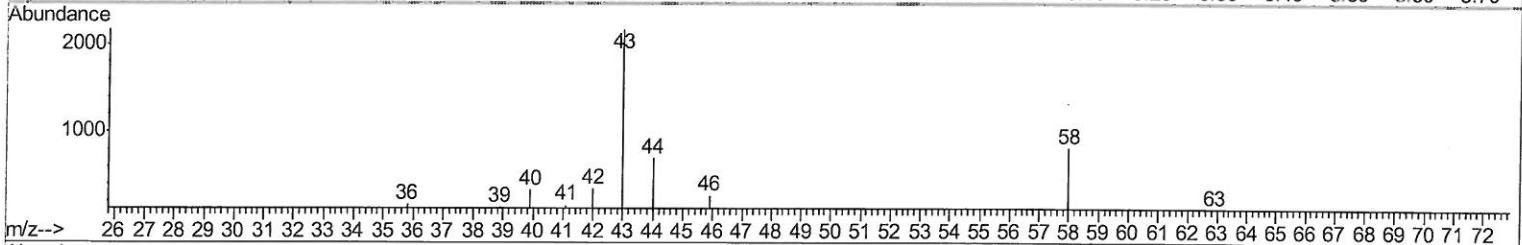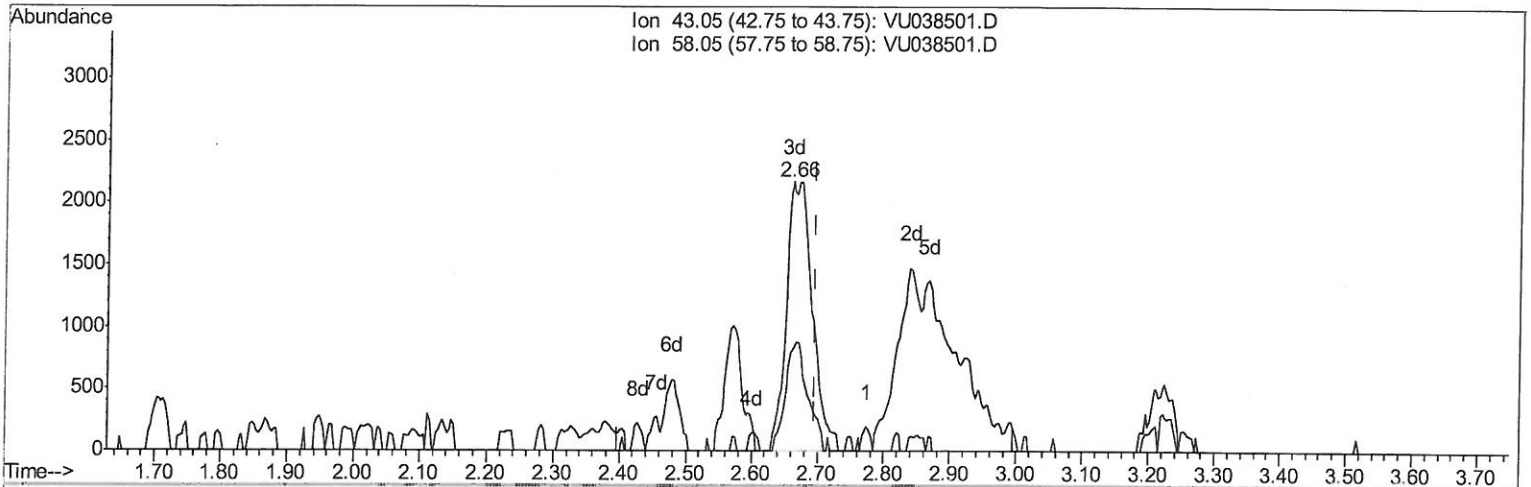

TIC: VU038501.D

(13) Acetone (T)

2.662min (-0.035) 1.47ug/L m

response 5922

Ion	Exp%	Act%
43.05	100	100
58.05	32.80	1.25
0.00	0.00	0.00
0.00	0.00	0.00

Handwritten: > md
06/11/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060220\
 Data File : VU038501.D
 Acq On : 02 Jun 2020 18:14
 Operator : JC/MD
 Sample : L2856-07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 02:26:29 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 03 00:48:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	313191	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	312220	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	147445	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	61636	3.04	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	60.80%		
7) Chloroethane-d5	1.93	69	60754	3.90	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	78.00%		
11) 1,1-Dichloroethene-d2	2.59	63	103503	2.59	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	51.80%#		
20) 2-Butanone-d5	4.67	46	326298	52.99	ug/L	-0.02
Spiked Amount 50.000	Range 40 - 130		Recovery =	105.98%		
24) Chloroform-d	5.10	84	171189	4.50	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	90.00%		
26) 1,2-Dichloroethane-d4	5.74	65	106275	4.92	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	98.40%		
32) Benzene-d6	5.76	84	328219	4.21	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	84.20%		
36) 1,2-Dichloropropane-d6	6.72	67	105870	4.42	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	88.40%		
41) Toluene-d8	7.92	98	267051	3.82	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	76.40%		
43) trans-1,3-Dichloropropene-	8.20	79	41771	4.05	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	81.00%		
46) 2-Hexanone-d5	8.65	63	279885	54.98	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	109.96%		
57) 1,1,2,2-Tetrachloroethane-	10.77	84	96251	4.73	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	94.60%		
64) 1,2-Dichlorobenzene-d4	12.20	152	116165	4.57	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	91.40%		

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.66	43	5922m	1.470	ug/L	

7 MD
06/11/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed