

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU060220\
 Data File : VU038495.D
 Acq On : 02 Jun 2020 15:55
 Operator : JC/MD
 Sample : L2844-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AE5

Quant Time: Jun 03 01:38:29 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 03 00:48:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	282112	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	283014	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	135253	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	67006	3.67	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.40%
7) Chloroethane-d5	1.93	69	65526	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.40%
11) 1,1-Dichloroethene-d2	2.59	63	107993	3.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.20%
20) 2-Butanone-d5	4.68	46	355494	64.09	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	128.18%
24) Chloroform-d	5.10	84	177392	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.40%
26) 1,2-Dichloroethane-d4	5.74	65	109029	5.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.00%
32) Benzene-d6	5.76	84	339885	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.20%
36) 1,2-Dichloropropane-d6	6.72	67	108452	4.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.80%
41) Toluene-d8	7.92	98	280251	4.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.40%
43) trans-1,3-Dichloropropene-	8.20	79	44028	4.71	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.20%
46) 2-Hexanone-d5	8.66	63	305781	66.27	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	132.54%#
57) 1,1,2,2-Tetrachloroethane-	10.77	84	102750	5.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	111.40%
64) 1,2-Dichlorobenzene-d4	12.20	152	122517	5.25	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.00%


Target Compounds					Qvalue
13) Acetone	2.69	43	10743	2.96 ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060220\
Data File : VU038495.D
Acq On : 02 Jun 2020 15:55
Operator : JC/MD
Sample : L2844-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AE5

Quant Time: Jun 03 01:38:29 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 03 00:48:29 2020
Response via : Initial Calibration

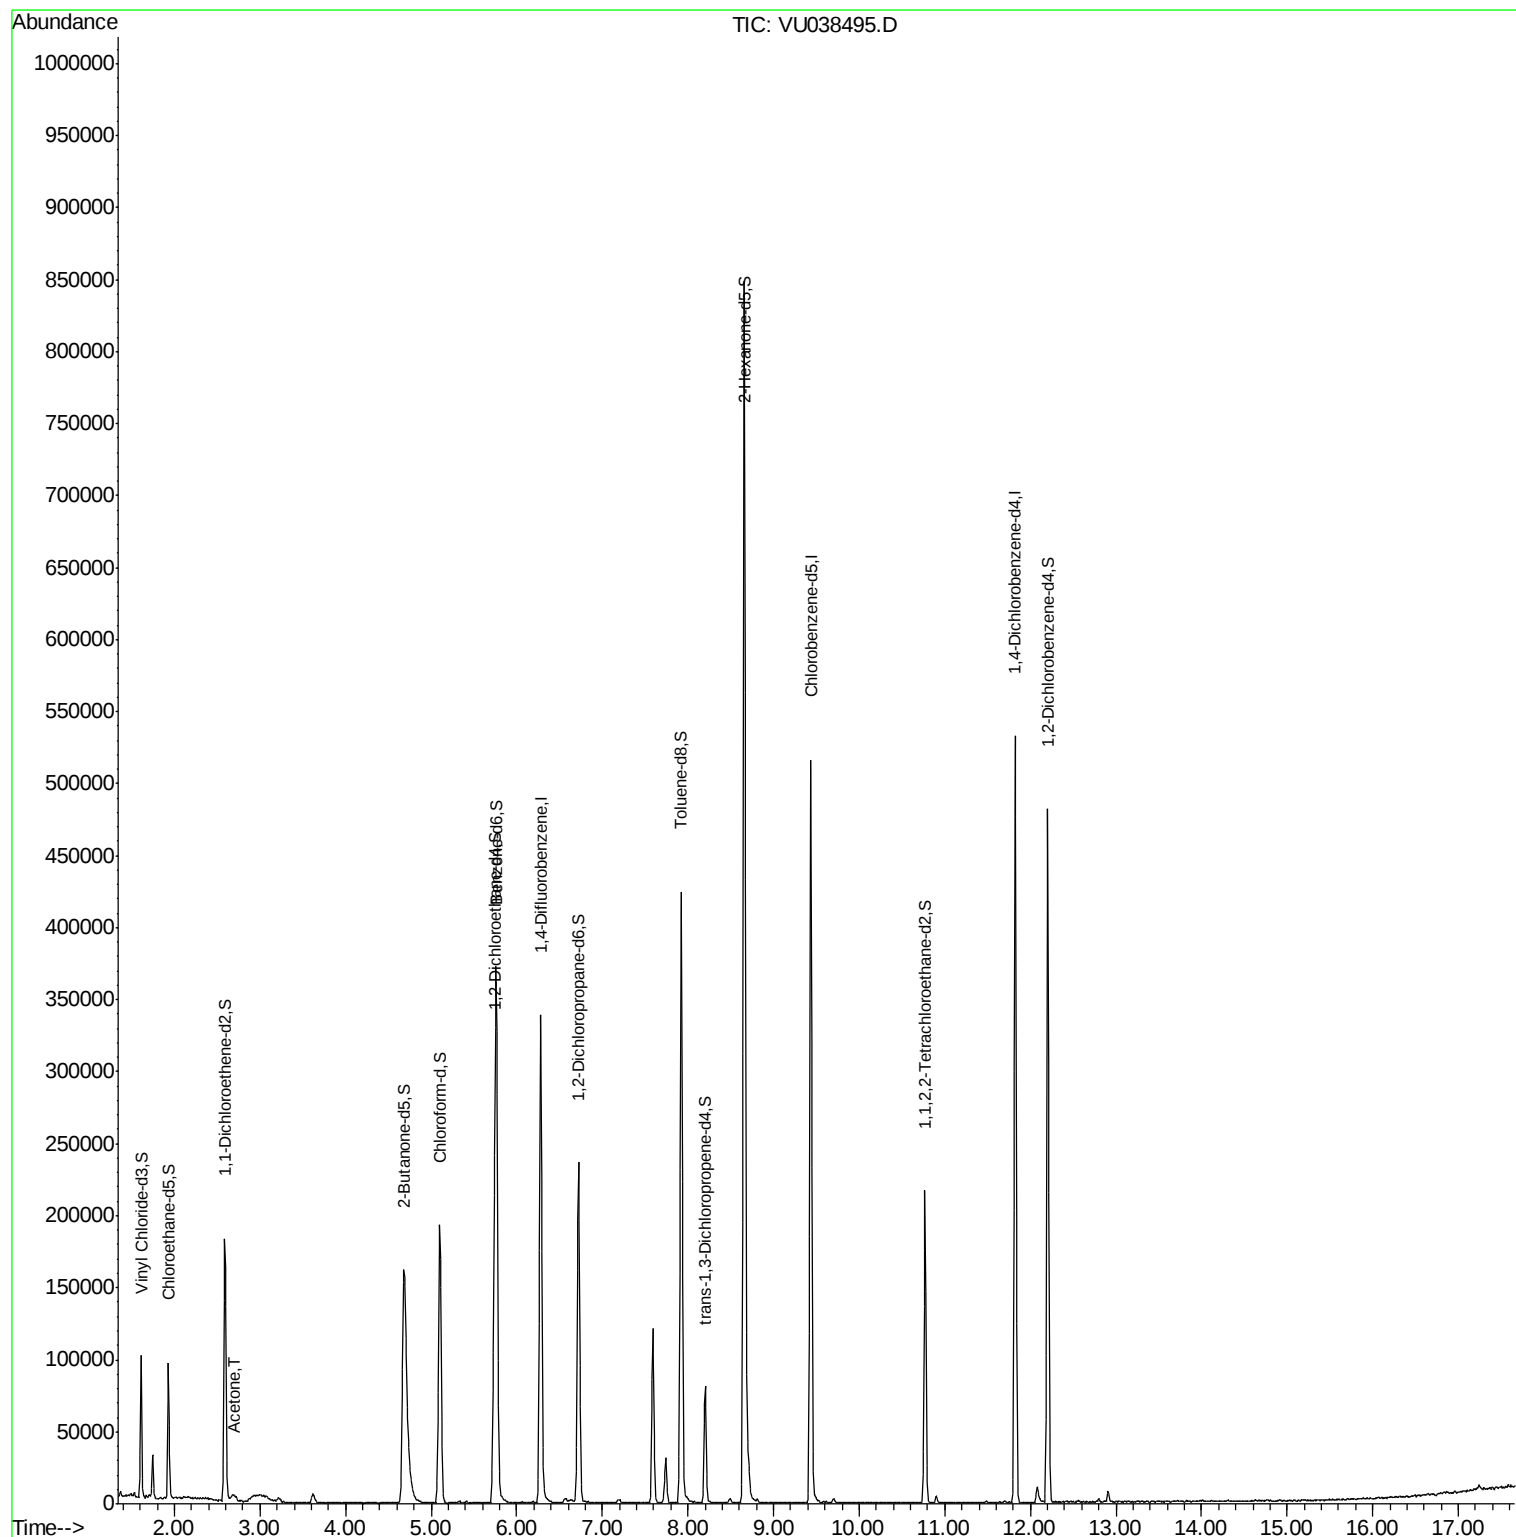

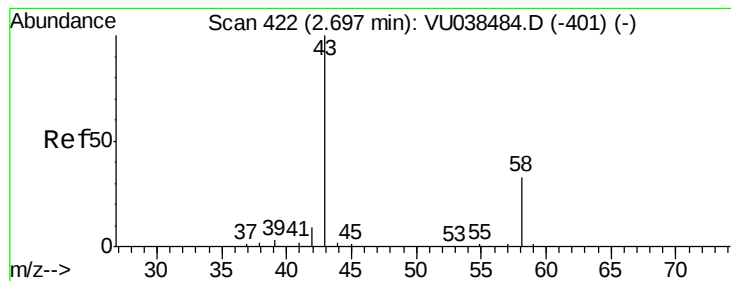

#13

Acetone

Concen: 2.96 ug/L

RT: 2.69 min Scan# 421

Delta R.T. -0.00 min

Lab File: VU038495.D

Acq: 02 Jun 2020 15:55

Instrument :

MSVOA_U

ClientSampleId :

C0AE5

Tgt Ion: 43 Resp: 10743

Ion Ratio Lower Upper

43 100

58 23.1 0.0 65.6

