

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060324\
 Data File : VU059125.D
 Acq On : 03 Jun 2024 16:22
 Operator : MD/SY
 Sample : P2659-08ME
 Misc : 4.60g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHC29ME

Quant Time: Jun 04 06:59:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 01 01:17:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	221379	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	229333	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	103858	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	78962	59.572	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 119.140%			
7) Chloroethane-d5	1.872	69	69375	61.100	ug/L	-0.04
Spiked Amount 50.000	Range 70 - 130		Recovery = 122.200%			
11) 1,1-Dichloroethene-d2	2.538	63	113476	43.372	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery = 86.740%			
21) 2-Butanone-d5	4.618	46	219598	175.769	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 175.770%#			
24) Chloroform-d	5.052	84	189785	71.924	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 143.840%#			
26) 1,2-Dichloroethane-d4	5.689	65	125610	77.667	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 155.340%#			
32) Benzene-d6	5.714	84	362704	68.909	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 137.820%#			
36) 1,2-Dichloropropane-d6	6.682	67	130049	71.658	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 143.320%#			
41) Toluene-d8	7.891	98	300315	67.211	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 134.420%#			
43) trans-1,3-Dichloroprop...	8.174	79	54052	73.681	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 147.360%#			
47) 2-Hexanone-d5	8.637	63	138865	165.465	ug/L	0.01
Spiked Amount 100.000	Range 45 - 130		Recovery = 165.460%#			
56) 1,1,2,2-Tetrachloroeth...	10.753	84	236005	76.837	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 153.680%#			
66) 1,2-Dichlorobenzene-d4	12.190	152	126421	81.567	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 163.140%#			
Target Compounds						Qvalue
15) Methyl Acetate	2.949	43	3453	1.484	ug/L	# 79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060324\
Data File : VU059125.D
Acq On : 03 Jun 2024 16:22
Operator : MD/SY
Sample : P2659-08ME
Misc : 4.60g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHC29ME

Quant Time: Jun 04 06:59:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 01 01:17:21 2024
Response via : Initial Calibration

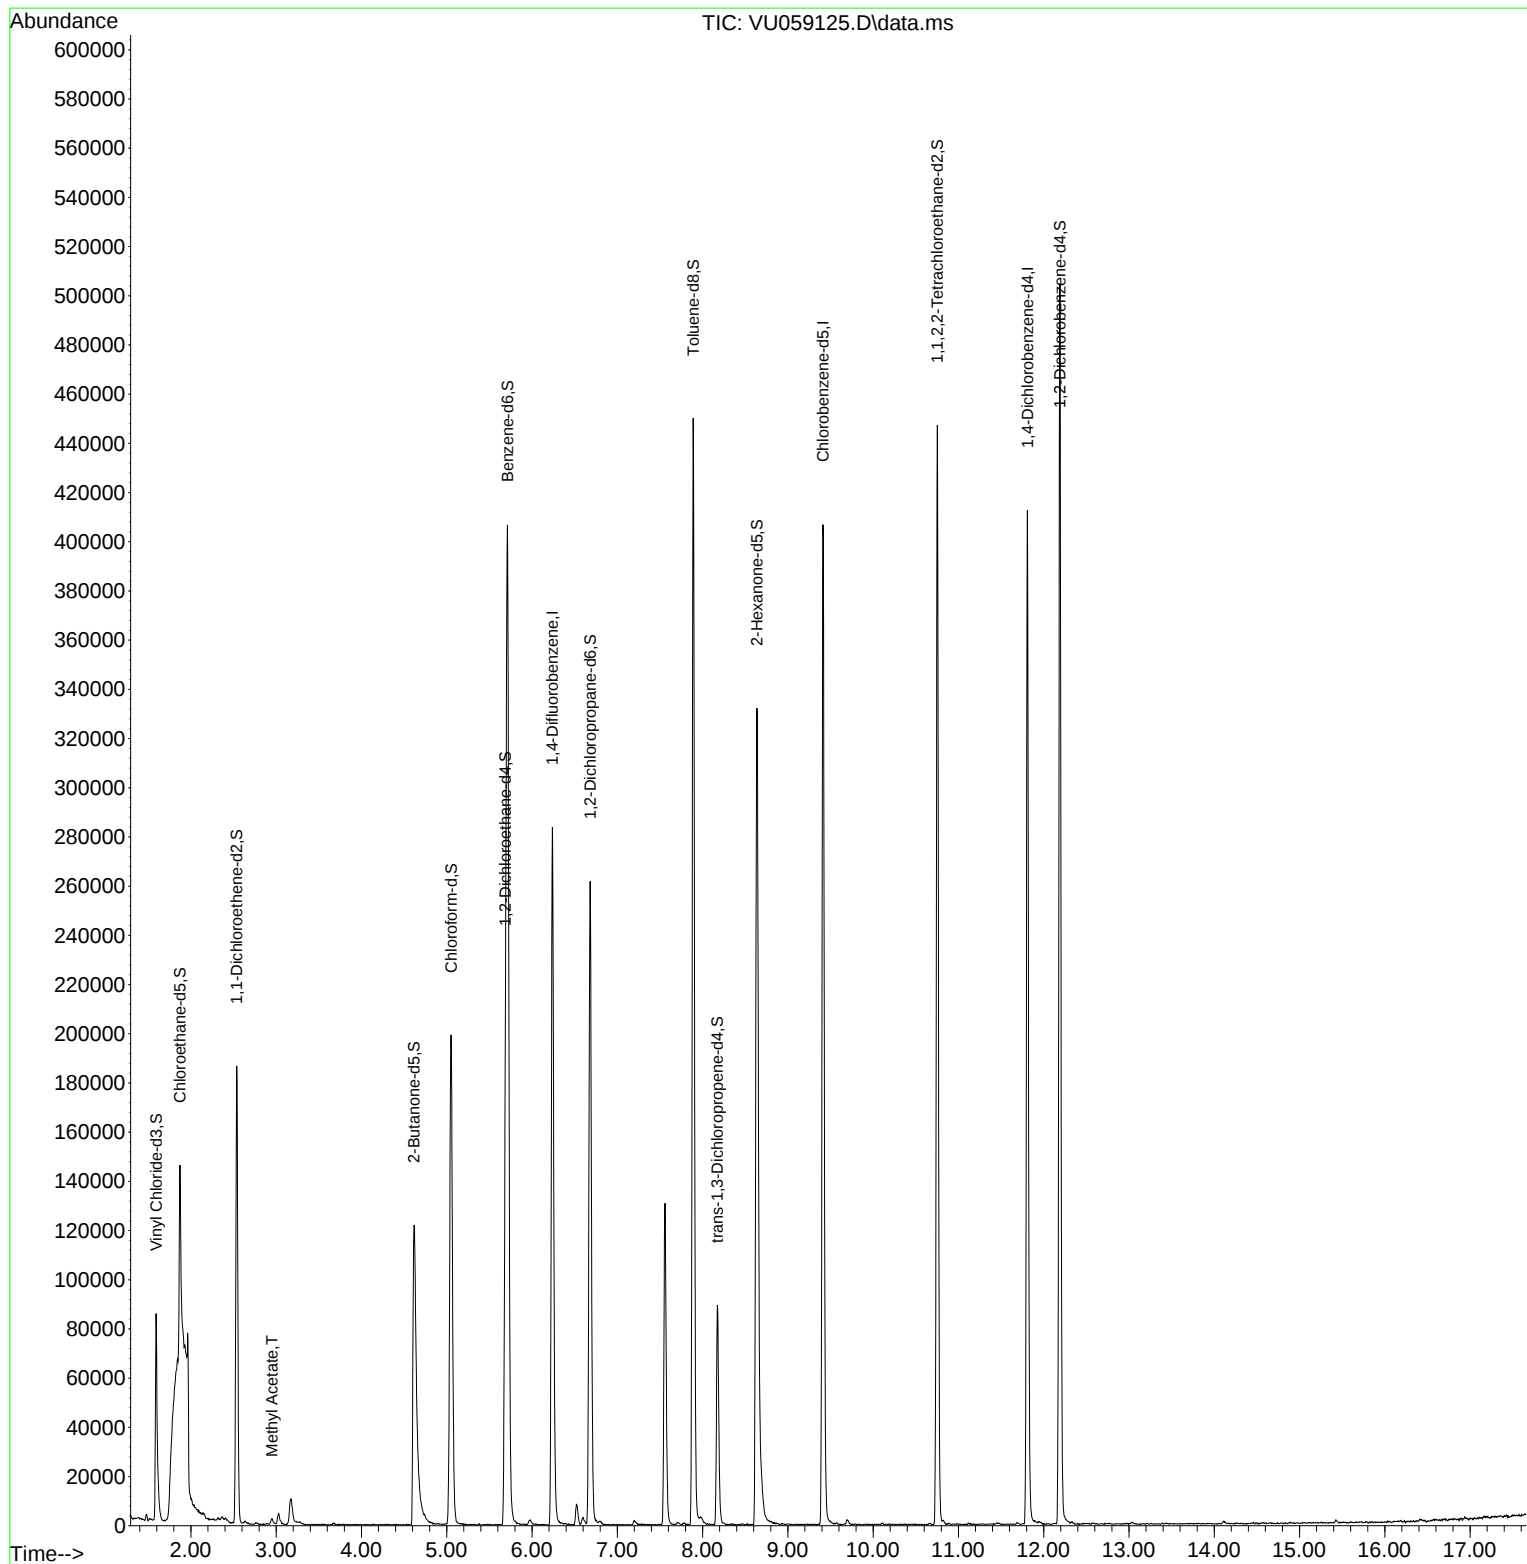

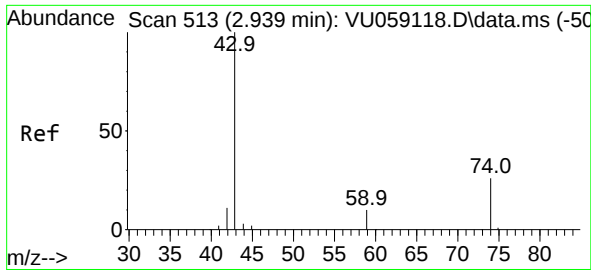

#15
Methyl Acetate
Concen: 1.484 ug/L
RT: 2.949 min Scan# 51
Delta R.T. 0.010 min
Lab File: VU059125.D
Acq: 03 Jun 2024 16:22

Instrument :
MSVOA_U
ClientSampleId :
BHC29ME

Tgt Ion: 43 Resp: 3453
Ion Ratio Lower Upper
43 100
74 15.1 20.8 31.2#

