

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060324\
 Data File : VU059120.D
 Acq On : 03 Jun 2024 13:27
 Operator : MD/SY
 Sample : VU0603WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK064

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	112	rVB	68541	81922	12.51%	1.529%
2	1.763	139	147	156	rBV3	7932	10753	1.64%	0.201%
3	1.908	184	192	207	rBV	60389	84014	12.83%	1.568%
4	2.560	384	395	411	rBV	116732	191582	29.26%	3.576%
5	2.750	452	454	458	rVB	273	165	0.03%	0.003%
6	2.789	458	466	475	rBV2	2107	3271	0.50%	0.061%
7	2.866	486	490	493	rVB	284	210	0.03%	0.004%
8	2.888	493	497	499	rBV2	252	209	0.03%	0.004%
9	2.956	513	518	524	rBV2	480	631	0.10%	0.012%
10	3.040	532	544	554	rBV3	3774	6865	1.05%	0.128%
11	3.316	625	630	635	rBV2	381	473	0.07%	0.009%
12	3.355	635	642	643	rBV3	1024	1095	0.17%	0.020%
13	3.638	726	730	732	rBV2	306	225	0.03%	0.004%
14	3.994	837	841	844	rBV2	269	239	0.04%	0.004%
15	4.056	857	860	864	rBV	296	281	0.04%	0.005%
16	4.130	880	883	887	rVB2	279	172	0.03%	0.003%
17	4.158	887	892	897	rVB2	298	307	0.05%	0.006%
18	4.194	900	903	905	rBV	224	174	0.03%	0.003%
19	4.223	909	912	916	rVB	247	216	0.03%	0.004%
20	4.326	940	944	950	rVB2	287	391	0.06%	0.007%
21	4.493	990	996	999	rBV	342	369	0.06%	0.007%
22	4.612	1023	1033	1065	rBV	78646	199933	30.54%	3.732%
23	4.824	1096	1099	1107	rVB2	724	727	0.11%	0.014%
24	5.056	1156	1171	1191	rBV	122903	275350	42.05%	5.139%
25	5.207	1215	1218	1221	rVV2	356	254	0.04%	0.005%
26	5.223	1221	1223	1227	rVV	322	216	0.03%	0.004%
27	5.242	1227	1229	1233	rVB2	308	275	0.04%	0.005%
28	5.290	1238	1244	1245	rBV2	339	226	0.03%	0.004%
29	5.313	1248	1251	1257	rVB3	441	434	0.07%	0.008%
30	5.380	1267	1272	1279	rVB2	521	593	0.09%	0.011%
31	5.509	1310	1312	1315	rBV2	333	171	0.03%	0.003%
32	5.567	1326	1330	1335	rBV	283	317	0.05%	0.006%
33	5.621	1341	1347	1349	rBV2	280	279	0.04%	0.005%
34	5.718	1358	1377	1399	rBV2	234207	654744	100.00%	12.221%
35	6.004	1460	1466	1468	rBV	301	287	0.04%	0.005%
36	6.242	1528	1540	1562	rBV	241603	471745	72.05%	8.805%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060324\
 Data File : VU059120.D
 Acq On : 03 Jun 2024 13:27
 Operator : MD/SY
 Sample : VU0603WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK064

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.531	1620	1630	1650	rVB6	6219	13658	2.09%	0.255%
38	6.605	1650	1653	1657	rBV2	252	255	0.04%	0.005%
39	6.682	1662	1677	1695	rBV	161093	314313	48.01%	5.867%
40	6.827	1719	1722	1726	rVB4	396	353	0.05%	0.007%
41	6.850	1726	1729	1732	rBV2	206	178	0.03%	0.003%
42	6.872	1732	1736	1738	rBV2	209	172	0.03%	0.003%
43	6.965	1760	1765	1769	rVB2	358	383	0.06%	0.007%
44	6.988	1769	1772	1774	rBV	258	183	0.03%	0.003%
45	7.049	1786	1791	1793	rBV2	183	190	0.03%	0.004%
46	7.097	1804	1806	1812	rBV2	353	351	0.05%	0.007%
47	7.252	1850	1854	1864	rVV2	274	426	0.07%	0.008%
48	7.371	1888	1891	1895	rVB	270	233	0.04%	0.004%
49	7.428	1906	1909	1913	rVB	356	285	0.04%	0.005%
50	7.454	1913	1917	1921	rBV2	221	264	0.04%	0.005%
51	7.560	1939	1950	1967	rBV	75611	137891	21.06%	2.574%
52	7.711	1993	1997	2001	rVB	303	241	0.04%	0.004%
53	7.895	2041	2054	2075	rVV	256174	452387	69.09%	8.444%
54	8.174	2131	2141	2160	rBV2	52118	91381	13.96%	1.706%
55	8.396	2207	2210	2218	rVB3	445	441	0.07%	0.008%
56	8.448	2220	2226	2228	rBV3	356	359	0.05%	0.007%
57	8.493	2235	2240	2243	rBV2	242	225	0.03%	0.004%
58	8.551	2253	2258	2266	rVB4	724	907	0.14%	0.017%
59	8.628	2271	2282	2325	rBV2	186317	387640	59.20%	7.235%
60	8.930	2367	2376	2382	rBV4	750	989	0.15%	0.018%
61	9.197	2455	2459	2462	rBV	202	211	0.03%	0.004%
62	9.264	2476	2480	2484	rBV2	280	228	0.03%	0.004%
63	9.319	2489	2497	2501	rVB	463	714	0.11%	0.013%
64	9.342	2501	2504	2506	rBV	265	198	0.03%	0.004%
65	9.412	2513	2526	2550	rBV	356907	619251	94.58%	11.558%
66	9.570	2568	2575	2586	rVB4	1215	2406	0.37%	0.045%
67	9.615	2586	2589	2592	rBV2	231	174	0.03%	0.003%
68	9.698	2612	2615	2616	rBV2	370	208	0.03%	0.004%
69	9.859	2657	2665	2670	rBV2	233	354	0.05%	0.007%
70	9.888	2670	2674	2678	rVB2	242	244	0.04%	0.005%
71	9.949	2685	2693	2698	rBV2	257	417	0.06%	0.008%
72	10.020	2713	2715	2718	rVB	305	172	0.03%	0.003%
73	10.100	2735	2740	2741	rBV2	740	584	0.09%	0.011%
74	10.444	2844	2847	2851	rBV2	280	271	0.04%	0.005%
75	10.489	2855	2861	2864	rVV3	473	562	0.09%	0.010%
76	10.647	2903	2910	2914	rBV5	821	903	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060324\
 Data File : VU059120.D
 Acq On : 03 Jun 2024 13:27
 Operator : MD/SY
 Sample : VU0603WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK064

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	10.750	2930	2942	2958	rBV	242979	398285	60.83%	7.434%
78	10.994	3014	3018	3022	rBV2	328	396	0.06%	0.007%
79	11.091	3045	3048	3051	rBV2	504	338	0.05%	0.006%
80	11.476	3161	3168	3176	rVB3	973	1446	0.22%	0.027%
81	11.522	3176	3182	3185	rBV	284	325	0.05%	0.006%
82	11.747	3247	3252	3259	rBV4	1134	1475	0.23%	0.028%
83	11.808	3259	3271	3291	rBV	308709	513458	78.42%	9.584%
84	12.100	3359	3362	3365	rVB	290	171	0.03%	0.003%
85	12.190	3377	3390	3416	rBV	239924	416314	63.58%	7.771%
86	12.402	3453	3456	3460	rBV	395	238	0.04%	0.004%
87	12.451	3469	3471	3475	rBV	238	192	0.03%	0.004%
88	13.145	3684	3687	3689	rBV2	299	172	0.03%	0.003%
89	13.271	3723	3726	3732	rVB2	437	389	0.06%	0.007%
90	13.438	3775	3778	3782	rVB2	237	207	0.03%	0.004%
91	13.464	3782	3786	3789	rBV	405	284	0.04%	0.005%
92	13.557	3813	3815	3822	rVB	332	296	0.05%	0.006%
93	13.743	3868	3873	3876	rBV	329	338	0.05%	0.006%
94	14.097	3979	3983	3984	rBV2	974	595	0.09%	0.011%
95	14.338	4051	4058	4070	rBV5	1128	1736	0.27%	0.032%
96	14.521	4113	4115	4118	rBV	347	199	0.03%	0.004%
97	14.550	4122	4124	4129	rBV	300	276	0.04%	0.005%
98	14.920	4236	4239	4243	rBV3	297	273	0.04%	0.005%
99	15.090	4290	4292	4297	rVB2	354	280	0.04%	0.005%
100	15.113	4297	4299	4301	rBV2	327	187	0.03%	0.003%




Sum of corrected areas: 5357587

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060324\
Data File : VU059120.D
Acq On : 03 Jun 2024 13:27
Operator : MD/SY
Sample : VU0603WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK064

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

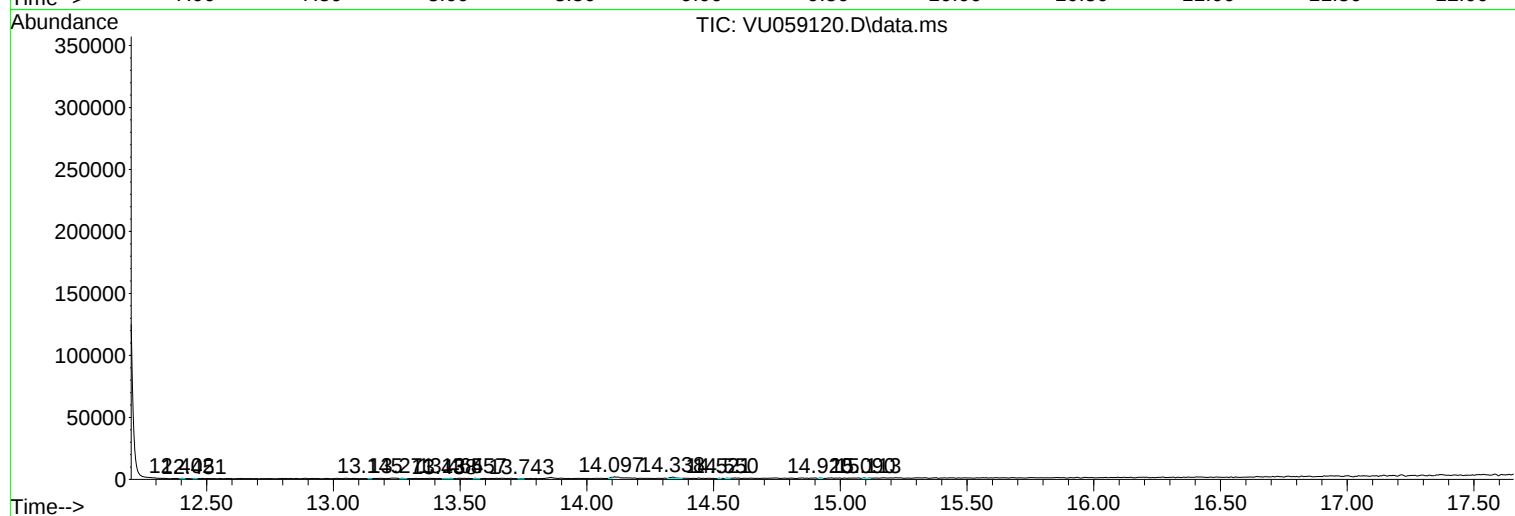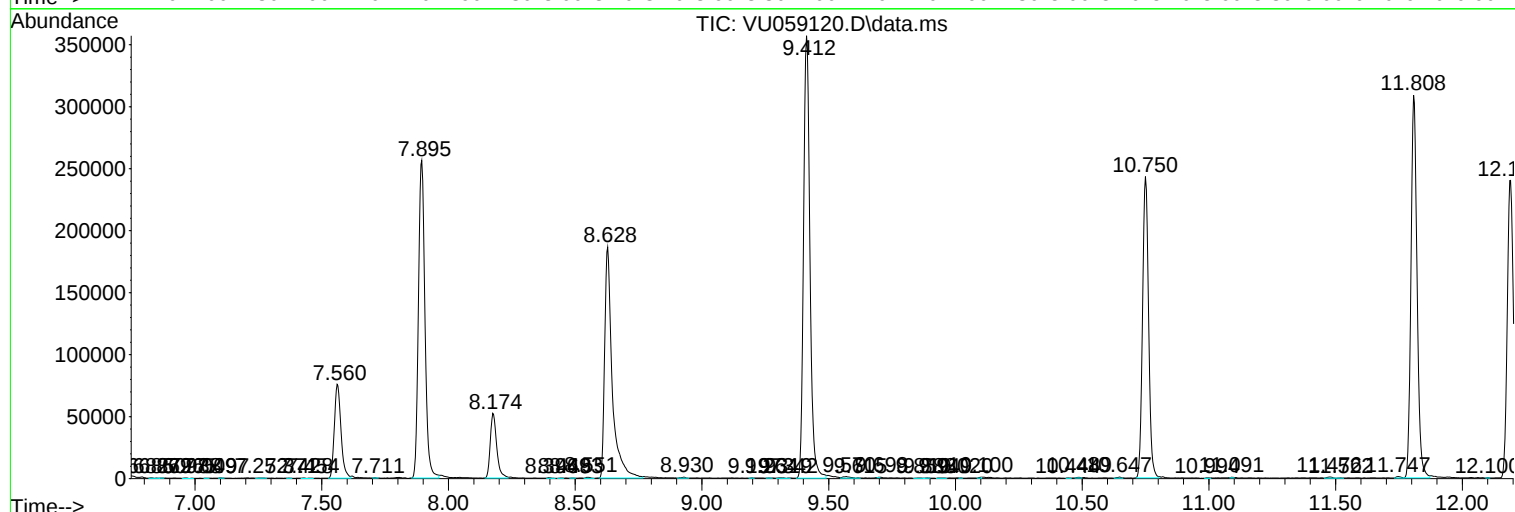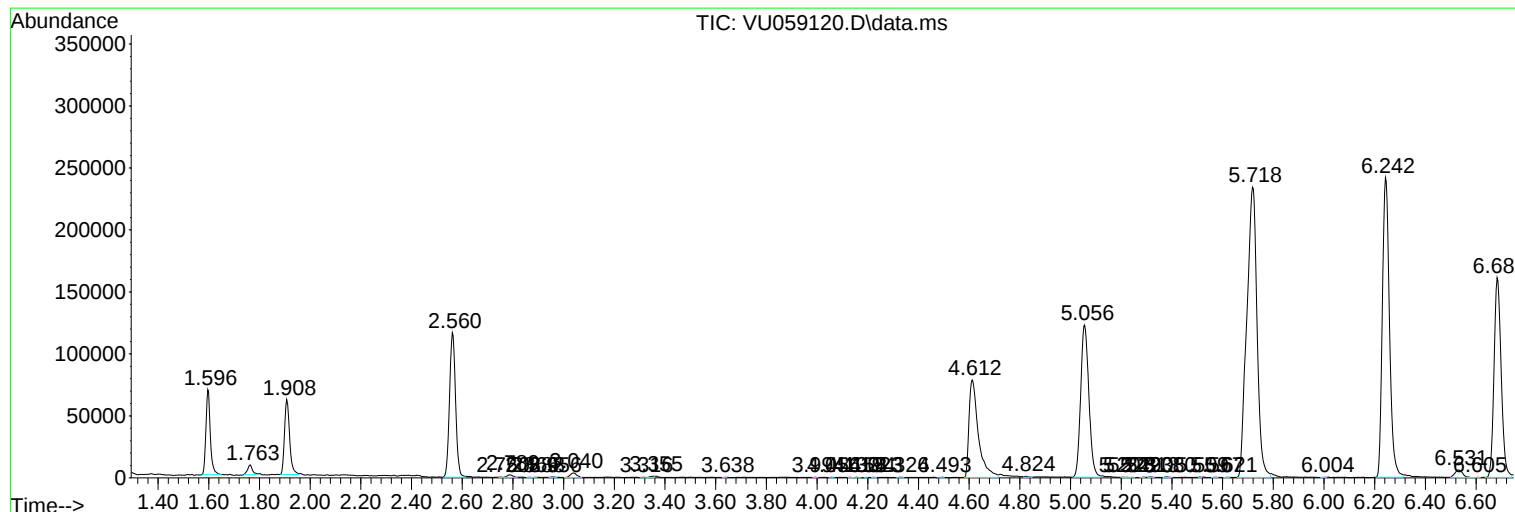

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060324\
Data File : VU059120.D
Acq On : 03 Jun 2024 13:27
Operator : MD/SY
Sample : VU0603WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK064

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060324\
Data File : VU059120.D
Acq On : 03 Jun 2024 13:27
Operator : MD/SY
Sample : VU0603WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK064

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------