

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
 Data File : VU059137.D
 Acq On : 04 Jun 2024 13:28
 Operator : MD/SY
 Sample : P2659-18ME
 Misc : 4.87g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jun 05 05:32:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 05 05:30:09 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	180271	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	190301	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	77465	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	42899	39.745	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.480%
7) Chloroethane-d5	1.907	69	41632	45.027	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.060%
11) 1,1-Dichloroethene-d2	2.560	63	60668	28.476	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	56.960%#
21) 2-Butanone-d5	4.612	46	128518	126.324	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	126.320%
24) Chloroform-d	5.055	84	112698	52.449	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.900%
26) 1,2-Dichloroethane-d4	5.695	65	73980	56.174	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	112.340%
32) Benzene-d6	5.721	84	203552	46.604	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.200%
36) 1,2-Dichloropropane-d6	6.682	67	76692	50.925	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.860%
41) Toluene-d8	7.891	98	160231	43.215	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.420%
43) trans-1,3-Dichloroprop...	8.174	79	29753	48.876	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.760%
47) 2-Hexanone-d5	8.627	63	64766	93.000	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.000%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	129717	50.894	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.780%
66) 1,2-Dichlorobenzene-d4	12.190	152	62332	53.919	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.840%
Target Compounds						
					Qvalue	
60) 1,2,3-Trichloropropane	11.807	75	10677	4.956	ug/L #	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
Data File : VU059137.D
Acq On : 04 Jun 2024 13:28
Operator : MD/SY
Sample : P2659-18ME
Misc : 4.87g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jun 05 05:32:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 05 05:30:09 2024
Response via : Initial Calibration

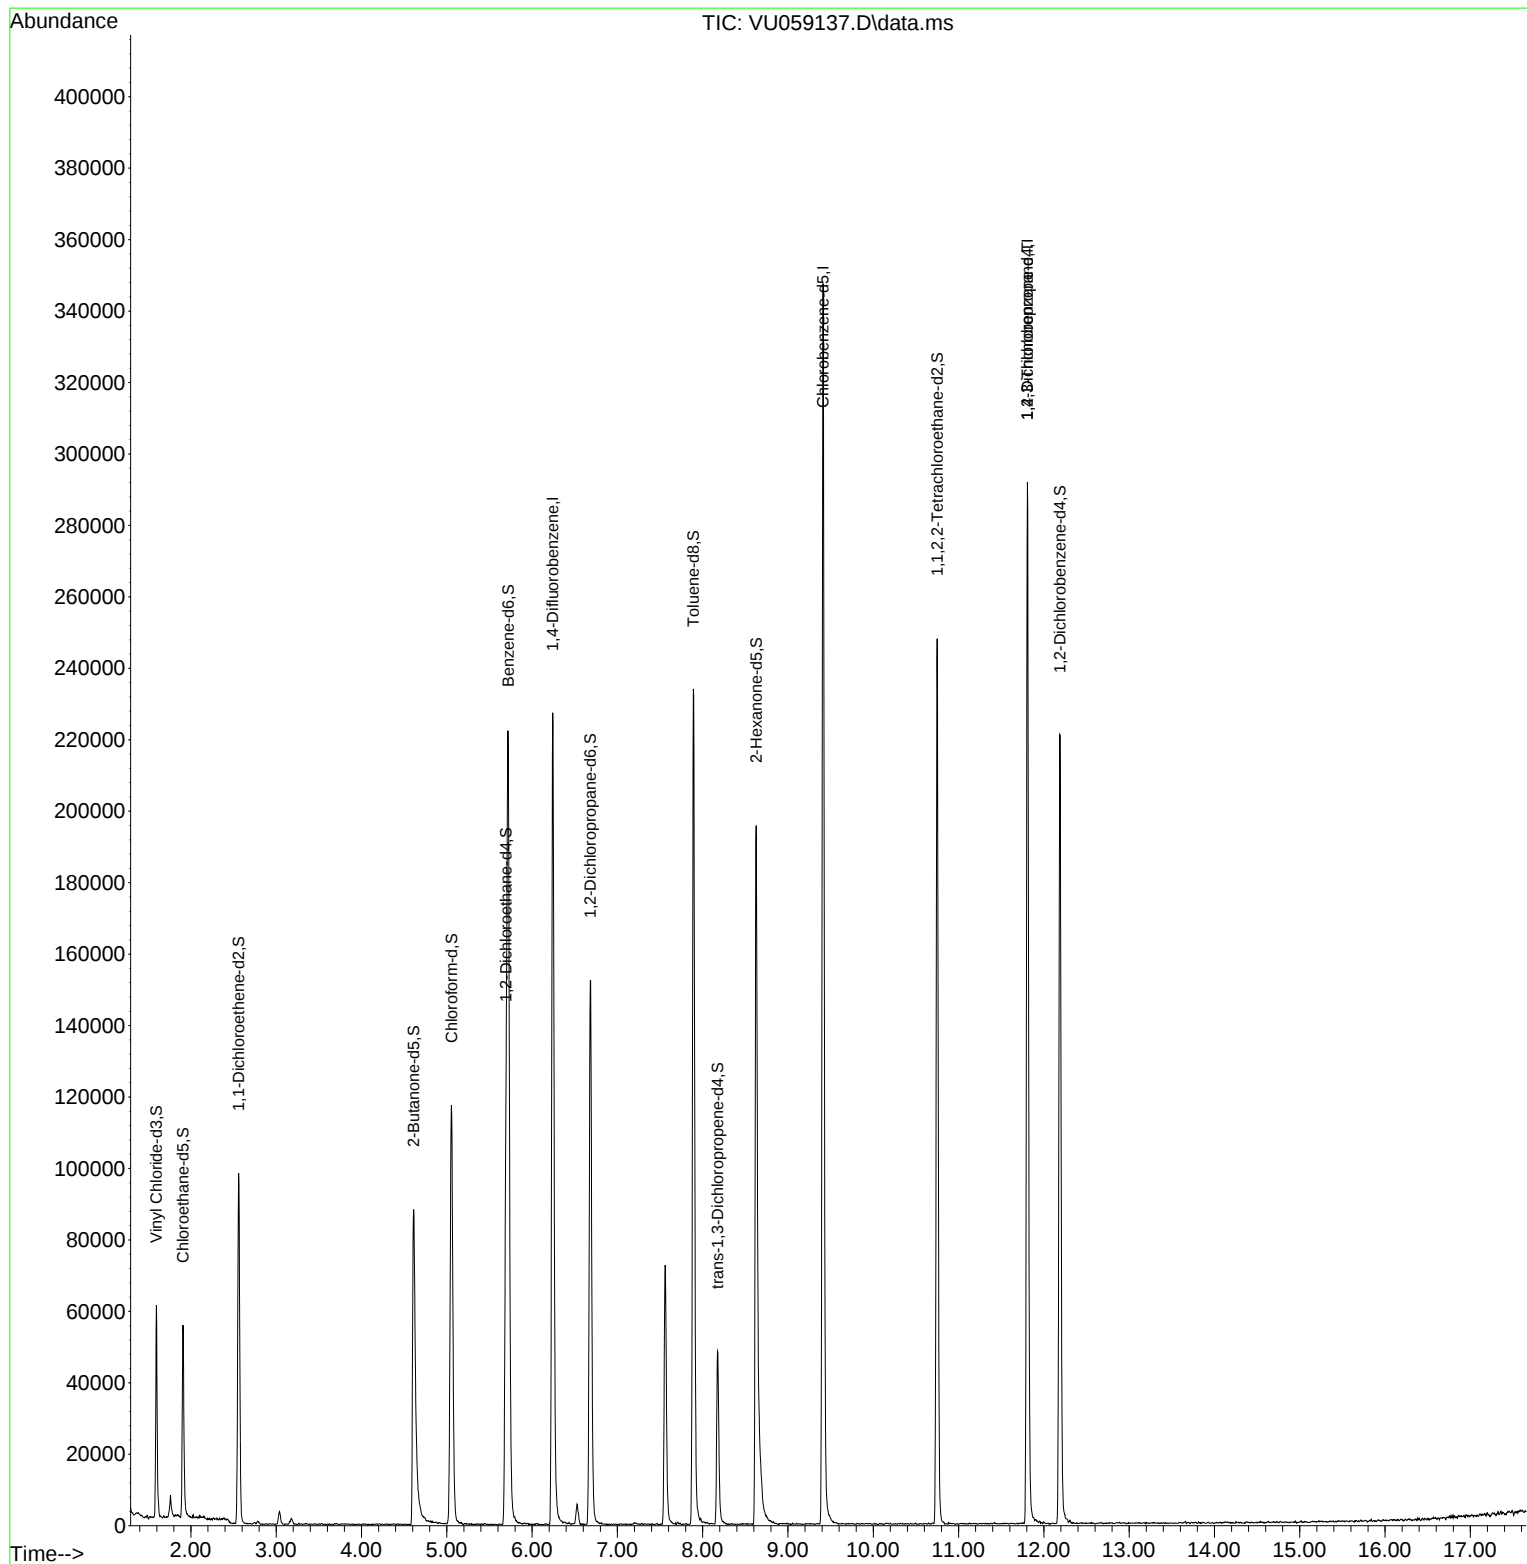

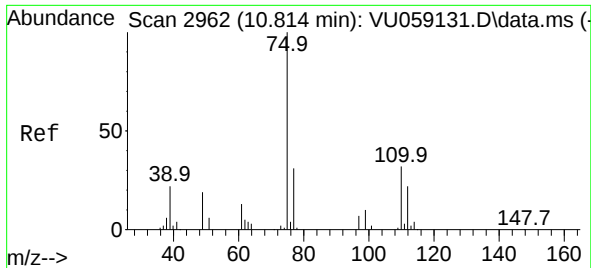

#60

1,2,3-Trichloropropane

Concen: 4.956 ug/L

RT: 11.807 min Scan# 31

Delta R.T. 0.993 min


Lab File: VU059137.D

Acq: 04 Jun 2024 13:28

Instrument :

MSVOA_U

ClientSampleId :

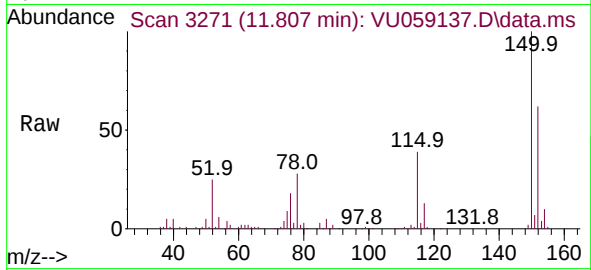

Tgt Ion: 75 Resp: 10677

Ion Ratio Lower Upper

75 100

77 32.7 26.2 39.2

110 2.1 28.4 42.6#

