

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
 Data File : VU059134.D
 Acq On : 04 Jun 2024 12:20
 Operator : MD/SY
 Sample : P2663-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059134.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	113	rVB	69097	81874	12.25%	1.515%
2	1.760	141	146	152	rVB4	3515	3983	0.60%	0.074%
3	1.907	184	192	215	rVB	62750	86864	12.99%	1.608%
4	2.560	382	395	411	rBV	116962	190734	28.53%	3.530%
5	2.788	459	466	473	rVB3	1165	2003	0.30%	0.037%
6	2.821	473	476	482	rVB2	228	237	0.04%	0.004%
7	2.850	482	485	488	rBV2	202	160	0.02%	0.003%
8	2.962	517	520	523	rBV	239	161	0.02%	0.003%
9	3.039	535	544	553	rBV5	2300	4187	0.63%	0.077%
10	3.100	560	563	566	rBV	214	180	0.03%	0.003%
11	3.120	566	569	573	rVV	233	165	0.02%	0.003%
12	3.181	575	588	599	rVB3	2028	4722	0.71%	0.087%
13	3.290	617	622	626	rVB2	292	370	0.06%	0.007%
14	3.325	626	633	635	rBV2	272	377	0.06%	0.007%
15	3.345	635	639	642	rBV	326	233	0.03%	0.004%
16	3.403	654	657	661	rBV	238	197	0.03%	0.004%
17	3.460	670	675	679	rBV2	248	255	0.04%	0.005%
18	3.518	690	693	699	rBV2	149	145	0.02%	0.003%
19	3.692	745	747	751	rVB	223	146	0.02%	0.003%
20	3.721	751	756	761	rBV2	293	361	0.05%	0.007%
21	3.801	773	781	786	rBV2	327	544	0.08%	0.010%
22	3.907	810	814	820	rBV	133	182	0.03%	0.003%
23	4.364	950	956	960	rVV2	153	206	0.03%	0.004%
24	4.515	998	1003	1008	rVV	269	276	0.04%	0.005%
25	4.573	1013	1021	1022	rBV2	193	204	0.03%	0.004%
26	4.612	1022	1033	1063	rBV	85311	217005	32.46%	4.016%
27	5.052	1155	1170	1194	rBV	126698	281657	42.13%	5.213%
28	5.290	1241	1244	1247	rVB2	360	177	0.03%	0.003%
29	5.505	1304	1311	1315	rBV2	267	317	0.05%	0.006%
30	5.550	1322	1325	1331	rBV2	220	217	0.03%	0.004%
31	5.602	1339	1341	1347	rVV	192	146	0.02%	0.003%
32	5.718	1357	1377	1404	rBV2	239843	668572	100.00%	12.373%
33	5.933	1440	1444	1451	rBV2	285	237	0.04%	0.004%
34	6.052	1478	1481	1483	rBV2	267	204	0.03%	0.004%
35	6.177	1516	1520	1526	rBV2	347	309	0.05%	0.006%
36	6.242	1526	1540	1571	rBV	239173	463747	69.36%	8.582%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
 Data File : VU059134.D
 Acq On : 04 Jun 2024 12:20
 Operator : MD/SY
 Sample : P2663-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.399	1585	1589	1592	rVB4	402	339	0.05%	0.006%
38	6.531	1619	1630	1640	rVB8	5464	11297	1.69%	0.209%
39	6.682	1664	1677	1699	rBV	163077	321577	48.10%	5.951%
40	6.798	1711	1713	1715	rVB2	403	184	0.03%	0.003%
41	7.046	1788	1790	1796	rBV2	209	229	0.03%	0.004%
42	7.197	1833	1837	1839	rBV3	366	221	0.03%	0.004%
43	7.402	1896	1901	1904	rBV2	188	208	0.03%	0.004%
44	7.418	1904	1906	1909	rVB	338	169	0.03%	0.003%
45	7.444	1909	1914	1919	rBV2	358	432	0.06%	0.008%
46	7.560	1938	1950	1975	rBV	76245	139138	20.81%	2.575%
47	7.708	1989	1996	1998	rBV3	521	594	0.09%	0.011%
48	7.750	2004	2009	2011	rBV2	295	246	0.04%	0.005%
49	7.894	2041	2054	2073	rBV	257860	462305	69.15%	8.556%
50	8.174	2131	2141	2157	rBV2	53033	94336	14.11%	1.746%
51	8.367	2200	2201	2205	rVB	301	155	0.02%	0.003%
52	8.396	2205	2210	2212	rBV2	205	201	0.03%	0.004%
53	8.431	2217	2221	2226	rVB2	202	232	0.03%	0.004%
54	8.573	2261	2265	2268	rVB	203	150	0.02%	0.003%
55	8.627	2271	2282	2321	rBV2	192754	405416	60.64%	7.503%
56	9.004	2397	2399	2401	rVB2	273	141	0.02%	0.003%
57	9.020	2401	2404	2407	rBV2	222	168	0.03%	0.003%
58	9.052	2411	2414	2417	rBV	363	212	0.03%	0.004%
59	9.412	2513	2526	2551	rBV	356081	603169	90.22%	11.163%
60	9.695	2611	2614	2619	rVV3	269	256	0.04%	0.005%
61	9.824	2651	2654	2660	rVB2	214	193	0.03%	0.004%
62	9.984	2702	2704	2709	rVB2	186	154	0.02%	0.003%
63	10.213	2772	2775	2776	rBV	269	182	0.03%	0.003%
64	10.377	2823	2826	2829	rBV	259	263	0.04%	0.005%
65	10.486	2855	2860	2864	rBV2	373	293	0.04%	0.005%
66	10.573	2883	2887	2891	rBV2	191	244	0.04%	0.005%
67	10.650	2908	2911	2913	rBV2	365	177	0.03%	0.003%
68	10.750	2929	2942	2965	rBV	251926	412351	61.68%	7.631%
69	10.856	2972	2975	2979	rVB2	357	276	0.04%	0.005%
70	11.074	3039	3043	3045	rBV	245	208	0.03%	0.004%
71	11.296	3109	3112	3114	rBV	208	152	0.02%	0.003%
72	11.550	3185	3191	3194	rBV	361	411	0.06%	0.008%
73	11.746	3248	3252	3257	rVB2	496	421	0.06%	0.008%
74	11.807	3260	3271	3293	rBV	297717	503684	75.34%	9.322%
75	11.994	3327	3329	3332	rBV	324	179	0.03%	0.003%
76	12.049	3344	3346	3349	rVB2	317	173	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
 Data File : VU059134.D
 Acq On : 04 Jun 2024 12:20
 Operator : MD/SY
 Sample : P2663-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	12.142	3372	3375	3377	rBV	308	216	0.03%	0.004%
78	12.190	3378	3390	3416	rVV	249808	424689	63.52%	7.860%
79	12.393	3451	3453	3457	rVB2	298	147	0.02%	0.003%
80	12.457	3470	3473	3476	rBV	262	203	0.03%	0.004%
81	12.502	3482	3487	3493	rVB2	321	290	0.04%	0.005%
82	12.766	3566	3569	3574	rVB2	272	209	0.03%	0.004%
83	13.261	3721	3723	3726	rVB2	328	155	0.02%	0.003%
84	13.322	3738	3742	3745	rBV	261	278	0.04%	0.005%
85	13.663	3841	3848	3853	rBV2	354	600	0.09%	0.011%
86	14.055	3967	3970	3973	rVB	334	213	0.03%	0.004%
87	14.074	3973	3976	3982	rBV3	323	321	0.05%	0.006%
88	14.106	3983	3986	3988	rBV2	279	202	0.03%	0.004%
89	14.351	4059	4062	4065	rVV2	327	204	0.03%	0.004%
90	14.528	4115	4117	4120	rBV2	317	183	0.03%	0.003%
91	14.608	4140	4142	4144	rBV2	432	222	0.03%	0.004%
92	14.695	4166	4169	4171	rBV2	249	162	0.02%	0.003%
93	14.714	4171	4175	4178	rVB2	245	184	0.03%	0.003%
94	14.730	4178	4180	4185	rBV2	314	314	0.05%	0.006%
95	14.810	4202	4205	4211	rBV2	339	381	0.06%	0.007%
96	14.843	4212	4215	4218	rBV	423	369	0.06%	0.007%
97	15.074	4284	4287	4289	rBV2	406	292	0.04%	0.005%
98	15.872	4532	4535	4541	rBV4	496	380	0.06%	0.007%
99	16.097	4603	4605	4607	rBV	463	286	0.04%	0.005%
100	16.386	4690	4695	4698	rBV2	795	852	0.13%	0.016%




Sum of corrected areas: 5403442

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
Data File : VU059134.D
Acq On : 04 Jun 2024 12:20
Operator : MD/SY
Sample : P2663-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

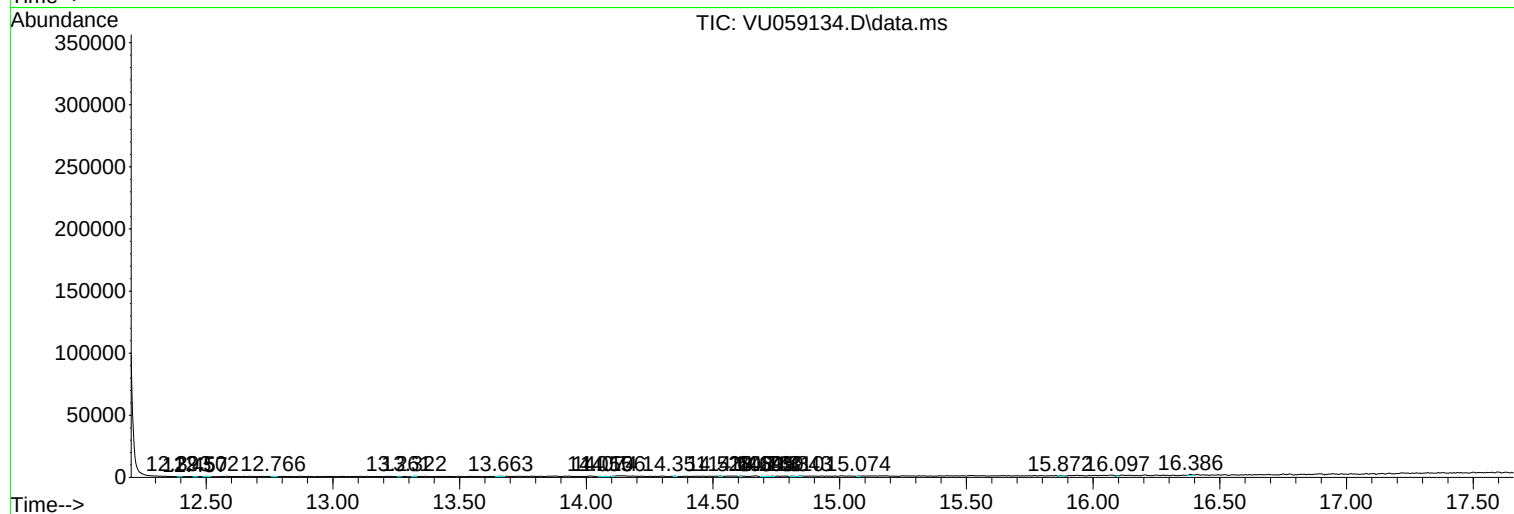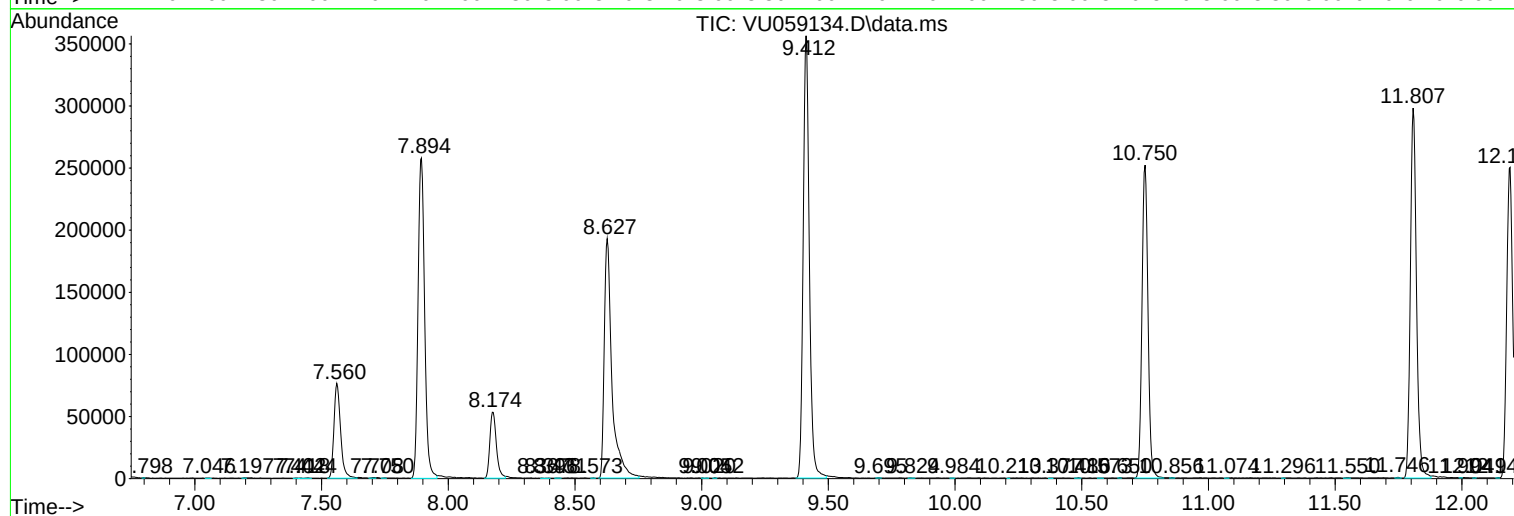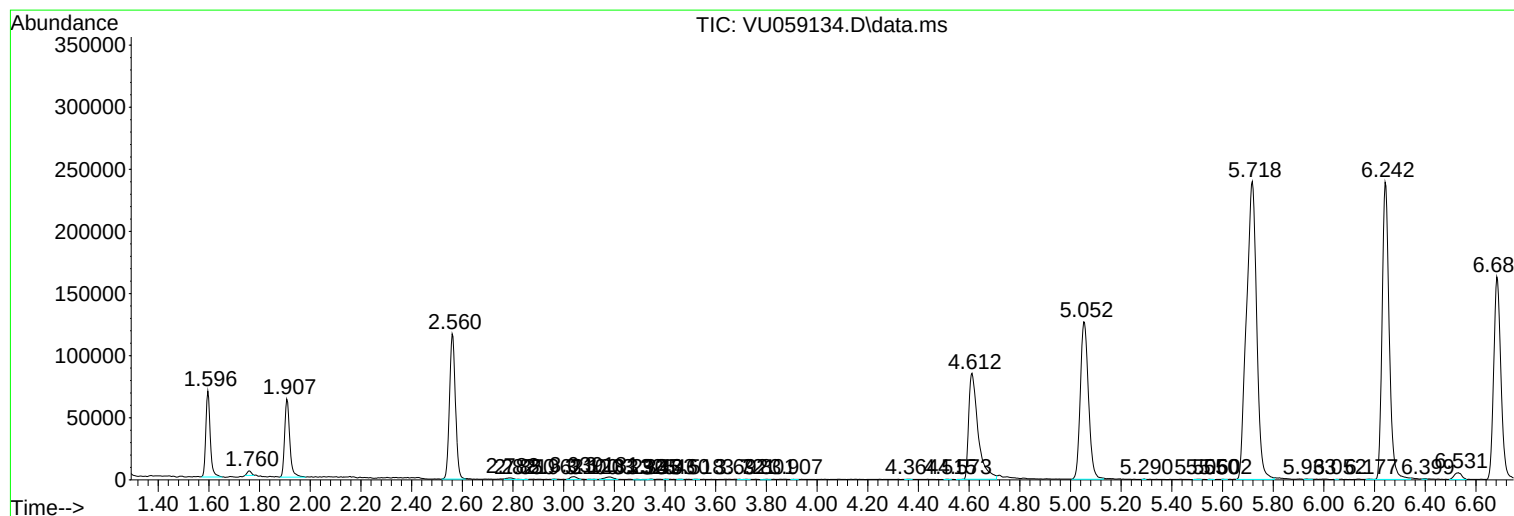

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
Data File : VU059134.D
Acq On : 04 Jun 2024 12:20
Operator : MD/SY
Sample : P2663-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
Data File : VU059134.D
Acq On : 04 Jun 2024 12:20
Operator : MD/SY
Sample : P2663-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc