

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
 Data File : VU059138.D
 Acq On : 04 Jun 2024 13:52
 Operator : MD/SY
 Sample : P2695-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4D61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059138.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	115	rVB	56019	67315	10.56%	1.277%
2	1.682	116	122	130	rVB2	5087	6006	0.94%	0.114%
3	1.759	141	146	153	rVB7	3208	4140	0.65%	0.079%
4	1.907	184	192	206	rBV	50436	67996	10.67%	1.290%
5	2.267	298	304	317	rVB3	3353	5660	0.89%	0.107%
6	2.390	340	342	347	rBV3	586	505	0.08%	0.010%
7	2.560	384	395	405	rBV	86434	141574	22.21%	2.685%
8	2.618	405	413	432	rVB	43671	75406	11.83%	1.430%
9	2.727	444	447	449	rBV2	572	423	0.07%	0.008%
10	2.750	449	454	459	rVB4	1248	1511	0.24%	0.029%
11	2.849	482	485	488	rVV2	317	185	0.03%	0.004%
12	2.949	513	516	520	rBV2	214	222	0.03%	0.004%
13	3.036	535	543	554	rBV3	1919	3151	0.49%	0.060%
14	3.097	559	562	567	rBV2	224	235	0.04%	0.004%
15	3.177	573	587	605	rVV2	9363	22265	3.49%	0.422%
16	3.583	709	713	716	rVV	260	221	0.03%	0.004%
17	3.721	754	756	759	rVV2	285	189	0.03%	0.004%
18	3.840	786	793	795	rBV	394	439	0.07%	0.008%
19	4.267	921	926	928	rBV	199	196	0.03%	0.004%
20	4.467	984	988	992	rBV4	691	764	0.12%	0.014%
21	4.611	1018	1033	1078	rBV2	92560	262680	41.22%	4.982%
22	5.055	1156	1171	1192	rVV	108819	243051	38.14%	4.610%
23	5.206	1215	1218	1221	rVB3	639	410	0.06%	0.008%
24	5.245	1226	1230	1234	rBV2	208	209	0.03%	0.004%
25	5.306	1247	1249	1253	rVB2	367	256	0.04%	0.005%
26	5.415	1280	1283	1286	rVV2	246	213	0.03%	0.004%
27	5.435	1286	1289	1295	rVB2	217	188	0.03%	0.004%
28	5.717	1358	1377	1408	rBV2	195825	554486	87.01%	10.517%
29	5.939	1444	1446	1454	rVB	372	337	0.05%	0.006%
30	6.242	1528	1540	1564	rBV	254472	495202	77.70%	9.393%
31	6.412	1589	1593	1598	rBV4	416	419	0.07%	0.008%
32	6.531	1620	1630	1641	rVB7	5279	10930	1.72%	0.207%
33	6.685	1665	1678	1703	rBV	140676	278930	43.77%	5.291%
34	6.891	1734	1742	1750	rBV7	2240	4366	0.69%	0.083%
35	6.946	1757	1759	1764	rVB3	328	273	0.04%	0.005%
36	6.978	1766	1769	1773	rVB2	255	211	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
 Data File : VU059138.D
 Acq On : 04 Jun 2024 13:52
 Operator : MD/SY
 Sample : P2695-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4D61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	7.045	1786	1790	1792	rBV2	264	185	0.03%	0.004%
38	7.190	1830	1835	1836	rBV	496	315	0.05%	0.006%
39	7.206	1836	1840	1847	rVB3	731	903	0.14%	0.017%
40	7.373	1890	1892	1896	rVB2	466	292	0.05%	0.006%
41	7.512	1932	1935	1939	rVB	442	369	0.06%	0.007%
42	7.560	1939	1950	1974	rBV	66480	121925	19.13%	2.313%
43	7.705	1992	1995	1999	rBV2	421	346	0.05%	0.007%
44	7.756	2008	2011	2017	rVB3	297	241	0.04%	0.005%
45	7.795	2018	2023	2025	rBV3	792	659	0.10%	0.012%
46	7.894	2040	2054	2071	rBV	201029	353648	55.49%	6.708%
47	8.087	2110	2114	2123	rVB4	474	696	0.11%	0.013%
48	8.174	2131	2141	2166	rVV2	45155	79906	12.54%	1.516%
49	8.332	2188	2190	2194	rVB2	323	216	0.03%	0.004%
50	8.454	2225	2228	2232	rBV	268	305	0.05%	0.006%
51	8.473	2232	2234	2238	rVB2	431	260	0.04%	0.005%
52	8.627	2271	2282	2322	rVV	189065	405167	63.58%	7.685%
53	8.785	2322	2331	2348	rVB3	16471	30630	4.81%	0.581%
54	8.904	2365	2368	2371	rBV2	375	311	0.05%	0.006%
55	8.936	2375	2378	2380	rBV	434	244	0.04%	0.005%
56	9.132	2436	2439	2442	rBV2	251	223	0.03%	0.004%
57	9.412	2510	2526	2550	rBV	372293	637291	100.00%	12.088%
58	9.563	2570	2573	2575	rBV2	589	432	0.07%	0.008%
59	9.595	2581	2583	2587	rVB2	434	242	0.04%	0.005%
60	9.701	2606	2616	2625	rBV3	1454	2626	0.41%	0.050%
61	10.103	2734	2741	2747	rBV5	985	1484	0.23%	0.028%
62	10.174	2760	2763	2768	rBV2	209	194	0.03%	0.004%
63	10.251	2778	2787	2789	rBV2	618	913	0.14%	0.017%
64	10.309	2803	2805	2808	rVB3	334	203	0.03%	0.004%
65	10.348	2811	2817	2818	rBV2	1720	1337	0.21%	0.025%
66	10.483	2857	2859	2863	rVB	374	218	0.03%	0.004%
67	10.534	2872	2875	2881	rVB2	253	226	0.04%	0.004%
68	10.566	2881	2885	2893	rBV4	440	614	0.10%	0.012%
69	10.647	2906	2910	2915	rBV2	276	212	0.03%	0.004%
70	10.749	2929	2942	2965	rBV	250361	406355	63.76%	7.707%
71	10.888	2978	2985	2992	rBV3	730	1182	0.19%	0.022%
72	11.010	3020	3023	3029	rBV2	255	248	0.04%	0.005%
73	11.039	3029	3032	3034	rVV	425	251	0.04%	0.005%
74	11.061	3037	3039	3041	rVV2	501	226	0.04%	0.004%
75	11.077	3041	3044	3053	rVB3	425	484	0.08%	0.009%
76	11.206	3081	3084	3089	rVB	351	327	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
 Data File : VU059138.D
 Acq On : 04 Jun 2024 13:52
 Operator : MD/SY
 Sample : P2695-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4D61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.280	3104	3107	3112	rVB	335	291	0.05%	0.006%
78	11.466	3162	3165	3167	rBV2	268	214	0.03%	0.004%
79	11.483	3167	3170	3175	rVV3	527	648	0.10%	0.012%
80	11.508	3175	3178	3185	rVB4	657	725	0.11%	0.014%
81	11.598	3201	3206	3211	rBV2	491	430	0.07%	0.008%
82	11.701	3228	3238	3243	rBV4	1027	1565	0.25%	0.030%
83	11.807	3259	3271	3296	rBV	321278	536092	84.12%	10.168%
84	12.077	3348	3355	3367	rBV8	2808	6210	0.97%	0.118%
85	12.190	3378	3390	3411	rVB	235209	397566	62.38%	7.541%
86	12.527	3487	3495	3507	rBV2	9627	15761	2.47%	0.299%
87	12.669	3532	3539	3546	rBV3	385	679	0.11%	0.013%
88	12.727	3553	3557	3559	rBV	262	209	0.03%	0.004%
89	12.762	3564	3568	3571	rBV	495	469	0.07%	0.009%
90	12.849	3592	3595	3601	rBV3	590	373	0.06%	0.007%
91	12.897	3601	3610	3618	rBV6	3700	5850	0.92%	0.111%
92	12.955	3624	3628	3631	rVB4	504	346	0.05%	0.007%
93	13.035	3650	3653	3655	rBV	337	194	0.03%	0.004%
94	13.923	3926	3929	3935	rBV2	322	275	0.04%	0.005%
95	14.129	3989	3993	3994	rBV2	506	343	0.05%	0.007%
96	14.325	4049	4054	4056	rBV2	399	424	0.07%	0.008%
97	14.547	4119	4123	4124	rBV2	529	380	0.06%	0.007%
98	14.695	4167	4169	4172	rBV	390	209	0.03%	0.004%
99	14.778	4192	4195	4197	rBV3	428	276	0.04%	0.005%
100	15.048	4276	4279	4281	rBV	361	222	0.03%	0.004%




Sum of corrected areas: 5272221

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
Data File : VU059138.D
Acq On : 04 Jun 2024 13:52
Operator : MD/SY
Sample : P2695-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4D61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

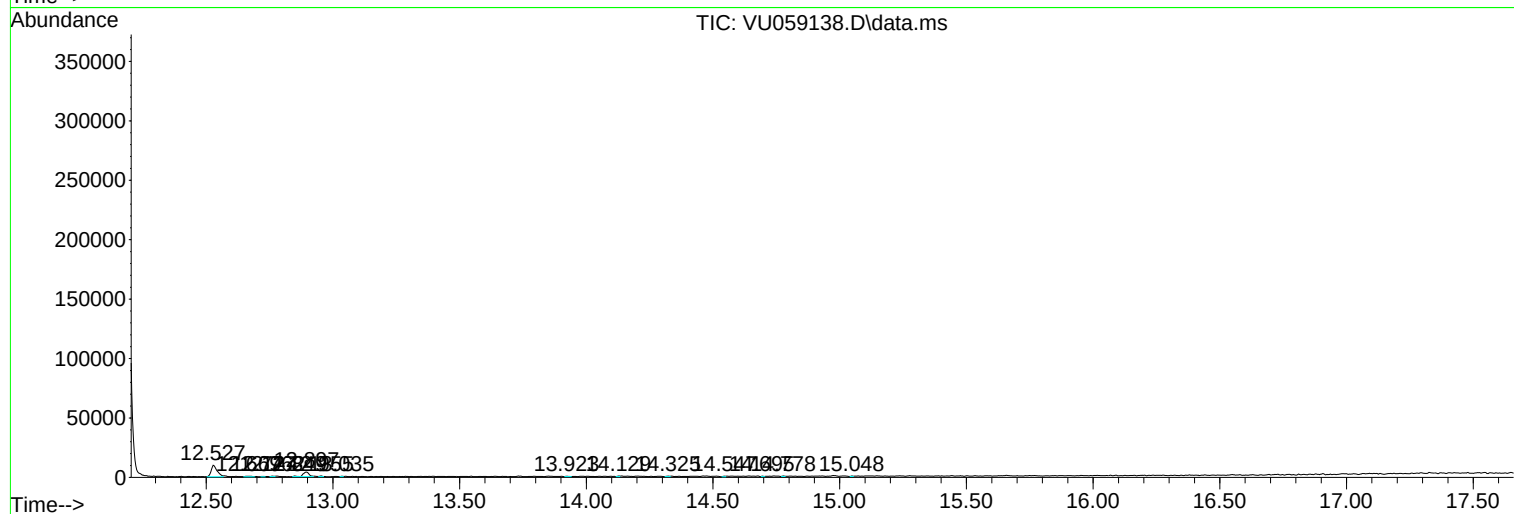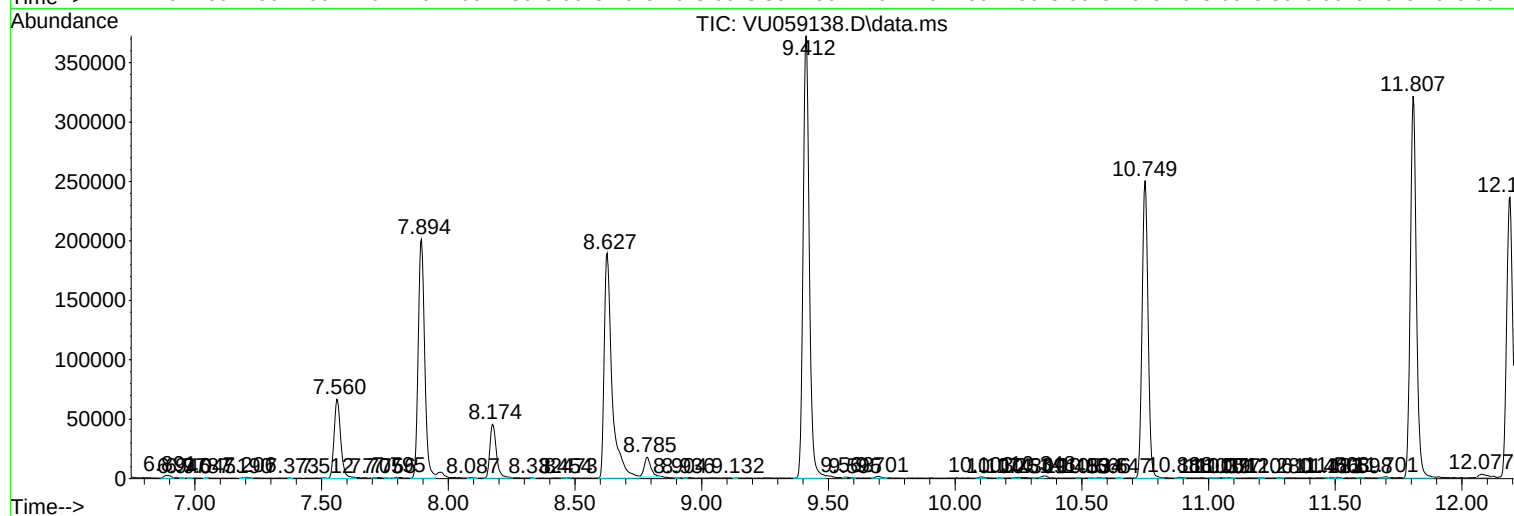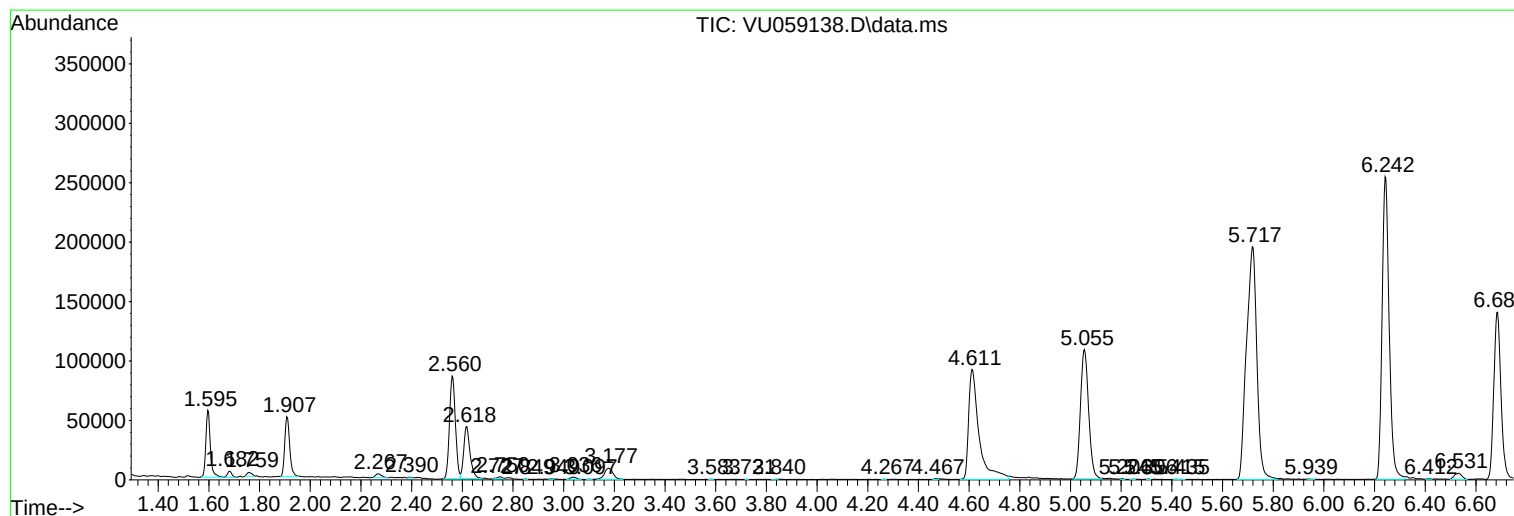

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
Data File : VU059138.D
Acq On : 04 Jun 2024 13:52
Operator : MD/SY
Sample : P2695-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4D61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
Data File : VU059138.D
Acq On : 04 Jun 2024 13:52
Operator : MD/SY
Sample : P2695-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4D61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------