

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
 Data File : VU059139.D
 Acq On : 04 Jun 2024 15:27
 Operator : MD/SY
 Sample : P2695-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059139.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	107	rBV	67137	78890	12.05%	1.450%
2	1.907	184	192	213	rVB	62366	85125	13.00%	1.564%
3	2.258	298	301	304	rBV3	698	676	0.10%	0.012%
4	2.306	313	316	318	rBV3	688	443	0.07%	0.008%
5	2.560	382	395	411	rBV	115521	190826	29.14%	3.507%
6	2.634	416	418	426	rVB4	607	557	0.09%	0.010%
7	2.730	445	448	450	rBV2	260	197	0.03%	0.004%
8	2.785	455	465	470	rBV3	520	825	0.13%	0.015%
9	2.878	489	494	497	rBV2	225	213	0.03%	0.004%
10	2.949	514	516	522	rVB2	206	179	0.03%	0.003%
11	3.039	534	544	554	rVV3	6369	10308	1.57%	0.189%
12	3.119	566	569	572	rVB2	276	178	0.03%	0.003%
13	3.142	572	576	581	rBV2	329	394	0.06%	0.007%
14	3.164	581	583	587	rVB2	319	194	0.03%	0.004%
15	3.187	587	590	592	rBV2	497	283	0.04%	0.005%
16	3.219	597	600	607	rVV	177	219	0.03%	0.004%
17	3.312	626	629	637	rVV2	248	316	0.05%	0.006%
18	3.444	662	670	673	rBV	265	378	0.06%	0.007%
19	3.476	677	680	685	rVB	173	183	0.03%	0.003%
20	3.554	700	704	707	rBV2	259	269	0.04%	0.005%
21	3.788	772	777	782	rVB	356	414	0.06%	0.008%
22	3.820	782	787	790	rBV2	283	244	0.04%	0.004%
23	3.882	803	806	813	rVV2	193	206	0.03%	0.004%
24	3.927	817	820	826	rVB	279	300	0.05%	0.006%
25	3.968	830	833	839	rBV	252	217	0.03%	0.004%
26	4.132	881	884	889	rBV2	304	317	0.05%	0.006%
27	4.238	913	917	923	rBV2	271	297	0.05%	0.005%
28	4.299	932	936	942	rBV2	222	242	0.04%	0.004%
29	4.521	1000	1005	1009	rVB	320	340	0.05%	0.006%
30	4.611	1023	1033	1072	rBV	80197	206117	31.48%	3.788%
31	5.055	1155	1171	1191	rVV	126703	279229	42.64%	5.132%
32	5.190	1209	1213	1218	rVB3	424	435	0.07%	0.008%
33	5.232	1223	1226	1229	rVB2	364	276	0.04%	0.005%
34	5.264	1229	1236	1241	rBV2	425	377	0.06%	0.007%
35	5.438	1286	1290	1295	rVB2	414	428	0.07%	0.008%
36	5.582	1331	1335	1342	rBV2	203	251	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
 Data File : VU059139.D
 Acq On : 04 Jun 2024 15:27
 Operator : MD/SY
 Sample : P2695-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	5.717	1357	1377	1406	rBV2	236592	654778	100.00%	12.034%
38	5.952	1447	1450	1454	rBV2	299	269	0.04%	0.005%
39	6.016	1468	1470	1474	rVB2	299	178	0.03%	0.003%
40	6.036	1474	1476	1479	rBV2	316	186	0.03%	0.003%
41	6.068	1480	1486	1489	rVB2	265	261	0.04%	0.005%
42	6.242	1528	1540	1569	rBV	249422	483874	73.90%	8.893%
43	6.344	1569	1572	1577	rVB2	549	506	0.08%	0.009%
44	6.415	1591	1594	1597	rBV3	330	186	0.03%	0.003%
45	6.528	1620	1629	1642	rVV5	6047	11881	1.81%	0.218%
46	6.682	1664	1677	1701	rBV2	160520	316516	48.34%	5.817%
47	6.978	1763	1769	1771	rBV	196	216	0.03%	0.004%
48	7.026	1780	1784	1788	rBV2	236	260	0.04%	0.005%
49	7.155	1820	1824	1826	rBV2	196	209	0.03%	0.004%
50	7.196	1833	1837	1838	rBV2	328	257	0.04%	0.005%
51	7.364	1886	1889	1894	rVB	262	222	0.03%	0.004%
52	7.393	1894	1898	1901	rBV2	226	202	0.03%	0.004%
53	7.489	1924	1928	1933	rVB2	357	328	0.05%	0.006%
54	7.560	1937	1950	1973	rBV	76586	141461	21.60%	2.600%
55	7.669	1981	1984	1987	rVB3	440	311	0.05%	0.006%
56	7.695	1987	1992	1994	rBV2	277	231	0.04%	0.004%
57	7.711	1994	1997	2000	rVV3	486	467	0.07%	0.009%
58	7.727	2000	2002	2008	rVB3	370	251	0.04%	0.005%
59	7.894	2041	2054	2079	rBV	260302	459619	70.19%	8.447%
60	8.174	2131	2141	2160	rBV2	54821	93344	14.26%	1.716%
61	8.277	2170	2173	2174	rBV2	282	193	0.03%	0.004%
62	8.627	2271	2282	2323	rBV2	183845	394213	60.21%	7.245%
63	8.862	2353	2355	2361	rBV3	300	349	0.05%	0.006%
64	8.885	2361	2362	2367	rVV3	454	281	0.04%	0.005%
65	8.926	2373	2375	2379	rVB	653	294	0.04%	0.005%
66	9.328	2497	2500	2505	rVB2	256	197	0.03%	0.004%
67	9.412	2513	2526	2555	rBV	376315	631901	96.51%	11.613%
68	9.627	2590	2593	2599	rVB2	300	221	0.03%	0.004%
69	9.701	2614	2616	2619	rBV2	280	201	0.03%	0.004%
70	9.933	2685	2688	2692	rVB2	281	226	0.03%	0.004%
71	10.048	2720	2724	2727	rBV2	249	195	0.03%	0.004%
72	10.113	2740	2744	2748	rVB	387	360	0.05%	0.007%
73	10.142	2748	2753	2754	rBV2	311	207	0.03%	0.004%
74	10.174	2759	2763	2766	rBV2	191	190	0.03%	0.003%
75	10.229	2773	2780	2787	rBV2	215	356	0.05%	0.007%
76	10.293	2797	2800	2806	rBV2	228	243	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
 Data File : VU059139.D
 Acq On : 04 Jun 2024 15:27
 Operator : MD/SY
 Sample : P2695-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	10.418	2831	2839	2845	rVB2	343	578	0.09%	0.011%
78	10.450	2845	2849	2851	rBV2	306	269	0.04%	0.005%
79	10.659	2910	2914	2920	rBV2	287	357	0.05%	0.007%
80	10.749	2929	2942	2963	rBV	244224	407121	62.18%	7.482%
81	10.865	2975	2978	2982	rVB2	249	178	0.03%	0.003%
82	10.888	2982	2985	2988	rBV2	421	377	0.06%	0.007%
83	11.074	3038	3043	3044	rBV	284	235	0.04%	0.004%
84	11.505	3172	3177	3180	rBV	394	336	0.05%	0.006%
85	11.579	3195	3200	3203	rBV	234	195	0.03%	0.004%
86	11.807	3259	3271	3295	rBV	322567	543964	83.08%	9.997%
87	12.013	3332	3335	3337	rBV2	242	178	0.03%	0.003%
88	12.190	3376	3390	3409	rBV	251838	427392	65.27%	7.855%
89	12.865	3597	3600	3604	rBV	233	188	0.03%	0.003%
90	13.129	3679	3682	3685	rBV	432	331	0.05%	0.006%
91	13.312	3737	3739	3743	rVB	358	239	0.04%	0.004%
92	13.344	3743	3749	3754	rBV2	311	491	0.07%	0.009%
93	13.971	3939	3944	3947	rBV2	339	396	0.06%	0.007%
94	14.042	3963	3966	3968	rBV	306	207	0.03%	0.004%
95	14.585	4133	4135	4137	rBV	368	179	0.03%	0.003%
96	14.717	4172	4176	4180	rBV3	496	500	0.08%	0.009%
97	14.778	4191	4195	4197	rBV2	349	261	0.04%	0.005%
98	14.794	4197	4200	4203	rBV2	378	287	0.04%	0.005%
99	15.180	4317	4320	4322	rBV	442	308	0.05%	0.006%
100	17.100	4915	4917	4919	rBV	966	599	0.09%	0.011%




Sum of corrected areas: 5441149

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
Data File : VU059139.D
Acq On : 04 Jun 2024 15:27
Operator : MD/SY
Sample : P2695-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

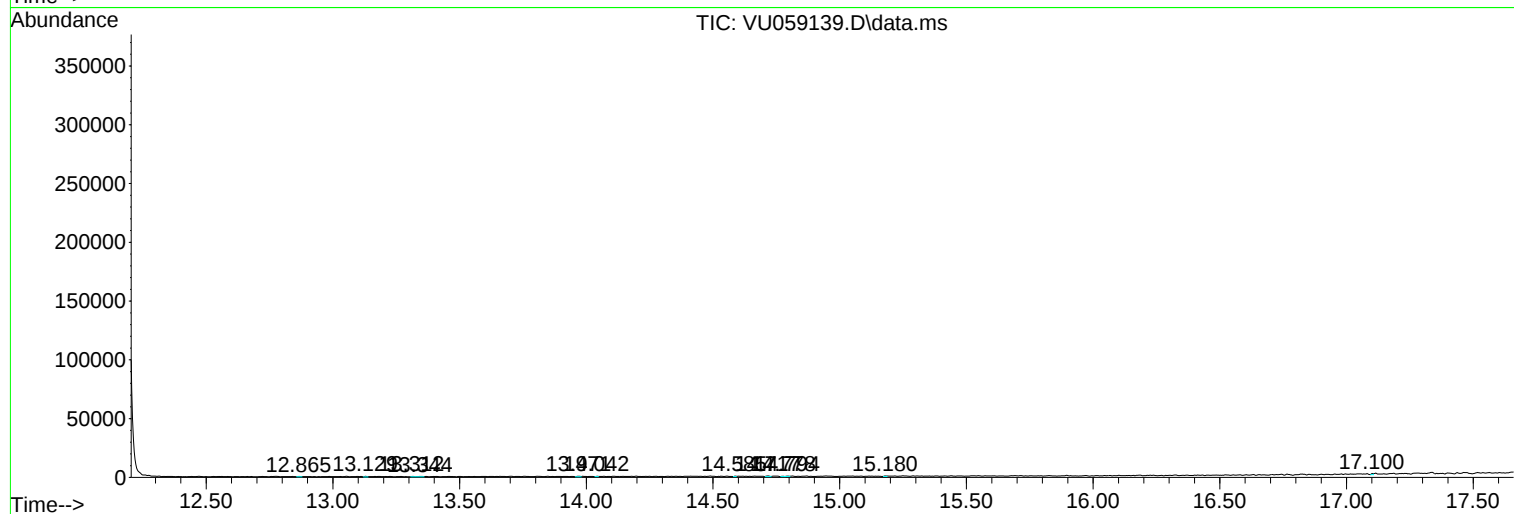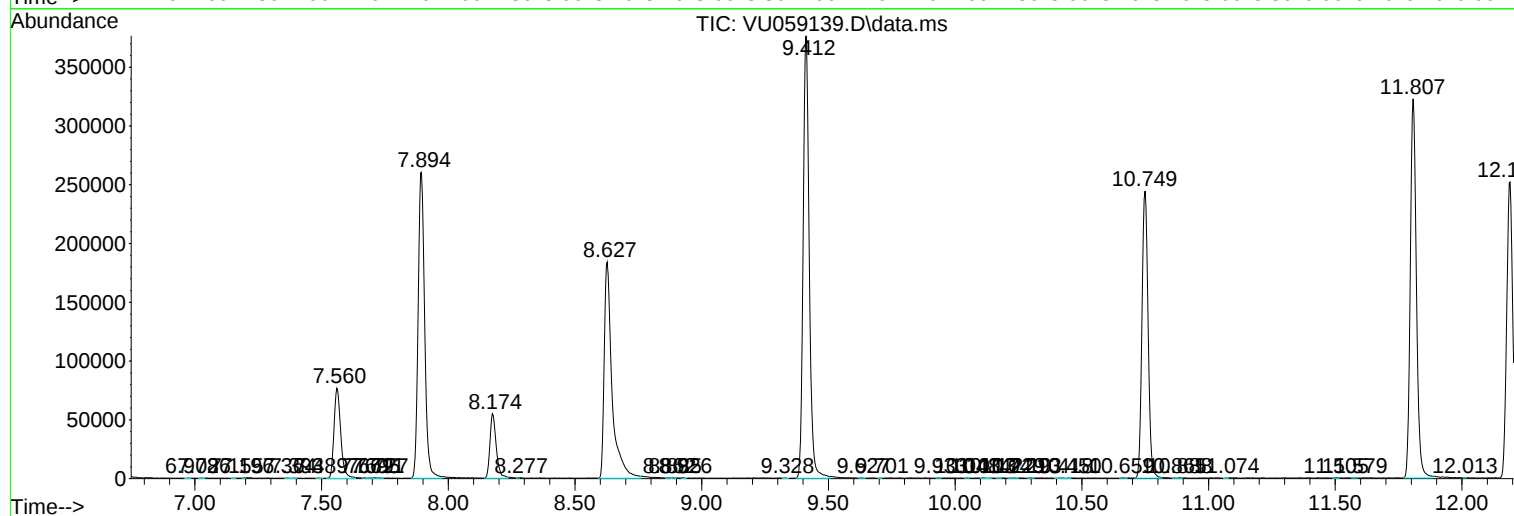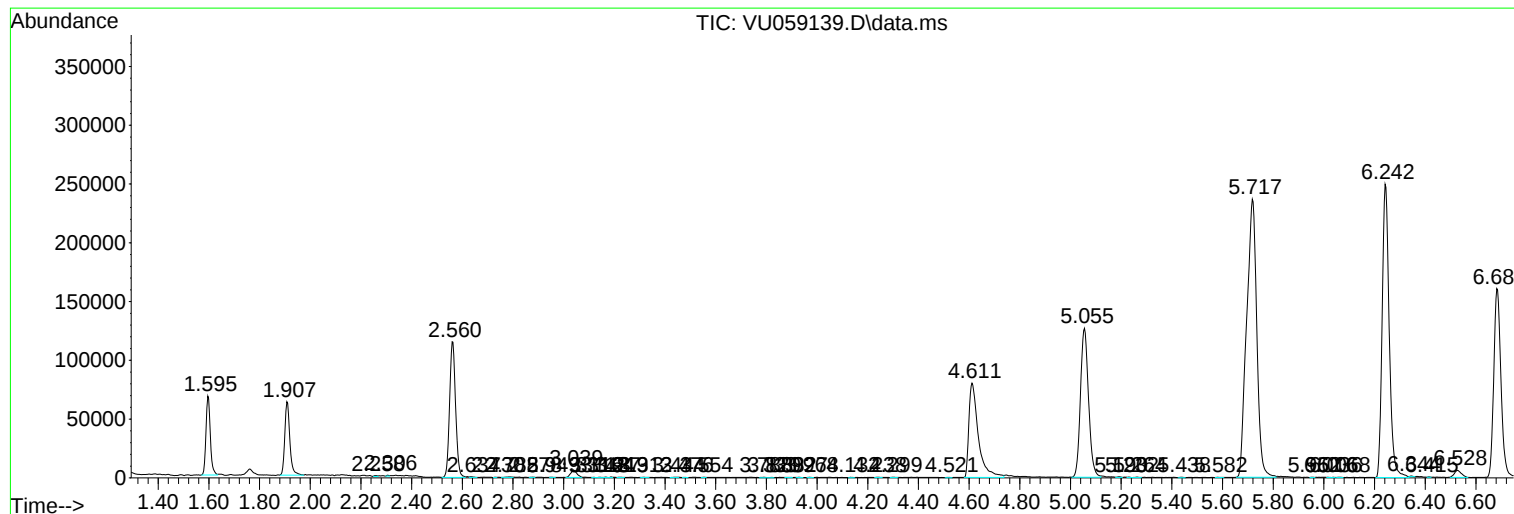

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
Data File : VU059139.D
Acq On : 04 Jun 2024 15:27
Operator : MD/SY
Sample : P2695-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
Data File : VU059139.D
Acq On : 04 Jun 2024 15:27
Operator : MD/SY
Sample : P2695-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------