


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060424\
Data File : VU059130.D
Acq On : 04 Jun 2024 09:35
Operator : MD/SY
Sample : BFB059
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB059

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Title : VOC Analysis
Last Update : Wed Jun 05 05:30:09 2024

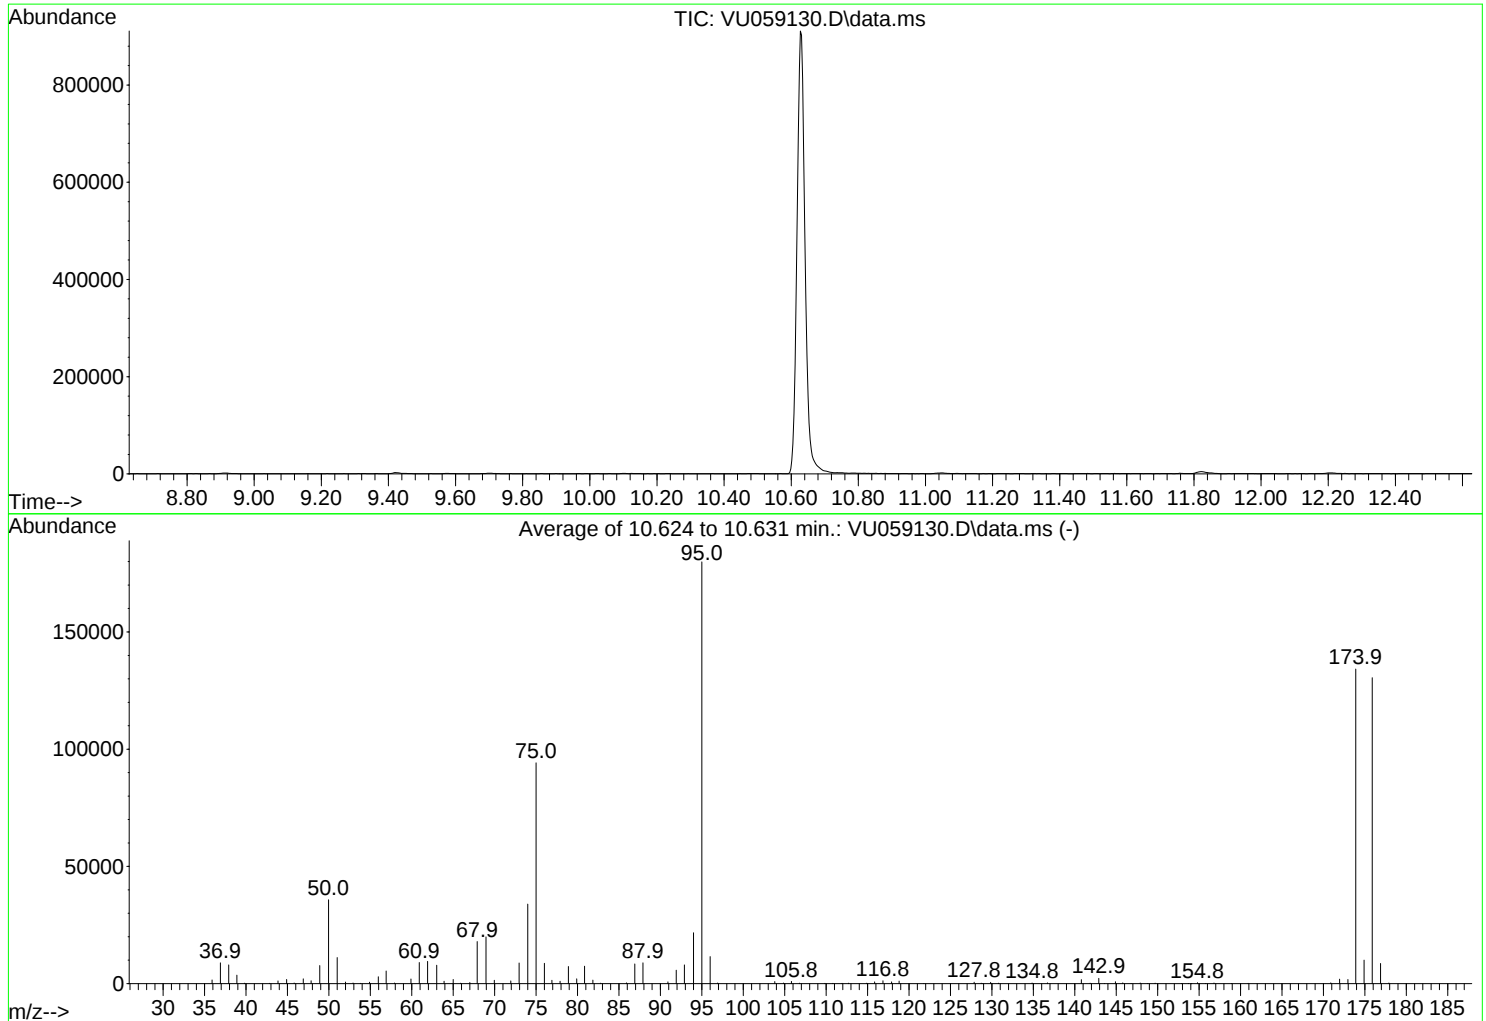

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.9	35744	PASS
75	95	30	80	52.4	94213	PASS
95	95	100	100	100.0	179904	PASS
96	95	5	9	6.4	11569	PASS
173	174	0.00	2	1.3	1780	PASS
174	95	50	120	74.6	134165	PASS
175	174	5	9	7.5	10063	PASS
176	174	95	101	97.3	130483	PASS
177	176	5	9	6.6	8571	PASS

m/z	Abundance
40.00	132.0
43.80	241.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

m/z	Abundance
35.90	1479.0
36.90	8558.0
37.90	7842.0
38.90	3545.0
39.80	317.0
42.90	175.0
43.90	1311.0
44.90	1689.0
45.90	348.0
46.90	2022.0
47.90	1280.0
48.90	7460.0
50.00	34376.0
51.00	11015.0
52.00	668.0
52.90	310.0
53.80	205.0
54.90	579.0
55.90	2681.0
56.90	4932.0
57.90	273.0
59.90	1804.0
60.90	8504.0
61.90	8767.0
63.00	7710.0
63.90	1004.0
65.00	1685.0
65.90	221.0
67.00	508.0
67.90	17560.0
69.00	19160.0
69.90	1318.0
71.90	1074.0
73.00	8467.0
74.00	32352.0
75.00	90472.0
76.00	8167.0
76.90	1326.0
77.90	1006.0
78.90	7072.0
79.90	2025.0
80.80	7304.0
81.80	1487.0
82.80	177.0
85.90	352.0
86.90	8377.0
87.90	8122.0
90.90	731.0
91.90	5656.0
92.90	7486.0
94.00	20896.0
95.00	169856.0
96.00	11062.0
96.90	261.0
103.80	829.0
104.90	249.0
105.80	914.0
106.80	196.0
109.90	111.0
110.80	125.0
112.70	203.0
115.00	218.0
115.80	782.0
116.90	1108.0
117.90	692.0
118.80	1059.0
121.80	117.0
127.90	514.0
128.70	295.0
129.80	514.0
130.70	221.0
134.90	268.0
136.70	362.0
140.80	1651.0
141.90	170.0
142.90	2302.0
144.90	869.0
145.80	291.0
147.90	269.0
149.70	263.0
152.90	114.0
153.70	123.0
154.80	378.0
156.80	241.0
160.90	169.0
170.90	322.0
171.90	1858.0
173.00	1760.0
173.90	124352.0
174.90	9794.0
175.90	120280.0
176.90	8046.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

177.90

229.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

m/z	Abundance
35.90	1629.0
36.90	9137.0
37.90	8250.0
38.90	3717.0
39.80	277.0
42.90	173.0
43.90	1442.0
44.90	1870.0
45.80	262.0
46.90	2093.0
47.90	1309.0
48.90	7952.0
50.00	36784.0
51.00	11400.0
52.00	668.0
52.90	298.0
53.80	169.0
54.90	657.0
55.90	3023.0
56.90	5625.0
57.90	342.0
59.90	2040.0
60.90	9208.0
61.90	9758.0
63.00	8143.0
63.90	1040.0
65.00	1793.0
65.90	200.0
67.00	522.0
67.90	18360.0
69.00	20488.0
69.90	1491.0
71.90	1205.0
73.00	9182.0
74.00	35136.0
75.00	97256.0
76.00	8970.0
76.90	1485.0
77.90	1085.0
78.90	7563.0
79.90	2120.0
80.90	7716.0
81.80	1575.0
82.80	188.0
85.90	369.0
86.90	8633.0
87.90	9264.0
90.90	793.0
91.90	5975.0
92.90	8176.0
94.00	22368.0
95.00	185792.0
96.00	11903.0
96.90	269.0
103.80	938.0
104.90	275.0
105.80	952.0
106.80	199.0
109.80	132.0
110.80	123.0
111.90	162.0
112.70	187.0
114.90	212.0
115.90	740.0
116.90	1247.0
117.90	753.0
118.80	1184.0
121.80	127.0
127.80	660.0
128.70	293.0
129.80	558.0
130.80	236.0
134.80	297.0
136.70	346.0
140.80	1778.0
141.80	184.0
142.90	2354.0
143.60	126.0
144.90	843.0
145.80	332.0
146.80	103.0
147.90	287.0
148.80	118.0
149.70	255.0
152.90	123.0
154.00	105.0
154.80	415.0
155.80	126.0
156.80	301.0
158.90	118.0
160.90	184.0
170.90	376.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

171.90	1987.0
173.00	1830.0
173.90	138048.0
174.90	10335.0
175.90	134912.0
176.90	8811.0
177.90	280.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

m/z	Abundance
35.90	1589.0
36.90	8950.0
37.90	7950.0
38.90	3541.0
40.00	272.0
42.80	142.0
43.90	1504.0
44.90	1787.0
45.70	163.0
46.90	1974.0
47.80	1191.0
48.90	7735.0
49.90	36072.0
51.00	10953.0
52.00	664.0
52.90	241.0
53.80	124.0
54.90	720.0
56.00	3128.0
56.90	5595.0
57.90	291.0
59.90	2073.0
60.90	9355.0
61.90	9889.0
63.00	7628.0
63.90	1034.0
65.00	1765.0
65.90	168.0
67.00	470.0
67.90	18040.0
68.90	20232.0
70.00	1584.0
72.00	1191.0
72.90	8801.0
74.00	34224.0
75.00	94912.0
76.00	8887.0
76.90	1440.0
77.90	973.0
78.90	7188.0
79.90	1993.0
80.90	7374.0
81.90	1555.0
82.80	178.0
85.90	357.0
86.90	8123.0
87.90	9199.0
90.90	764.0
91.90	5634.0
92.90	8385.0
94.00	21864.0
95.00	184064.0
96.00	11743.0
96.90	255.0
103.80	888.0
104.80	300.0
105.80	955.0
106.80	207.0
109.80	139.0
110.80	142.0
111.90	204.0
112.70	179.0
114.80	214.0
115.90	655.0
116.80	1355.0
117.90	747.0
118.80	1150.0
127.80	782.0
128.90	264.0
129.90	601.0
130.90	247.0
134.80	343.0
136.70	279.0
140.80	1758.0
141.80	201.0
142.90	2200.0
143.60	120.0
144.90	750.0
145.80	333.0
146.80	104.0
147.90	340.0
148.80	119.0
149.70	191.0
154.80	405.0
155.80	136.0
156.80	349.0
158.90	170.0
160.90	166.0
170.90	340.0
172.00	1981.0
172.90	1750.0
173.90	140096.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

174.90	10059.0
175.90	136256.0
176.90	8855.0
177.90	260.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059