

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060620\
 Data File : VU038616.D
 Acq On : 06 Jun 2020 14:58
 Operator : SY/MD
 Sample : L2906-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG6

Quant Time: Jun 07 05:16:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sun Jun 07 04:01:21 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	312843	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	309512	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	148797	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	66119	3.27	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	65.40%
7) Chloroethane-d5	1.93	69	63627	4.09	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.80%
11) 1,1-Dichloroethene-d2	2.59	63	115137	2.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.80%#
20) 2-Butanone-d5	4.67	46	342384	55.66	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.32%
24) Chloroform-d	5.10	84	181308	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
26) 1,2-Dichloroethane-d4	5.74	65	107047	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.20%
32) Benzene-d6	5.76	84	354562	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.80%
36) 1,2-Dichloropropane-d6	6.72	67	112719	4.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.80%
41) Toluene-d8	7.92	98	296496	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.60%
43) trans-1,3-Dichloropropene-	8.20	79	45356	4.44	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.80%
46) 2-Hexanone-d5	8.65	63	293010	58.06	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	116.12%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	104752	5.19	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.80%
64) 1,2-Dichlorobenzene-d4	12.20	152	130659	5.09	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.80%


Target Compounds					Ovalue
13) Acetone	2.68	43	19807	4.921 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060620\
Data File : VU038616.D
Acq On : 06 Jun 2020 14:58
Operator : SY/MD
Sample : L2906-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AG6

Quant Time: Jun 07 05:16:33 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun Jun 07 04:01:21 2020
Response via : Initial Calibration

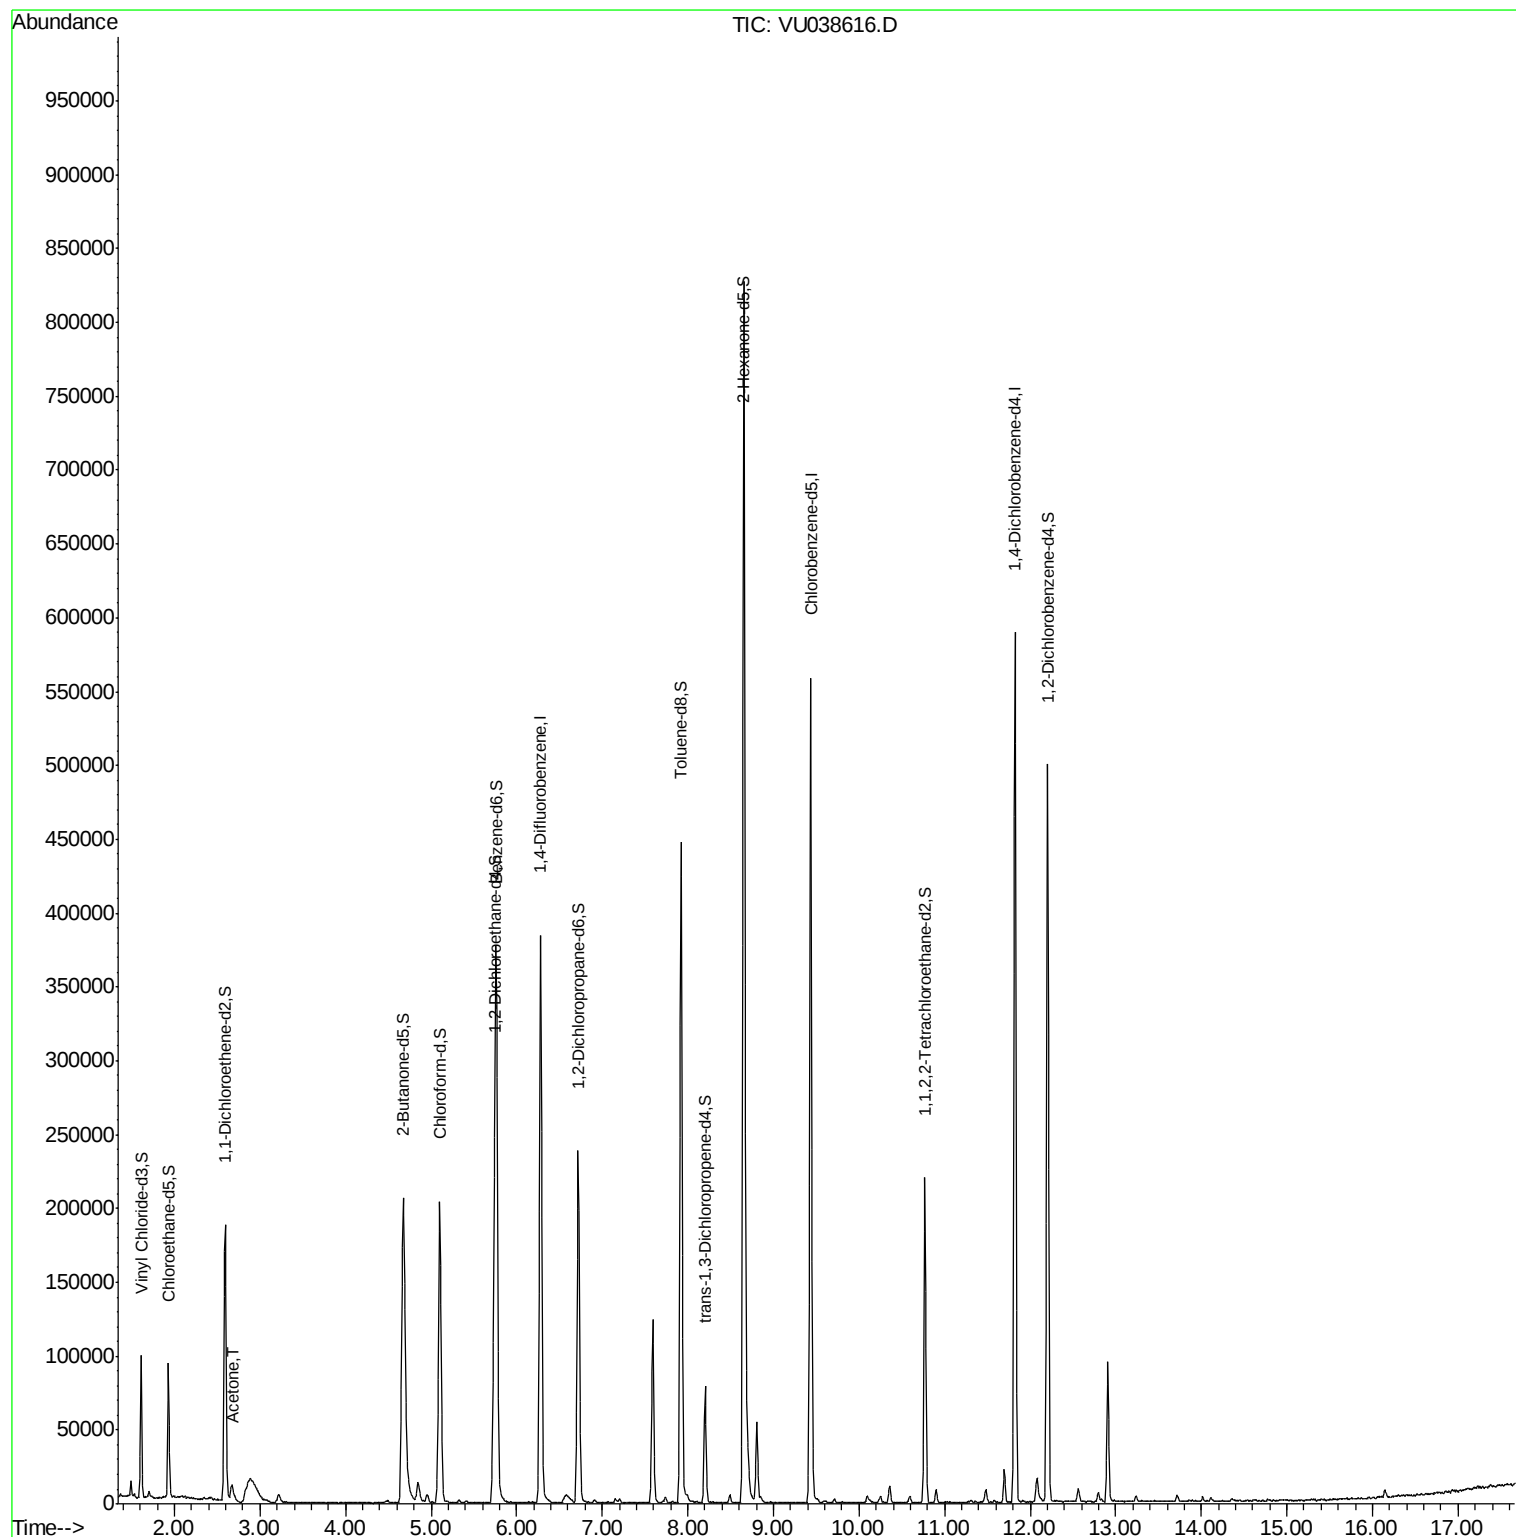

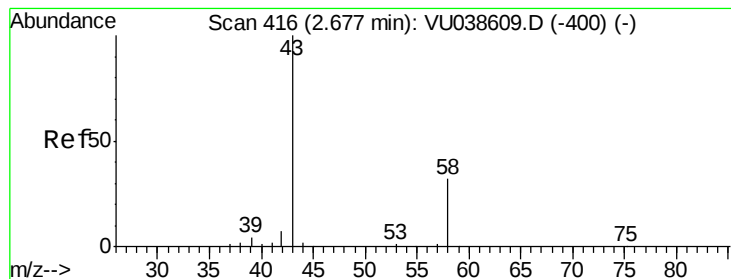

#13
 Acetone
 Concen: 4.921 ug/L
 RT: 2.68 min Scan# 416
 Delta R.T. 0.00 min
 Lab File: VU038616.D
 Acq: 06 Jun 2020 14:58

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG6

Tot Ion: 43 Resp: 19807
 Ion Ratio Lower Upper
 43 100
 58 26.1 0.0 65.6

