

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060620\
 Data File : VU038636.D
 Acq On : 06 Jun 2020 23:49
 Operator : SY/MD
 Sample : L2912-07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9D52

Quant Time: Jun 08 03:18:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 08 02:53:04 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	306487	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	308508	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	147969	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	58256	2.94	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	58.80%
7) Chloroethane-d5	1.93	69	61451	4.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.60%
11) 1,1-Dichloroethene-d2	2.59	63	107027	2.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	54.80%#
20) 2-Butanone-d5	4.68	46	336577	55.86	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.72%
24) Chloroform-d	5.10	84	175874	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
26) 1,2-Dichloroethane-d4	5.74	65	104114	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.40%
32) Benzene-d6	5.76	84	339919	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.20%
36) 1,2-Dichloropropane-d6	6.72	67	110901	4.68	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.60%
41) Toluene-d8	7.92	98	281191	4.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.40%
43) trans-1,3-Dichloropropene-	8.20	79	41431	4.07	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.40%
46) 2-Hexanone-d5	8.65	63	278574	55.38	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	110.76%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	100073	4.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.60%
64) 1,2-Dichlorobenzene-d4	12.20	152	124253	4.87	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.40%


Target Compounds					Ovalue
13) Acetone	2.68	43	28690	7.275 ug/L	100
30) Cyclohexane	5.43	56	7335	0.214 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060620\
Data File : VU038636.D
Acq On : 06 Jun 2020 23:49
Operator : SY/MD
Sample : L2912-07
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9D52

Quant Time: Jun 08 03:18:26 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 08 02:53:04 2020
Response via : Initial Calibration

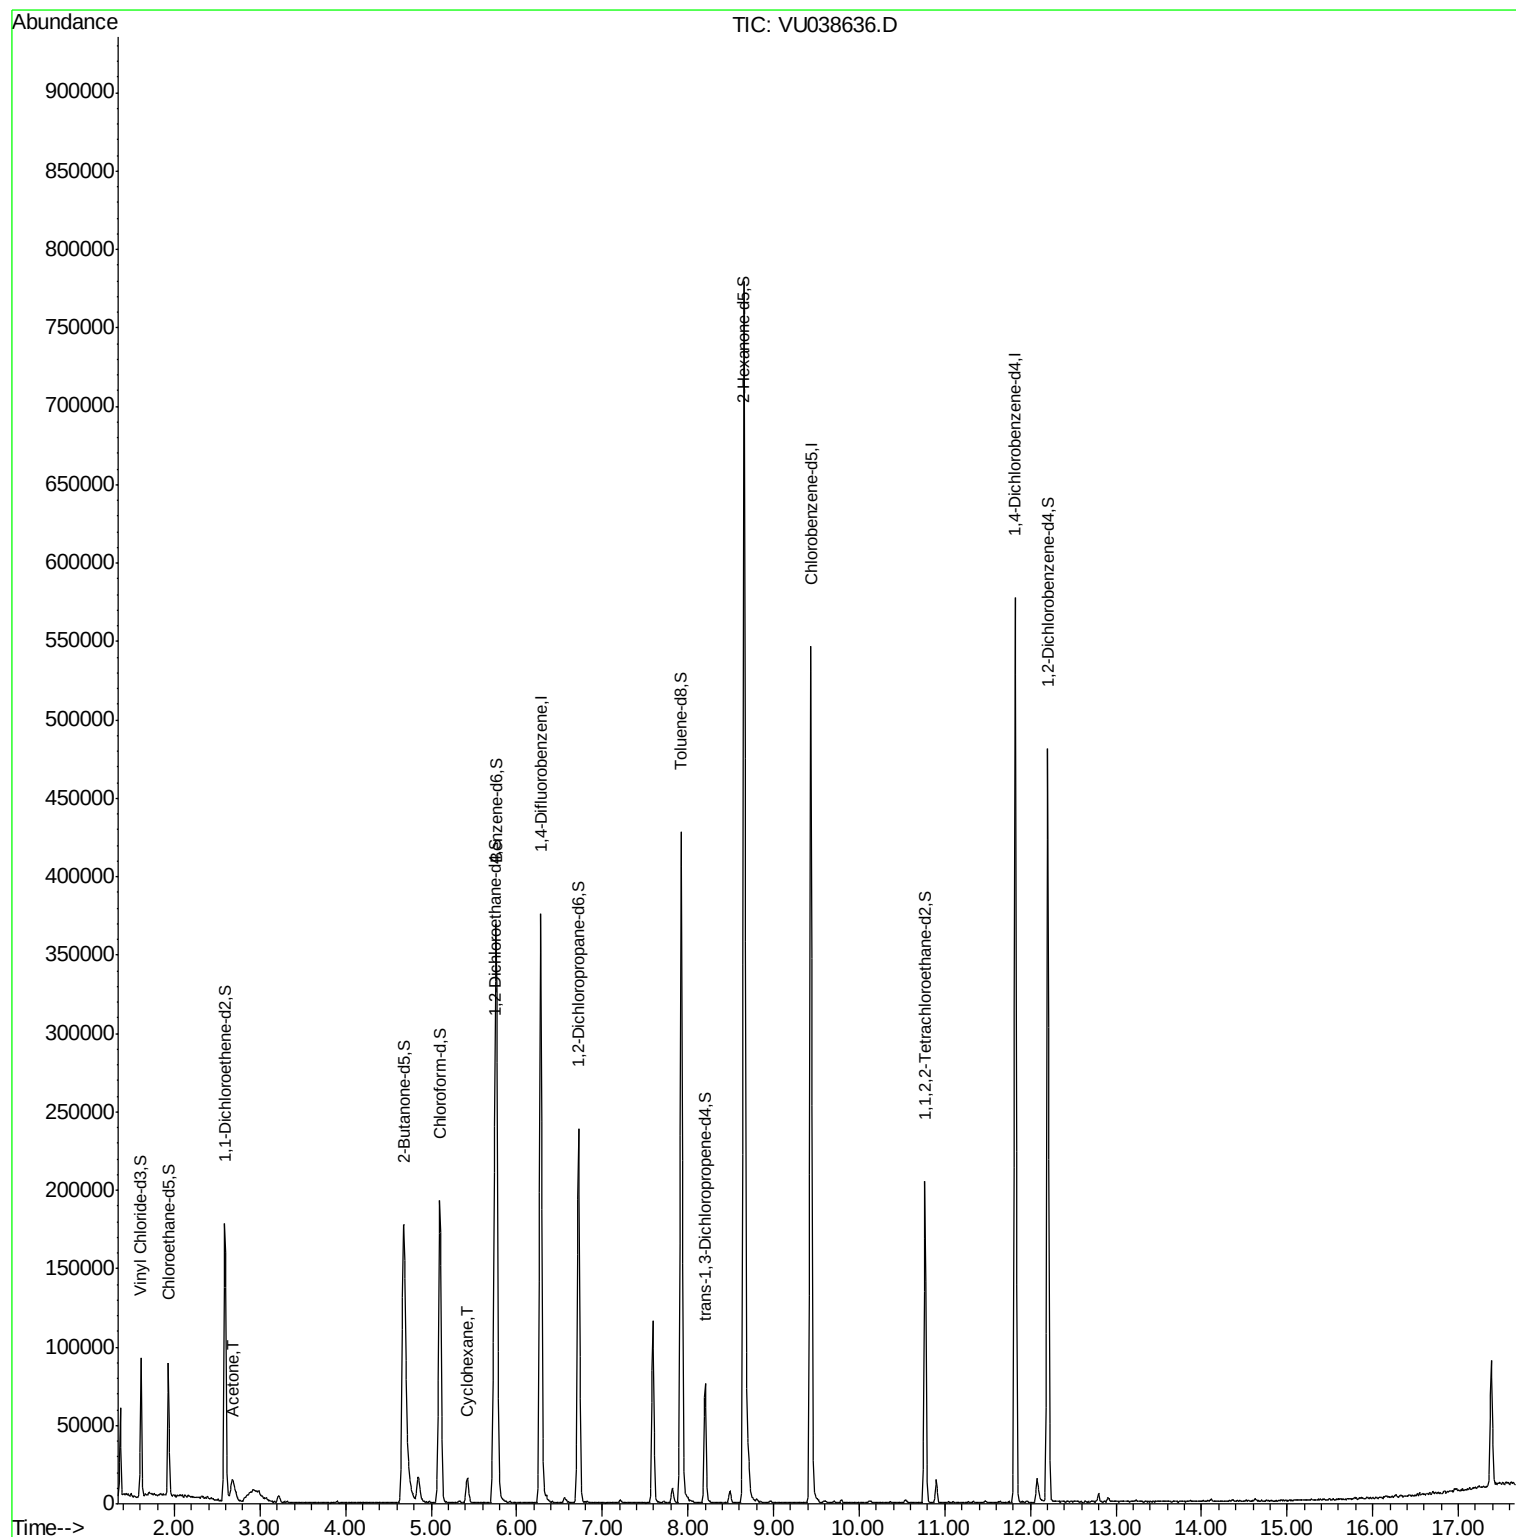

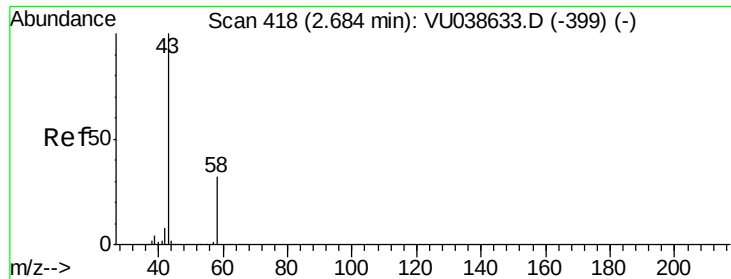

#13

Acetone

Concen: 7.275 ug/L

RT: 2.68 min Scan# 417

Delta R.T. -0.00 min

Lab File: VU038636.D

Acq: 06 Jun 2020 23:49

Instrument :

MSVOA_U

ClientSampleId :


F9D52

Tot Ion: 43 Resp: 28690

Ion Ratio Lower Upper




43 100

58 32.8 0.0 65.6

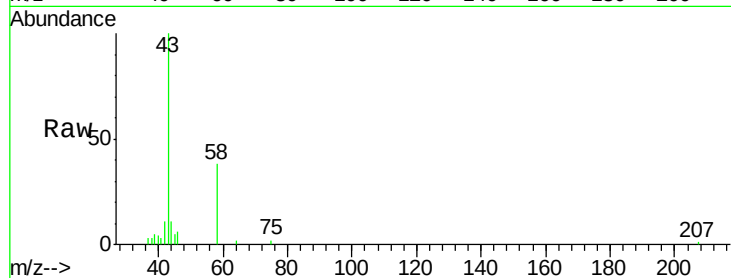

Abundance Ion 43.05 (42.75 to 43.75): VU038636.D (-325) (-)

Ion 58.05 (57.75 to 58.75): VU038636.D (-325) (-)

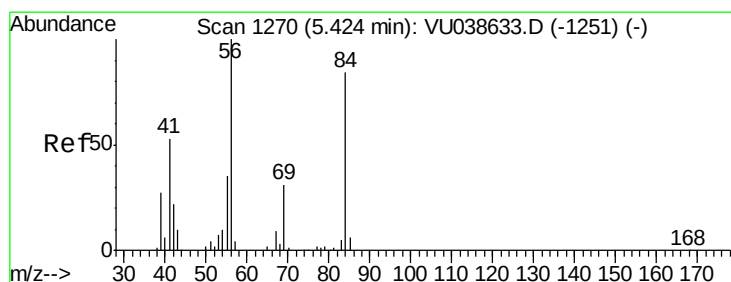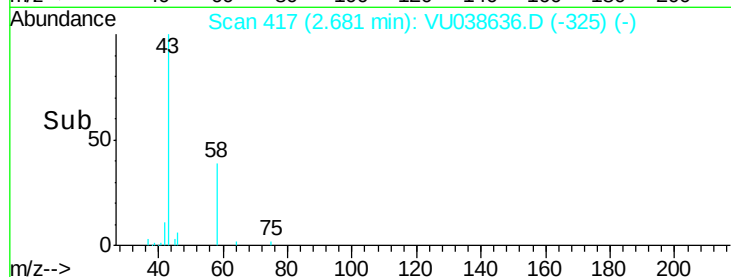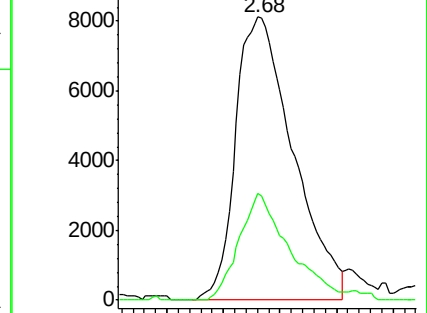

#30

Cyclohexane

Concen: 0.214 ug/L

RT: 5.43 min Scan# 1271

Delta R.T. 0.00 min

Lab File: VU038636.D

Acq: 06 Jun 2020 23:49


Tgt Ion: 56 Resp: 7335

Ion Ratio Lower Upper

56 100

69 31.3 24.2 36.4

84 89.3 70.8 106.2

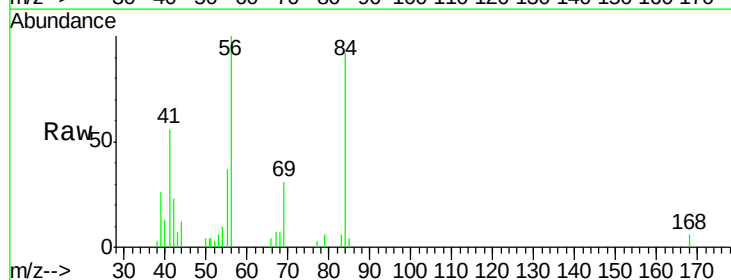

Abundance Ion 56.10 (55.80 to 56.80): VU038636.D (-1177) (-)

Ion 69.15 (68.85 to 69.85): VU038636.D (-1177) (-)

Ion 84.15 (83.85 to 84.85): VU038636.D (-1177) (-)

