


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU060620\
 Data File : VU038608.D
 Acq On : 06 Jun 2020 10:13
 Operator : SY/MD
 Sample : BFB09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB09

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Jun 08 02:53:04 2020

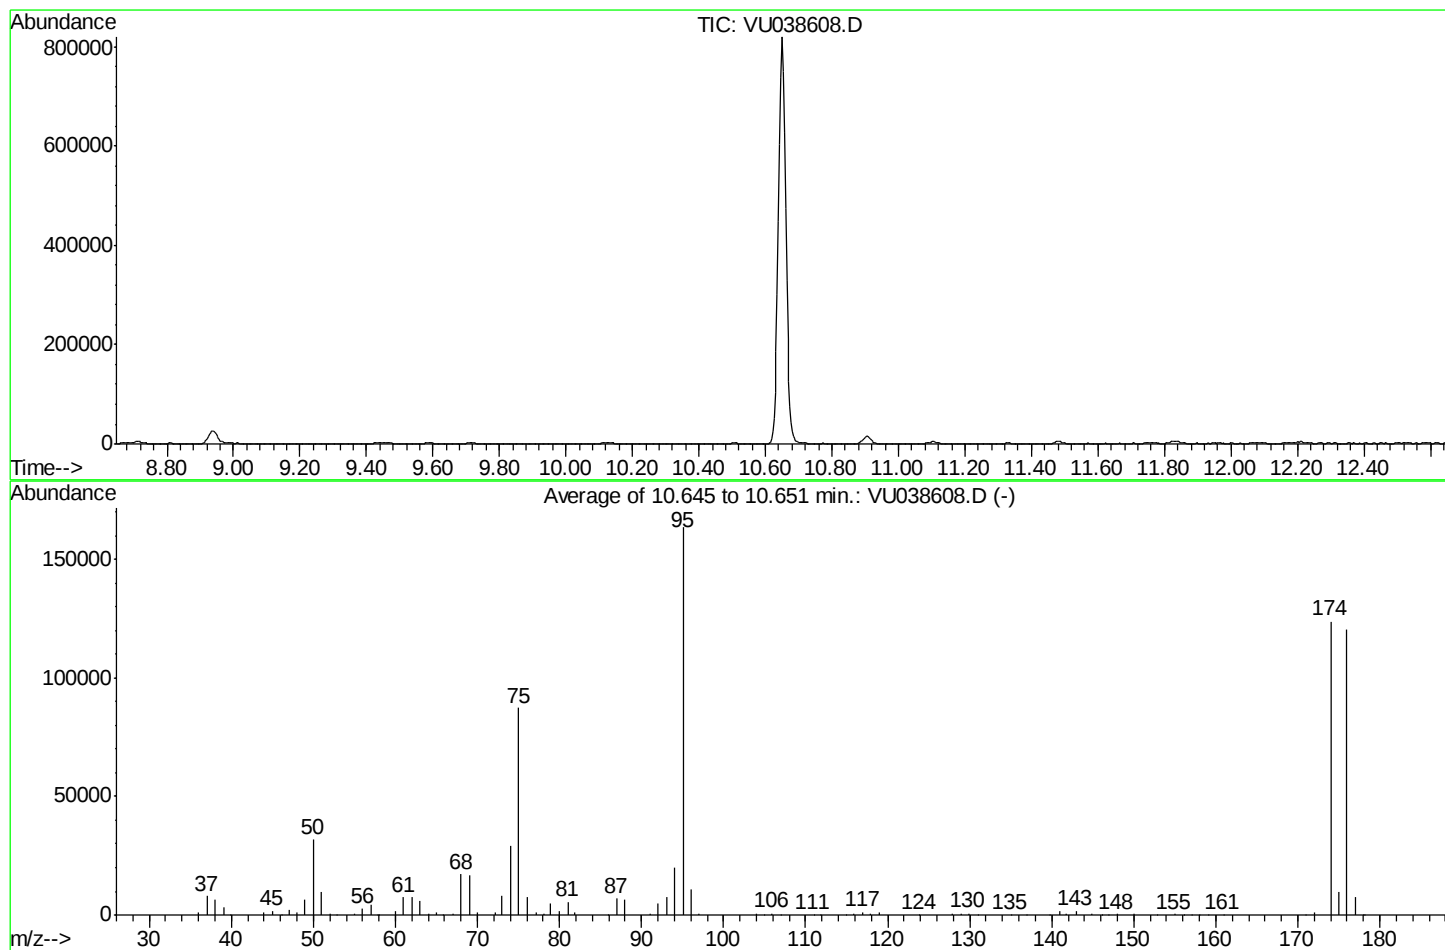

AutoFind: Scans 2894, 2895, 2896; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	31712	PASS
75	95	30	80	53.5	87458	PASS
95	95	100	100	100.0	163541	PASS
96	95	5	9	6.7	11031	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.7	123872	PASS
175	174	5	9	8.0	9910	PASS
176	174	95	101	97.3	120466	PASS
177	176	5	9	6.4	7768	PASS

m/z	Abundance
36.00	1247.0
37.00	7744.0
38.00	6258.0
39.00	2925.0
39.90	331.0
44.00	1582.0
45.00	1663.0
46.00	205.0
47.00	2232.0
47.90	1083.0
49.00	6254.0
50.00	30232.0
51.00	9089.0
52.00	355.0
52.90	109.0
55.00	313.0
56.00	2365.0
57.10	3956.0
57.90	181.0
58.10	185.0
60.00	1395.0
61.00	6910.0
62.00	6955.0
63.00	5748.0
64.00	770.0
65.00	1009.0
65.90	115.0
67.10	716.0
68.00	16096.0
69.00	15892.0
70.00	1248.0
72.10	1015.0
73.00	7281.0
74.00	27368.0
75.00	82184.0
76.10	7064.0
77.10	839.0
78.00	516.0
78.90	4656.0
79.90	1565.0
81.00	5081.0
81.90	1026.0
86.00	183.0
87.00	6525.0
88.00	6361.0
91.00	564.0
92.00	4657.0
93.00	6803.0
94.00	18992.0
95.10	153984.0
96.00	10553.0
97.00	290.0
103.90	571.0
105.00	168.0
105.90	715.0
107.00	156.0
110.90	146.0
111.80	107.0
115.00	184.0
115.90	651.0
117.00	1131.0
117.90	577.0
119.00	868.0
123.90	138.0
127.90	496.0
128.90	322.0
129.80	594.0
131.00	160.0
135.00	276.0
136.90	244.0
139.70	100.0
141.00	1525.0
141.80	294.0
143.00	1825.0
145.00	292.0
146.00	200.0
147.00	141.0
148.00	401.0
150.00	309.0
152.80	128.0
154.90	379.0
156.10	134.0
157.10	247.0
159.10	193.0
161.00	255.0
171.00	172.0
172.10	1007.0
174.00	112944.0
175.00	9359.0
176.00	109520.0
177.00	7121.0
177.90	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
36.00	1282.0
37.00	8388.0
38.00	6520.0
39.00	3208.0
39.90	433.0
44.00	1785.0
45.00	1798.0
46.10	220.0
47.00	2250.0
47.90	1149.0
49.00	6881.0
50.00	32816.0
51.00	10242.0
52.00	386.0
52.90	150.0
55.00	347.0
56.00	2580.0
57.10	4337.0
58.00	212.0
60.10	1674.0
61.00	7771.0
62.00	7597.0
63.00	6234.0
64.00	670.0
65.00	1111.0
65.80	156.0
67.10	674.0
68.00	17648.0
69.00	17176.0
70.00	1314.0
72.10	1060.0
73.00	8272.0
74.00	29872.0
75.00	90280.0
76.10	7792.0
77.10	904.0
78.90	5172.0
79.90	1717.0
81.00	5683.0
81.90	1175.0
85.90	269.0
87.00	7214.0
88.00	6674.0
91.00	616.0
92.00	5027.0
93.10	7673.0
94.00	20840.0
95.10	168768.0
96.00	11262.0
97.10	332.0
104.00	669.0
105.00	205.0
105.90	798.0
107.00	189.0
111.00	172.0
111.80	140.0
115.00	211.0
115.90	712.0
117.00	1243.0
117.90	506.0
119.00	938.0
123.80	104.0
127.90	539.0
128.90	382.0
129.90	625.0
131.00	152.0
135.00	287.0
136.90	253.0
139.70	107.0
141.00	1766.0
141.80	294.0
143.00	1981.0
144.90	310.0
146.10	192.0
147.00	130.0
148.00	453.0
150.00	365.0
152.80	111.0
155.00	347.0
156.10	195.0
157.10	293.0
159.00	185.0
160.90	247.0
171.00	230.0
172.10	1118.0
174.00	127344.0
175.10	10190.0
176.00	124016.0
177.00	8077.0
178.10	220.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
36.00	1224.0
37.00	8151.0
38.00	6605.0
39.10	3145.0
39.80	480.0
43.90	1649.0
45.00	1732.0
46.10	217.0
47.00	2058.0
48.00	1090.0
49.00	6943.0
50.00	32088.0
51.00	10579.0
52.00	417.0
52.90	125.0
55.00	394.0
56.00	2512.0
57.00	4474.0
58.00	221.0
60.10	1718.0
61.00	7989.0
62.00	7808.0
63.00	6233.0
64.00	568.0
65.10	1085.0
65.80	126.0
67.00	527.0
68.00	17408.0
69.00	17536.0
70.00	1320.0
72.10	1007.0
73.00	8245.0
74.00	29896.0
75.00	89912.0
76.10	7651.0
77.10	957.0
78.10	690.0
78.90	5287.0
79.90	1775.0
81.00	5666.0
81.90	1231.0
85.90	335.0
87.00	7242.0
88.00	6342.0
91.00	638.0
92.00	4780.0
93.00	7612.0
94.00	20864.0
95.10	167872.0
96.00	11278.0
97.00	311.0
104.00	746.0
104.90	206.0
105.90	761.0
107.00	172.0
111.00	168.0
111.80	138.0
115.00	210.0
115.90	675.0
117.00	1244.0
117.80	458.0
118.90	864.0
127.90	579.0
128.90	366.0
129.90	674.0
131.00	180.0
135.00	245.0
137.00	248.0
141.00	1794.0
141.80	283.0
143.00	1878.0
145.00	273.0
146.10	172.0
146.90	113.0
148.00	430.0
149.90	296.0
152.80	104.0
155.00	319.0
156.10	177.0
157.10	263.0
158.00	106.0
159.00	176.0
160.90	218.0
170.90	206.0
172.10	1216.0
174.00	131328.0
175.10	10181.0
176.00	127864.0
177.00	8106.0
178.10	246.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

Scan 2881 (10.603 min): VU038608.D
BFB09

m/z	Abundance
40.00	315.0
43.90	683.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09