

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU060624\  
 Data File : VU059170.D  
 Acq On : 06 Jun 2024 17:08  
 Operator : MD/SY  
 Sample : P2693-01 200X  
 Misc : 5.0mL/MSVOA\_U/WATER  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :

Quant Time: Jun 07 05:10:17 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMULM052924WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Fri Jun 07 05:05:14 2024  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----						
Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	199938	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	200256	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	84541	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	44261	36.973	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	73.940%	
7) Chloroethane-d5	1.907	69	42851	41.787	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	83.580%	
11) 1,1-Dichloroethene-d2	2.560	63	62369	26.395	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	52.780%#	
21) 2-Butanone-d5	4.611	46	118559	105.072	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	105.070%	
24) Chloroform-d	5.055	84	110333	46.298	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.600%	
26) 1,2-Dichloroethane-d4	5.695	65	71830	49.177	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.360%	
32) Benzene-d6	5.721	84	199379	43.379	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	86.760%	
36) 1,2-Dichloropropane-d6	6.685	67	73977	46.681	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	93.360%	
41) Toluene-d8	7.894	98	162883	41.746	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	83.500%	
43) trans-1,3-Dichloroprop...	8.177	79	27795	43.390	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	86.780%	
47) 2-Hexanone-d5	8.627	63	62121	84.768	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	84.770%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84	127234	47.439	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	94.880%	
66) 1,2-Dichlorobenzene-d4	12.190	152	63175	50.074	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	100.140%	
Target Compounds						
37) 1,2-Dichloropropane	6.682	63	7598	3.700	ug/L #	90
-----						


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU060624\  
 Data File : VU059170.D  
 Acq On : 06 Jun 2024 17:08  
 Operator : MD/SY  
 Sample : P2693-01 200X  
 Misc : 5.0mL/MSVOA\_U/WATER  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :

Quant Time: Jun 07 05:10:17 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMULM052924WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Fri Jun 07 05:05:14 2024  
 Response via : Initial Calibration

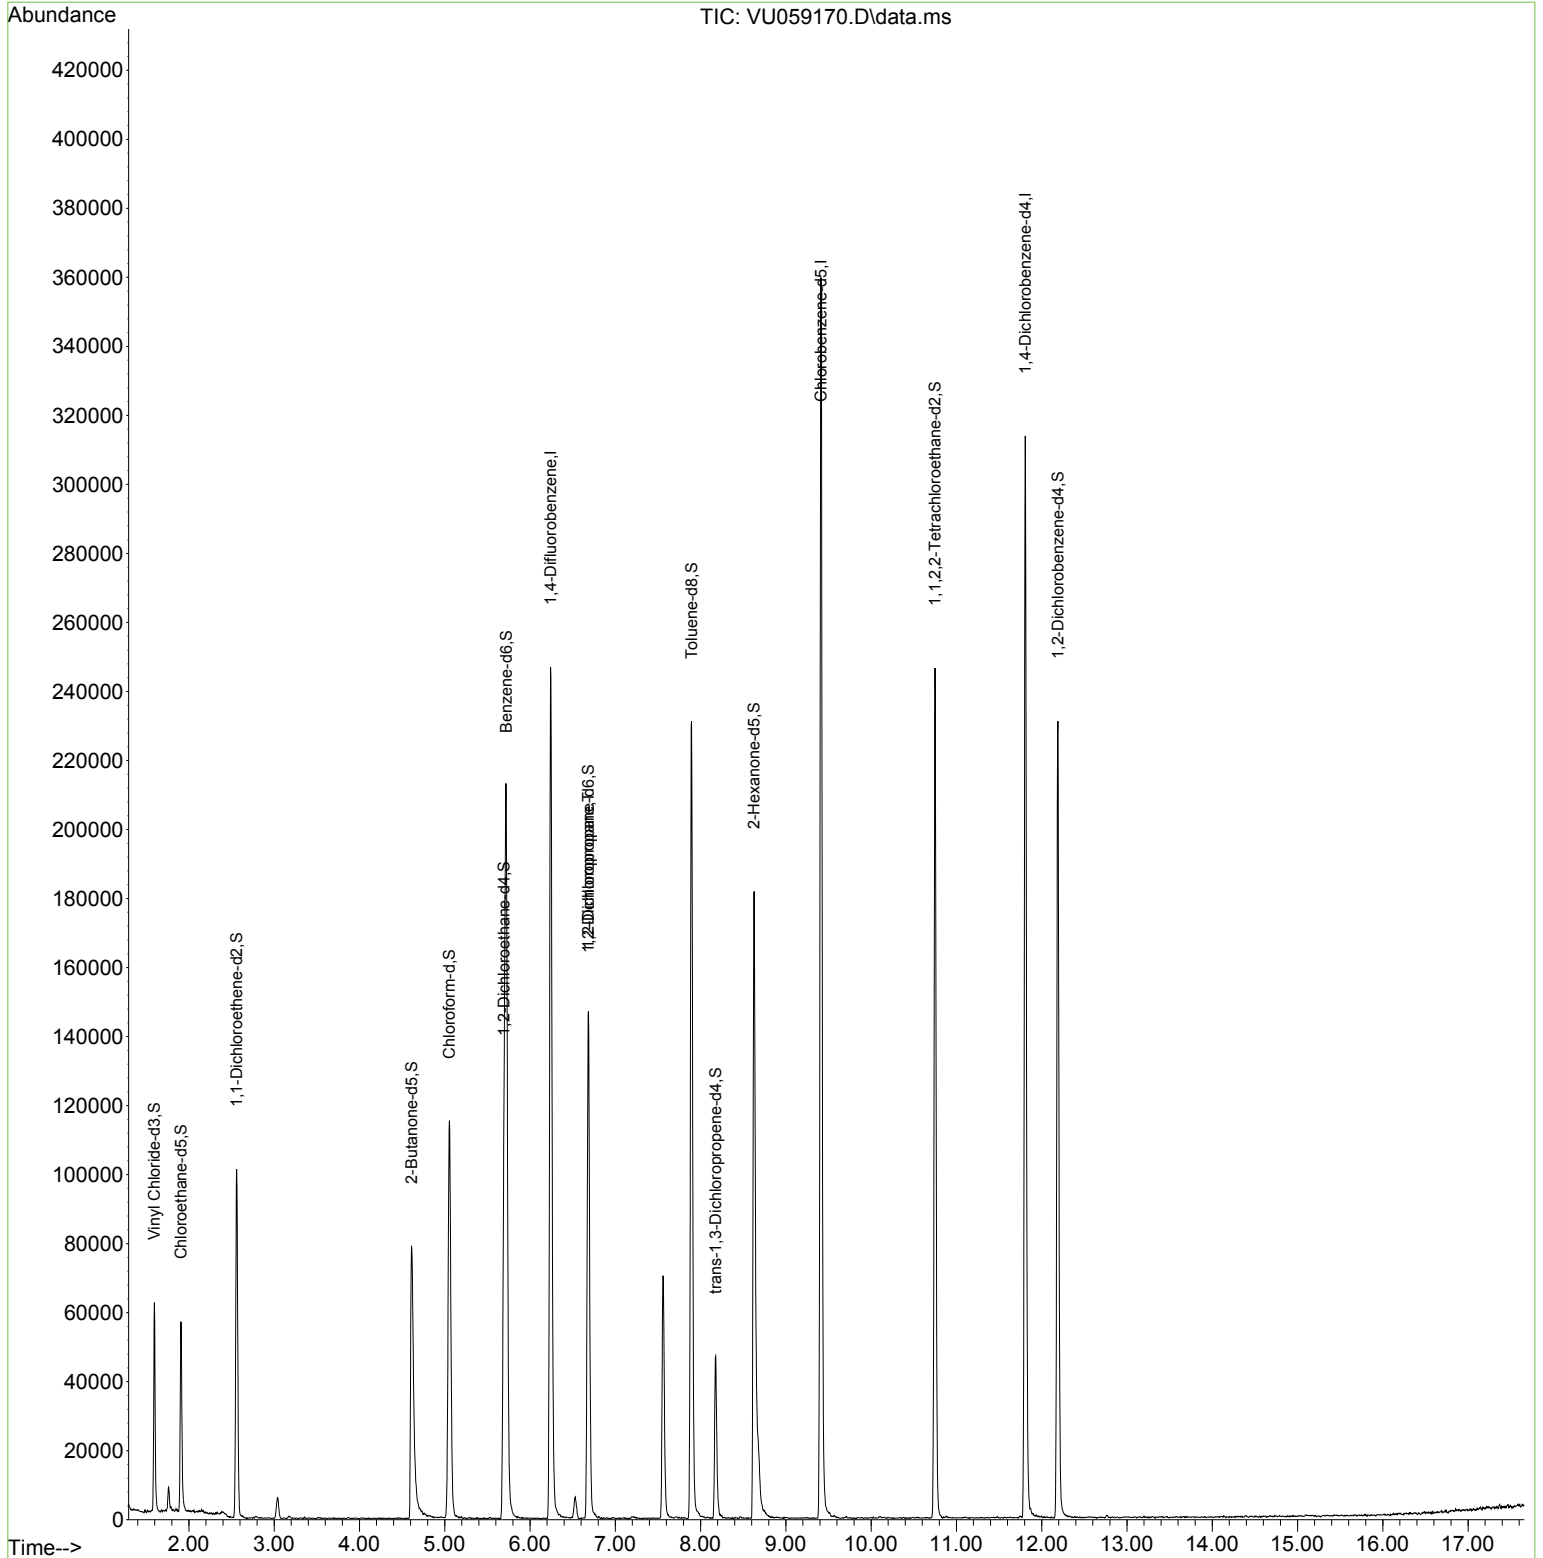

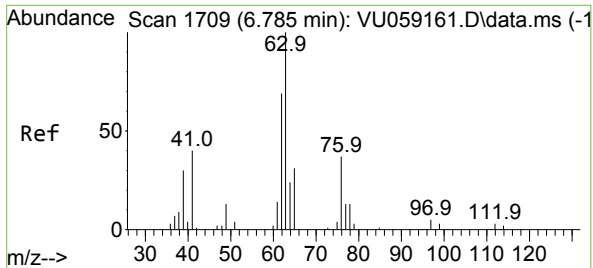

#37  
 1,2-Dichloropropane  
 Concen: 3.700 ug/L  
 RT: 6.682 min Scan# 1  
 Delta R.T. -0.103 min  
 Lab File: VU059170.D  
 Acq: 06 Jun 2024 17:08

Instrument :  
 MSVOA\_U  
 ClientSampleId :

Tgt Ion: 63 Resp: 7598  
 Ion Ratio Lower Upper  
 63 100  
 112 0.0 2.6 4.0#

