

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059162.D
 Acq On : 06 Jun 2024 12:46
 Operator : MD/SY
 Sample : VU0606MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK067

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	87	94	113	rVB	65282	80229	12.76%	1.506%
2	1.814	139	163	177	rBV3	50589	145940	23.20%	2.739%
3	1.891	179	187	206	rVB	54906	81098	12.89%	1.522%
4	2.554	382	393	410	rBV	111066	179862	28.60%	3.376%
5	2.663	425	427	435	rVB2	462	517	0.08%	0.010%
6	2.705	435	440	443	rBV3	440	411	0.07%	0.008%
7	2.782	454	464	473	rVV3	1839	2841	0.45%	0.053%
8	2.901	499	501	506	rVB	318	268	0.04%	0.005%
9	3.033	534	542	552	rVB3	3351	5802	0.92%	0.109%
10	3.120	562	569	575	rBV2	274	425	0.07%	0.008%
11	3.174	575	586	603	rVB	3630	7278	1.16%	0.137%
12	3.280	615	619	621	rBV	234	224	0.04%	0.004%
13	3.338	633	637	641	rBV2	465	530	0.08%	0.010%
14	3.467	674	677	682	rVB	358	319	0.05%	0.006%
15	3.496	682	686	687	rBV2	273	232	0.04%	0.004%
16	3.557	700	705	711	rBV2	262	381	0.06%	0.007%
17	3.682	741	744	746	rBV	241	183	0.03%	0.003%
18	3.808	779	783	786	rBV	228	185	0.03%	0.003%
19	3.859	795	799	804	rBV2	218	236	0.04%	0.004%
20	3.923	815	819	822	rVB	250	165	0.03%	0.003%
21	3.946	822	826	830	rVB	278	238	0.04%	0.004%
22	3.972	830	834	838	rBV	209	268	0.04%	0.005%
23	4.052	857	859	862	rBV	273	158	0.03%	0.003%
24	4.110	871	877	882	rBV2	289	388	0.06%	0.007%
25	4.608	1022	1032	1056	rBV	77189	190186	30.24%	3.569%
26	4.792	1087	1089	1091	rBV2	316	178	0.03%	0.003%
27	4.978	1144	1147	1152	rBV3	240	219	0.03%	0.004%
28	5.052	1155	1170	1198	rVV	120340	266311	42.34%	4.998%
29	5.171	1205	1207	1214	rVB3	379	307	0.05%	0.006%
30	5.264	1231	1236	1240	rBV2	182	203	0.03%	0.004%
31	5.354	1260	1264	1269	rVB2	182	163	0.03%	0.003%
32	5.467	1296	1299	1303	rBV2	241	204	0.03%	0.004%
33	5.714	1356	1376	1404	rBV2	228545	628928	100.00%	11.804%
34	5.956	1445	1451	1454	rBV2	434	453	0.07%	0.009%
35	6.242	1524	1540	1566	rBV	242296	471133	74.91%	8.842%
36	6.435	1597	1600	1605	rVB2	472	424	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059162.D
 Acq On : 06 Jun 2024 12:46
 Operator : MD/SY
 Sample : VU0606MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK067

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.493	1614	1618	1619	rBV2	399	293	0.05%	0.005%
38	6.528	1619	1629	1642	rVV5	6535	12595	2.00%	0.236%
39	6.682	1663	1677	1698	rBV	153151	300772	47.82%	5.645%
40	6.911	1741	1748	1753	rBV2	284	454	0.07%	0.009%
41	7.001	1773	1776	1779	rBV	233	198	0.03%	0.004%
42	7.203	1833	1839	1842	rBV2	617	673	0.11%	0.013%
43	7.560	1934	1950	1969	rBV	73429	129655	20.62%	2.433%
44	7.701	1991	1994	1997	rBV	420	324	0.05%	0.006%
45	7.795	2018	2023	2029	rBV2	299	367	0.06%	0.007%
46	7.891	2041	2053	2071	rBV	245914	429558	68.30%	8.062%
47	8.174	2131	2141	2158	rBV2	48881	84388	13.42%	1.584%
48	8.428	2217	2220	2223	rBV	217	176	0.03%	0.003%
49	8.470	2227	2233	2236	rVV2	389	446	0.07%	0.008%
50	8.550	2253	2258	2263	rBV3	795	862	0.14%	0.016%
51	8.627	2271	2282	2326	rBV	190551	385796	61.34%	7.241%
52	8.853	2349	2352	2356	rBV3	375	332	0.05%	0.006%
53	9.036	2404	2409	2411	rBV2	300	212	0.03%	0.004%
54	9.071	2418	2420	2422	rBV	273	184	0.03%	0.003%
55	9.164	2446	2449	2462	rVB2	294	483	0.08%	0.009%
56	9.219	2462	2466	2469	rBV	245	182	0.03%	0.003%
57	9.264	2477	2480	2482	rBV	281	220	0.03%	0.004%
58	9.280	2482	2485	2488	rVV	189	180	0.03%	0.003%
59	9.412	2514	2526	2551	rBV	346644	590895	93.95%	11.090%
60	9.692	2608	2613	2614	rBV	384	252	0.04%	0.005%
61	9.856	2660	2664	2670	rBV	386	289	0.05%	0.005%
62	9.926	2683	2686	2692	rBV	295	270	0.04%	0.005%
63	9.971	2693	2700	2704	rBV2	227	290	0.05%	0.005%
64	10.107	2739	2742	2747	rBV3	333	241	0.04%	0.005%
65	10.229	2775	2780	2784	rBV	261	242	0.04%	0.005%
66	10.370	2821	2824	2828	rVB2	341	248	0.04%	0.005%
67	10.415	2835	2838	2843	rVB2	243	207	0.03%	0.004%
68	10.640	2905	2908	2909	rBV	484	211	0.03%	0.004%
69	10.750	2929	2942	2967	rVV	242177	395835	62.94%	7.429%
70	10.891	2982	2986	2988	rVV	312	220	0.03%	0.004%
71	10.994	3014	3018	3024	rVB2	363	339	0.05%	0.006%
72	11.039	3029	3032	3037	rVV2	241	175	0.03%	0.003%
73	11.097	3045	3050	3057	rBV3	451	610	0.10%	0.011%
74	11.251	3094	3098	3101	rVB2	299	245	0.04%	0.005%
75	11.332	3121	3123	3127	rVB	325	188	0.03%	0.004%
76	11.364	3131	3133	3139	rVB	437	270	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059162.D
 Acq On : 06 Jun 2024 12:46
 Operator : MD/SY
 Sample : VU0606MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK067

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.428	3148	3153	3156	rBV2	404	400	0.06%	0.008%
78	11.470	3160	3166	3170	rBV3	493	481	0.08%	0.009%
79	11.531	3182	3185	3188	rVV2	208	159	0.03%	0.003%
80	11.666	3224	3227	3233	rBV2	238	244	0.04%	0.005%
81	11.714	3239	3242	3247	rVB2	227	221	0.04%	0.004%
82	11.743	3247	3251	3255	rBV2	1057	946	0.15%	0.018%
83	11.807	3259	3271	3296	rBV	301719	498875	79.32%	9.363%
84	12.061	3347	3350	3356	rVB2	280	257	0.04%	0.005%
85	12.126	3363	3370	3372	rBV2	205	209	0.03%	0.004%
86	12.187	3377	3389	3417	rVV	232678	397707	63.24%	7.464%
87	12.428	3461	3464	3466	rBV	319	180	0.03%	0.003%
88	12.688	3541	3545	3548	rBV2	294	262	0.04%	0.005%
89	12.727	3553	3557	3560	rBV2	335	289	0.05%	0.005%
90	13.119	3676	3679	3683	rBV2	369	295	0.05%	0.006%
91	13.769	3878	3881	3888	rBV2	399	459	0.07%	0.009%
92	13.814	3892	3895	3899	rVV2	244	269	0.04%	0.005%
93	13.852	3900	3907	3917	rVB6	1725	2752	0.44%	0.052%
94	14.100	3976	3984	3997	rBV2	6721	12558	2.00%	0.236%
95	14.274	4035	4038	4042	rBV	387	310	0.05%	0.006%
96	14.331	4051	4056	4065	rVB4	2239	3284	0.52%	0.062%
97	14.743	4181	4184	4186	rBV2	292	218	0.03%	0.004%
98	14.833	4209	4212	4222	rVB3	492	656	0.10%	0.012%
99	14.984	4256	4259	4261	rBV	381	286	0.05%	0.005%
100	15.042	4270	4277	4280	rBV3	484	645	0.10%	0.012%


Sum of corrected areas: 5328226

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059162.D
Acq On : 06 Jun 2024 12:46
Operator : MD/SY
Sample : VU0606MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK067

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

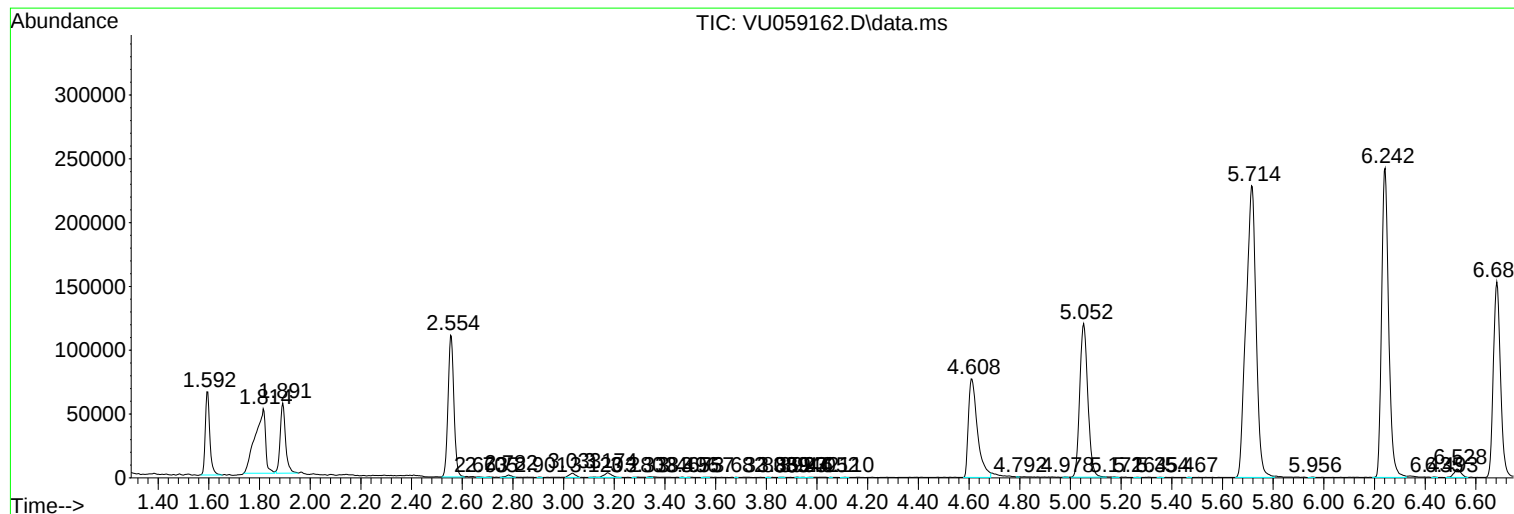

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059162.D
Acq On : 06 Jun 2024 12:46
Operator : MD/SY
Sample : VU0606MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK067

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059162.D
Acq On : 06 Jun 2024 12:46
Operator : MD/SY
Sample : VU0606MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK067

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc