

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059163.D
 Acq On : 06 Jun 2024 14:13
 Operator : MD/SY
 Sample : VU0606WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK068

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	117	rVB	93279	111197	16.89%	2.129%
2	1.910	184	193	216	rVB	73145	100912	15.33%	1.932%
3	2.563	383	396	415	rBV	137814	227095	34.50%	4.349%
4	2.785	460	465	472	rVB3	746	1114	0.17%	0.021%
5	3.042	534	545	557	rVB3	3766	7328	1.11%	0.140%
6	3.335	628	636	642	rVB2	285	479	0.07%	0.009%
7	3.367	642	646	647	rBV	267	202	0.03%	0.004%
8	3.592	712	716	721	rBV2	155	196	0.03%	0.004%
9	3.750	759	765	770	rBV2	171	241	0.04%	0.005%
10	3.946	823	826	830	rVB	315	260	0.04%	0.005%
11	4.036	851	854	859	rBV2	190	217	0.03%	0.004%
12	4.065	859	863	866	rBV2	200	173	0.03%	0.003%
13	4.190	897	902	906	rBV2	182	188	0.03%	0.004%
14	4.428	971	976	981	rVB2	287	345	0.05%	0.007%
15	4.618	1025	1035	1067	rBV	52282	135186	20.54%	2.589%
16	4.962	1139	1142	1145	rVB	359	234	0.04%	0.004%
17	4.991	1145	1151	1154	rBV2	303	410	0.06%	0.008%
18	5.055	1156	1171	1196	rBV2	115572	260701	39.60%	4.992%
19	5.190	1211	1213	1218	rVB3	410	291	0.04%	0.006%
20	5.332	1252	1257	1259	rBV2	178	180	0.03%	0.003%
21	5.393	1271	1276	1280	rVB2	293	298	0.05%	0.006%
22	5.492	1300	1307	1316	rVB2	354	682	0.10%	0.013%
23	5.563	1326	1329	1334	rVB	213	218	0.03%	0.004%
24	5.624	1345	1348	1352	rBV2	250	266	0.04%	0.005%
25	5.717	1357	1377	1400	rBV2	242312	658318	100.00%	12.606%
26	5.926	1439	1442	1443	rBV	261	173	0.03%	0.003%
27	6.074	1484	1488	1492	rVB2	367	362	0.05%	0.007%
28	6.097	1492	1495	1497	rBV2	284	183	0.03%	0.004%
29	6.129	1503	1505	1508	rVB	353	188	0.03%	0.004%
30	6.148	1508	1511	1516	rVB3	344	272	0.04%	0.005%
31	6.245	1528	1541	1567	rBV	249116	490148	74.45%	9.386%
32	6.383	1581	1584	1589	rVB4	546	541	0.08%	0.010%
33	6.428	1596	1598	1601	rVB2	354	207	0.03%	0.004%
34	6.454	1601	1606	1608	rBV2	272	268	0.04%	0.005%
35	6.531	1620	1630	1639	rVV6	5102	9896	1.50%	0.189%
36	6.685	1664	1678	1703	rBV	152529	298053	45.27%	5.707%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059163.D
 Acq On : 06 Jun 2024 14:13
 Operator : MD/SY
 Sample : VU0606WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK068

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.807	1714	1716	1719	rVV3	492	363	0.06%	0.007%
38	6.987	1766	1772	1775	rBV2	194	221	0.03%	0.004%
39	7.052	1787	1792	1797	rBV2	208	284	0.04%	0.005%
40	7.103	1803	1808	1811	rBV2	185	183	0.03%	0.004%
41	7.196	1831	1837	1844	rBV4	739	1072	0.16%	0.021%
42	7.393	1892	1898	1903	rBV2	315	486	0.07%	0.009%
43	7.428	1906	1909	1916	rBV2	318	372	0.06%	0.007%
44	7.563	1940	1951	1976	rBV	73821	134991	20.51%	2.585%
45	7.798	2019	2024	2030	rBV2	221	260	0.04%	0.005%
46	7.894	2041	2054	2083	rBV	274210	494684	75.14%	9.472%
47	8.007	2087	2089	2097	rVB3	580	550	0.08%	0.011%
48	8.177	2132	2142	2161	rBV2	49036	86924	13.20%	1.664%
49	8.335	2186	2191	2194	rBV2	339	282	0.04%	0.005%
50	8.367	2198	2201	2203	rBV	241	170	0.03%	0.003%
51	8.553	2257	2259	2264	rBV2	340	213	0.03%	0.004%
52	8.630	2273	2283	2313	rBV2	130251	281458	42.75%	5.389%
53	8.823	2340	2343	2349	rVB	375	257	0.04%	0.005%
54	9.000	2395	2398	2402	rBV2	234	195	0.03%	0.004%
55	9.042	2407	2411	2414	rVV	204	176	0.03%	0.003%
56	9.119	2431	2435	2438	rBV	240	234	0.04%	0.004%
57	9.158	2443	2447	2453	rVB	278	268	0.04%	0.005%
58	9.412	2514	2526	2562	rBV	366426	632450	96.07%	12.110%
59	9.704	2613	2617	2620	rBV	385	194	0.03%	0.004%
60	9.737	2624	2627	2630	rBV2	195	192	0.03%	0.004%
61	9.839	2655	2659	2665	rVB2	194	172	0.03%	0.003%
62	10.052	2723	2725	2728	rBV	305	219	0.03%	0.004%
63	10.103	2738	2741	2746	rVB2	225	185	0.03%	0.004%
64	10.280	2793	2796	2802	rVB2	259	183	0.03%	0.004%
65	10.344	2812	2816	2821	rBV2	283	372	0.06%	0.007%
66	10.656	2906	2913	2916	rBV4	628	739	0.11%	0.014%
67	10.749	2930	2942	2965	rVV	198746	325612	49.46%	6.235%
68	10.865	2974	2978	2981	rVB2	318	239	0.04%	0.005%
69	10.894	2982	2987	2989	rVB2	297	200	0.03%	0.004%
70	10.981	3011	3014	3016	rBV2	227	177	0.03%	0.003%
71	11.068	3038	3041	3045	rBV2	235	205	0.03%	0.004%
72	11.347	3122	3128	3129	rBV2	209	189	0.03%	0.004%
73	11.434	3152	3155	3161	rVB	312	250	0.04%	0.005%
74	11.662	3222	3226	3229	rBV	299	307	0.05%	0.006%
75	11.810	3259	3272	3290	rBV	314830	533916	81.10%	10.224%
76	12.087	3354	3358	3362	rVB2	282	235	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059163.D
 Acq On : 06 Jun 2024 14:13
 Operator : MD/SY
 Sample : VU0606WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK068

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	12.109	3362	3365	3367	rBV	407	205	0.03%	0.004%
78	12.190	3378	3390	3411	rBV	239346	408313	62.02%	7.819%
79	12.389	3447	3452	3456	rBV	353	349	0.05%	0.007%
80	12.685	3539	3544	3546	rBV2	286	254	0.04%	0.005%
81	12.701	3546	3549	3553	rBV2	242	223	0.03%	0.004%
82	12.765	3566	3569	3573	rVB3	452	378	0.06%	0.007%
83	13.203	3702	3705	3708	rBV	261	175	0.03%	0.003%
84	13.466	3785	3787	3792	rVB	289	188	0.03%	0.004%
85	13.560	3813	3816	3820	rVB	318	216	0.03%	0.004%
86	13.791	3886	3888	3895	rVB2	407	258	0.04%	0.005%
87	13.878	3910	3915	3919	rVB3	654	629	0.10%	0.012%
88	13.900	3919	3922	3929	rBV2	235	281	0.04%	0.005%
89	13.981	3944	3947	3951	rVB2	291	188	0.03%	0.004%
90	14.244	4024	4029	4032	rBV2	420	444	0.07%	0.009%
91	14.450	4090	4093	4097	rBV	303	252	0.04%	0.005%
92	14.482	4101	4103	4107	rVV2	370	258	0.04%	0.005%
93	14.553	4122	4125	4136	rVB2	584	631	0.10%	0.012%
94	14.740	4180	4183	4189	rBV2	563	640	0.10%	0.012%
95	14.820	4205	4208	4211	rBV2	399	341	0.05%	0.007%
96	14.916	4235	4238	4242	rBV3	355	296	0.04%	0.006%
97	15.174	4315	4318	4322	rBV2	379	389	0.06%	0.007%
98	15.428	4394	4397	4400	rBV	450	308	0.05%	0.006%
99	15.598	4448	4450	4451	rBV	434	180	0.03%	0.003%
100	15.836	4521	4524	4526	rBV	439	261	0.04%	0.005%




Sum of corrected areas: 5222358

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059163.D
Acq On : 06 Jun 2024 14:13
Operator : MD/SY
Sample : VU0606WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK068

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

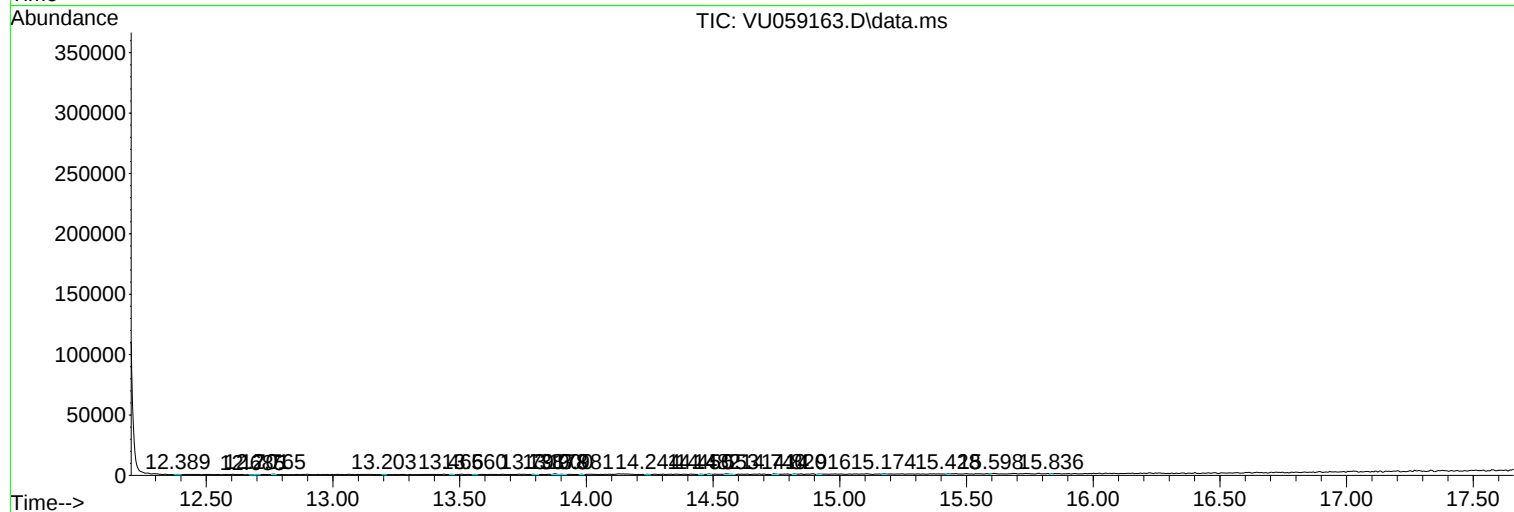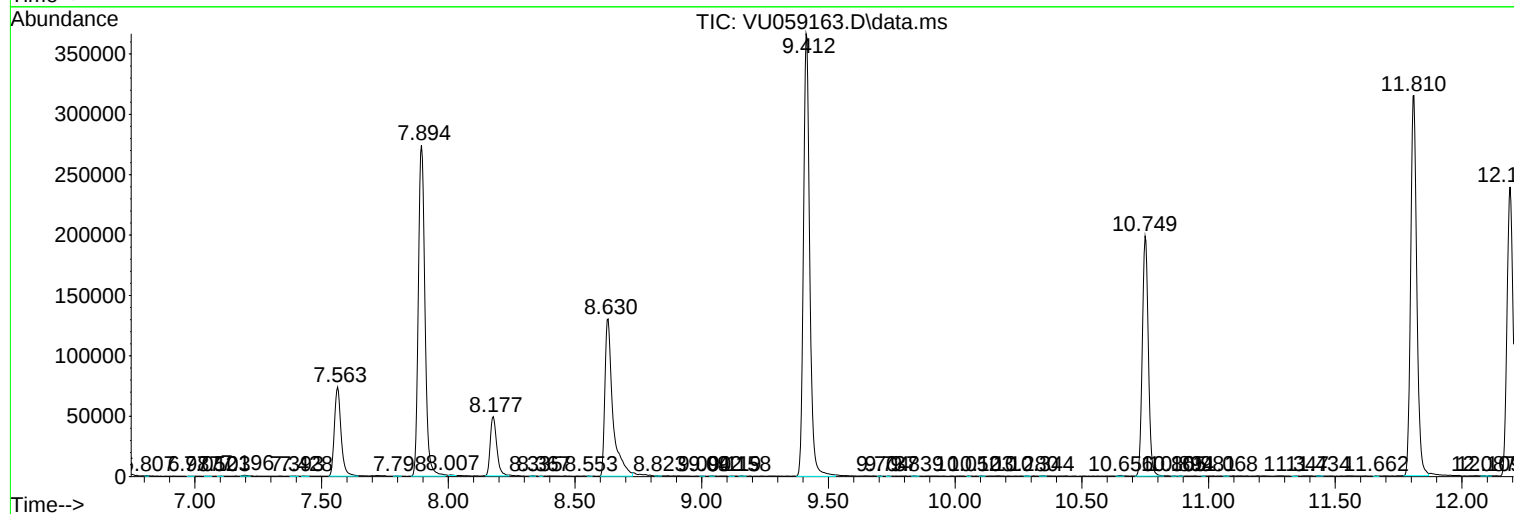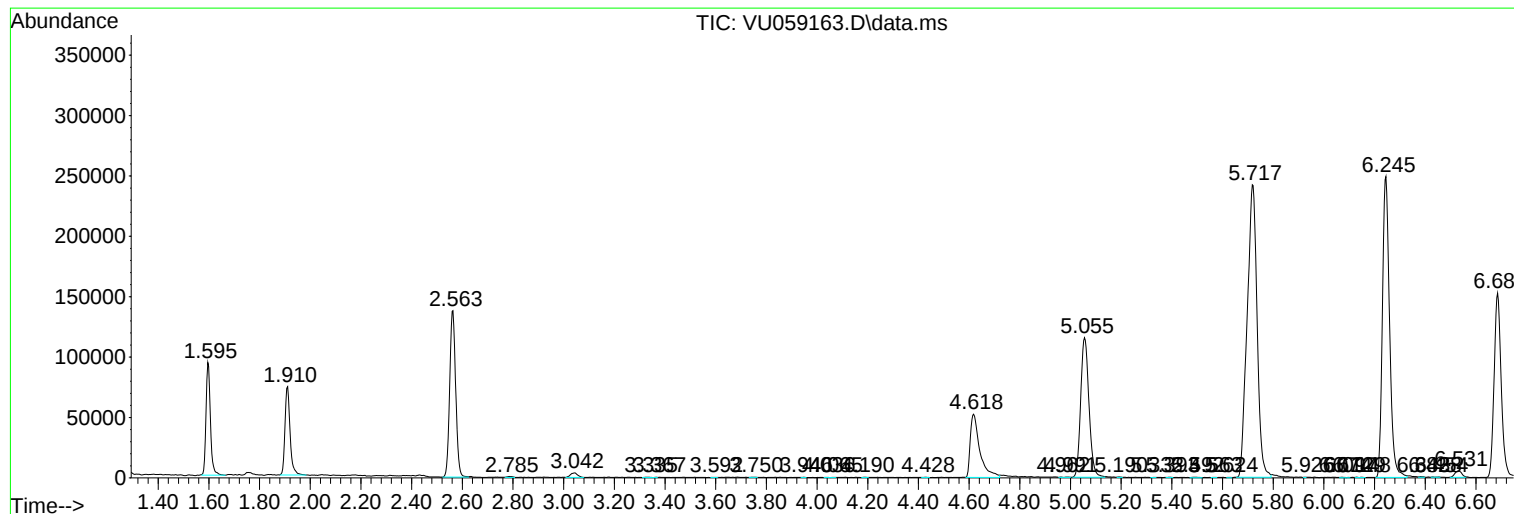

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059163.D
Acq On : 06 Jun 2024 14:13
Operator : MD/SY
Sample : VU0606WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK068

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059163.D
Acq On : 06 Jun 2024 14:13
Operator : MD/SY
Sample : VU0606WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK068

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------