

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059164.D
 Acq On : 06 Jun 2024 14:49
 Operator : MD/SY
 Sample : P2635-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059164.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	118	rVB	87808	105367	16.61%	2.093%
2	1.911	184	193	212	rVB	70209	95393	15.04%	1.895%
3	2.396	341	344	347	rVB3	977	555	0.09%	0.011%
4	2.509	376	379	382	rBV2	243	179	0.03%	0.004%
5	2.560	382	395	417	rVV	130374	214233	33.77%	4.256%
6	2.753	452	455	458	rBV2	275	194	0.03%	0.004%
7	2.920	505	507	512	rBV2	192	185	0.03%	0.004%
8	3.039	533	544	559	rVB3	5023	9490	1.50%	0.189%
9	3.094	559	561	564	rBV2	306	195	0.03%	0.004%
10	3.178	580	587	591	rBV4	536	763	0.12%	0.015%
11	3.576	702	711	718	rBV2	317	604	0.10%	0.012%
12	3.612	718	722	724	rVB2	285	203	0.03%	0.004%
13	3.708	743	752	754	rBV	234	377	0.06%	0.007%
14	3.779	770	774	778	rBV	269	277	0.04%	0.006%
15	3.850	790	796	801	rVB	229	286	0.05%	0.006%
16	3.978	830	836	838	rBV2	260	259	0.04%	0.005%
17	4.155	889	891	897	rVB	233	223	0.04%	0.004%
18	4.213	904	909	912	rBV	196	189	0.03%	0.004%
19	4.386	960	963	966	rBV2	222	187	0.03%	0.004%
20	4.618	1025	1035	1059	rBV	50988	131618	20.75%	2.615%
21	5.055	1156	1171	1192	rBV	111793	250779	39.54%	4.982%
22	5.296	1245	1246	1252	rVB2	318	214	0.03%	0.004%
23	5.364	1264	1267	1271	rVB	178	185	0.03%	0.004%
24	5.412	1276	1282	1284	rVB2	345	328	0.05%	0.007%
25	5.431	1284	1288	1290	rBV2	313	259	0.04%	0.005%
26	5.721	1358	1378	1400	rBV2	232798	634319	100.00%	12.602%
27	5.923	1437	1441	1445	rBV3	266	234	0.04%	0.005%
28	5.946	1445	1448	1451	rVB2	373	317	0.05%	0.006%
29	5.972	1451	1456	1459	rBV2	303	313	0.05%	0.006%
30	6.036	1472	1476	1477	rBV	361	222	0.03%	0.004%
31	6.058	1480	1483	1488	rVV2	436	376	0.06%	0.007%
32	6.097	1491	1495	1498	rBV2	226	245	0.04%	0.005%
33	6.129	1503	1505	1511	rVB2	192	233	0.04%	0.005%
34	6.245	1528	1541	1568	rBV	244700	471120	74.27%	9.360%
35	6.393	1585	1587	1591	rBV2	329	271	0.04%	0.005%
36	6.534	1619	1631	1641	rBV8	5354	10170	1.60%	0.202%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059164.D
 Acq On : 06 Jun 2024 14:49
 Operator : MD/SY
 Sample : P2635-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.576	1642	1644	1648	rVB3	335	212	0.03%	0.004%
38	6.611	1648	1655	1657	rBV2	248	197	0.03%	0.004%
39	6.685	1665	1678	1702	rBV	145254	286722	45.20%	5.696%
40	6.833	1720	1724	1728	rBV3	428	461	0.07%	0.009%
41	6.898	1739	1744	1748	rBV2	358	339	0.05%	0.007%
42	6.949	1754	1760	1763	rBV	304	309	0.05%	0.006%
43	7.197	1832	1837	1843	rBV2	751	965	0.15%	0.019%
44	7.338	1877	1881	1885	rBV2	205	206	0.03%	0.004%
45	7.563	1939	1951	1979	rBV2	71900	131663	20.76%	2.616%
46	7.718	1993	1999	2006	rVB4	637	989	0.16%	0.020%
47	7.894	2042	2054	2077	rBV	265525	468541	73.87%	9.308%
48	8.123	2121	2125	2127	rBV	266	230	0.04%	0.005%
49	8.177	2132	2142	2164	rBV2	49337	85618	13.50%	1.701%
50	8.476	2233	2235	2244	rVB2	347	447	0.07%	0.009%
51	8.631	2272	2283	2320	rBV2	121896	272380	42.94%	5.411%
52	8.865	2352	2356	2359	rVB2	537	463	0.07%	0.009%
53	8.888	2359	2363	2368	rBV3	502	545	0.09%	0.011%
54	8.978	2388	2391	2396	rVV	342	261	0.04%	0.005%
55	9.036	2402	2409	2417	rBV2	306	573	0.09%	0.011%
56	9.071	2417	2420	2426	rVV2	290	311	0.05%	0.006%
57	9.129	2435	2438	2445	rVB	304	393	0.06%	0.008%
58	9.177	2446	2453	2456	rBV	317	367	0.06%	0.007%
59	9.222	2464	2467	2471	rVB2	269	190	0.03%	0.004%
60	9.328	2495	2500	2503	rBV	300	297	0.05%	0.006%
61	9.351	2503	2507	2512	rVB	248	221	0.03%	0.004%
62	9.412	2513	2526	2563	rBV	351895	609765	96.13%	12.114%
63	9.640	2594	2597	2599	rBV	318	204	0.03%	0.004%
64	9.653	2599	2601	2604	rVB	381	184	0.03%	0.004%
65	9.698	2611	2615	2620	rVB2	409	330	0.05%	0.007%
66	9.791	2640	2644	2647	rBV	306	221	0.03%	0.004%
67	10.280	2794	2796	2799	rBV2	275	181	0.03%	0.004%
68	10.650	2906	2911	2914	rBV2	614	501	0.08%	0.010%
69	10.750	2929	2942	2958	rBV	194229	319558	50.38%	6.349%
70	11.254	3095	3099	3102	rBV	308	246	0.04%	0.005%
71	11.319	3116	3119	3120	rBV	427	232	0.04%	0.005%
72	11.393	3137	3142	3147	rVB2	361	454	0.07%	0.009%
73	11.425	3147	3152	3155	rBV2	412	401	0.06%	0.008%
74	11.566	3193	3196	3199	rBV	304	238	0.04%	0.005%
75	11.650	3218	3222	3224	rBV2	217	188	0.03%	0.004%
76	11.811	3259	3272	3294	rBV	304214	516371	81.41%	10.259%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059164.D
 Acq On : 06 Jun 2024 14:49
 Operator : MD/SY
 Sample : P2635-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	12.052	3340	3347	3349	rBV2	317	384	0.06%	0.008%
78	12.190	3378	3390	3412	rBV	234947	394893	62.25%	7.845%
79	12.328	3430	3433	3436	rBV2	366	267	0.04%	0.005%
80	12.450	3468	3471	3474	rBV	290	227	0.04%	0.005%
81	12.759	3563	3567	3569	rBV	334	275	0.04%	0.005%
82	12.807	3578	3582	3585	rBV2	335	312	0.05%	0.006%
83	13.074	3662	3665	3670	rVB	350	329	0.05%	0.007%
84	13.158	3688	3691	3696	rBV	351	353	0.06%	0.007%
85	13.184	3696	3699	3704	rVB	468	480	0.08%	0.010%
86	13.216	3704	3709	3711	rBV	318	313	0.05%	0.006%
87	13.454	3780	3783	3785	rBV	280	195	0.03%	0.004%
88	13.868	3909	3912	3914	rBV	376	212	0.03%	0.004%
89	14.431	4083	4087	4089	rBV	257	213	0.03%	0.004%
90	14.486	4102	4104	4109	rBV2	290	264	0.04%	0.005%
91	14.550	4122	4124	4127	rBV	348	275	0.04%	0.005%
92	14.618	4142	4145	4148	rVB2	340	197	0.03%	0.004%
93	14.743	4181	4184	4188	rVB2	370	284	0.04%	0.006%
94	14.762	4188	4190	4193	rBV	279	227	0.04%	0.005%
95	14.907	4232	4235	4238	rBV	473	300	0.05%	0.006%
96	15.138	4304	4307	4308	rBV	347	207	0.03%	0.004%
97	15.193	4321	4324	4326	rBV	400	231	0.04%	0.005%
98	15.232	4334	4336	4337	rBV	341	188	0.03%	0.004%
99	15.547	4431	4434	4435	rBV	444	242	0.04%	0.005%
100	16.003	4574	4576	4580	rBV3	502	330	0.05%	0.007%




Sum of corrected areas: 5033534

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059164.D
Acq On : 06 Jun 2024 14:49
Operator : MD/SY
Sample : P2635-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

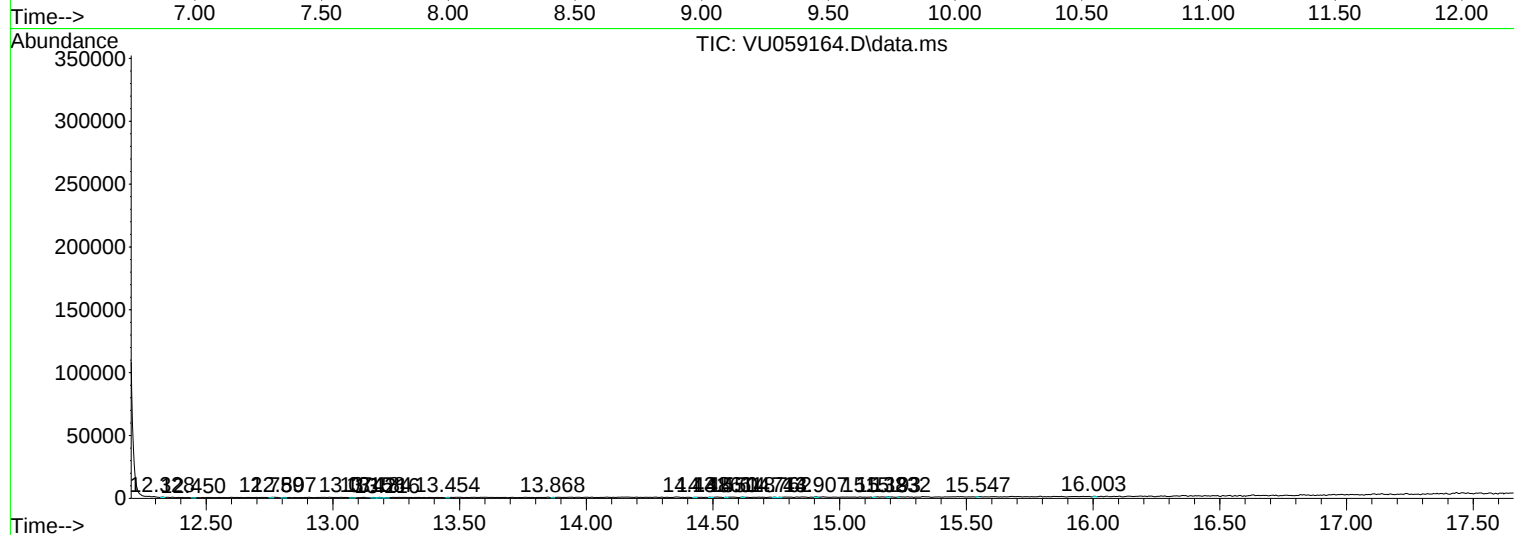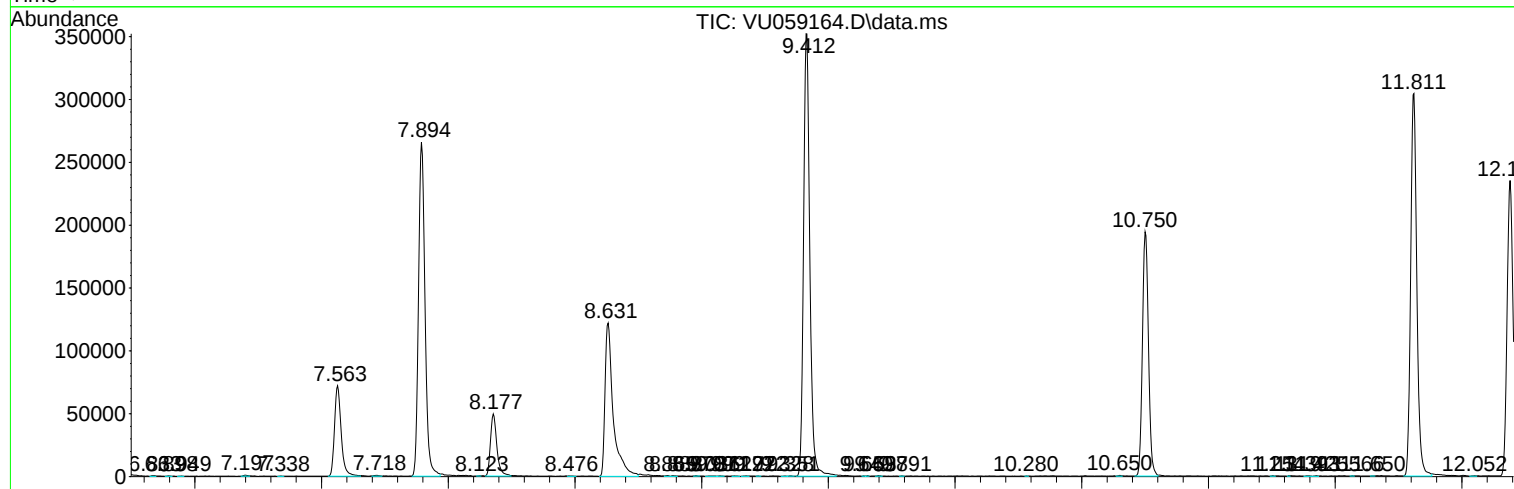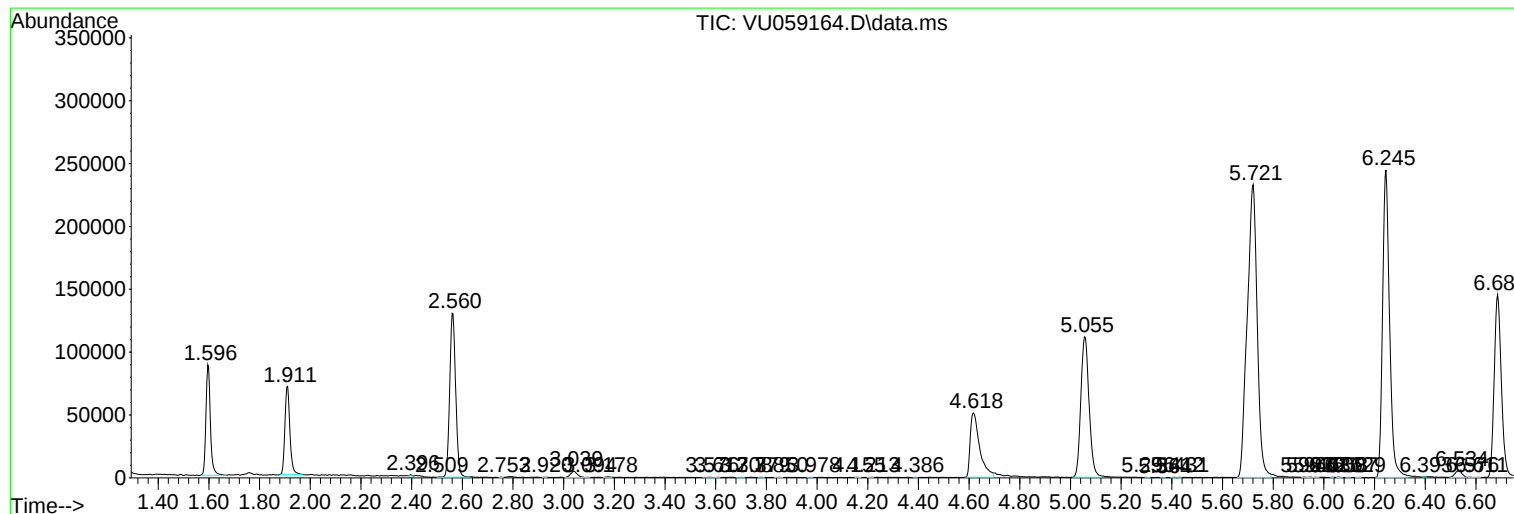

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059164.D
Acq On : 06 Jun 2024 14:49
Operator : MD/SY
Sample : P2635-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059164.D
Acq On : 06 Jun 2024 14:49
Operator : MD/SY
Sample : P2635-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------