

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059165.D
 Acq On : 06 Jun 2024 15:12
 Operator : MD/SY
 Sample : P2696-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4D66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059165.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	116	rVB	62189	74979	11.85%	1.395%
2	1.907	184	192	212	rBV	56228	77572	12.26%	1.443%
3	2.004	220	222	227	rBV2	759	641	0.10%	0.012%
4	2.560	382	395	407	rBV	103204	168658	26.65%	3.138%
5	2.618	408	413	423	rVB	6039	9528	1.51%	0.177%
6	2.753	445	455	458	rBV3	661	1091	0.17%	0.020%
7	2.843	480	483	487	rVB	262	180	0.03%	0.003%
8	2.985	525	527	533	rBV2	278	245	0.04%	0.005%
9	3.036	537	543	544	rBV2	1572	1350	0.21%	0.025%
10	3.178	571	587	609	rVV	21882	50761	8.02%	0.945%
11	3.550	700	703	712	rVB2	423	470	0.07%	0.009%
12	3.673	732	741	744	rBV2	290	450	0.07%	0.008%
13	3.785	773	776	779	rVB2	312	245	0.04%	0.005%
14	3.808	779	783	786	rBV	345	342	0.05%	0.006%
15	3.856	794	798	802	rBV2	191	192	0.03%	0.004%
16	3.927	813	820	827	rVV2	258	465	0.07%	0.009%
17	4.059	856	861	863	rBV2	201	214	0.03%	0.004%
18	4.113	873	878	884	rBV2	224	261	0.04%	0.005%
19	4.200	898	905	906	rBV	257	265	0.04%	0.005%
20	4.415	969	972	978	rBV2	293	339	0.05%	0.006%
21	4.473	987	990	993	rVB	259	169	0.03%	0.003%
22	4.496	993	997	999	rBV2	225	173	0.03%	0.003%
23	4.515	999	1003	1007	rVB	402	343	0.05%	0.006%
24	4.612	1017	1033	1067	rBV	103155	284903	45.01%	5.301%
25	5.055	1156	1171	1194	rBV2	117829	262299	41.44%	4.881%
26	5.203	1215	1217	1230	rVB5	726	977	0.15%	0.018%
27	5.267	1230	1237	1241	rBV3	323	501	0.08%	0.009%
28	5.380	1268	1272	1278	rBV2	257	353	0.06%	0.007%
29	5.435	1285	1289	1294	rBV3	227	207	0.03%	0.004%
30	5.502	1306	1310	1314	rBV3	225	276	0.04%	0.005%
31	5.570	1328	1331	1334	rBV2	301	278	0.04%	0.005%
32	5.718	1358	1377	1406	rBV2	220962	613927	96.99%	11.424%
33	5.904	1432	1435	1440	rVB	436	329	0.05%	0.006%
34	6.242	1528	1540	1571	rBV	254431	494884	78.19%	9.208%
35	6.464	1604	1609	1610	rBV	204	198	0.03%	0.004%
36	6.528	1619	1629	1642	rBV4	6338	12783	2.02%	0.238%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059165.D
 Acq On : 06 Jun 2024 15:12
 Operator : MD/SY
 Sample : P2696-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4D66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.685	1663	1678	1701	rBV	149934	299135	47.26%	5.566%
38	6.804	1713	1715	1719	rBV	269	196	0.03%	0.004%
39	6.898	1740	1744	1746	rBV	372	222	0.04%	0.004%
40	7.065	1793	1796	1804	rBV2	179	281	0.04%	0.005%
41	7.197	1833	1837	1843	rVV3	592	744	0.12%	0.014%
42	7.290	1862	1866	1870	rBV	240	218	0.03%	0.004%
43	7.438	1909	1912	1916	rVB	243	172	0.03%	0.003%
44	7.473	1921	1923	1926	rBV2	225	169	0.03%	0.003%
45	7.563	1939	1951	1972	rBV	70716	128929	20.37%	2.399%
46	7.711	1991	1997	1999	rBV4	513	529	0.08%	0.010%
47	7.817	2027	2030	2039	rVB3	364	520	0.08%	0.010%
48	7.894	2039	2054	2076	rBV	237922	424155	67.01%	7.892%
49	8.177	2131	2142	2167	rBV	47681	86546	13.67%	1.610%
50	8.412	2212	2215	2218	rBV	267	184	0.03%	0.003%
51	8.467	2224	2232	2245	rVB3	2660	4691	0.74%	0.087%
52	8.557	2257	2260	2262	rVB2	327	195	0.03%	0.004%
53	8.573	2262	2265	2270	rBV	265	348	0.05%	0.006%
54	8.627	2271	2282	2323	rBV2	175885	377844	59.69%	7.031%
55	8.788	2326	2332	2341	rVB6	4425	7183	1.13%	0.134%
56	8.949	2375	2382	2385	rBV	268	357	0.06%	0.007%
57	9.000	2393	2398	2399	rBV	344	234	0.04%	0.004%
58	9.152	2443	2445	2449	rVB	358	224	0.04%	0.004%
59	9.177	2450	2453	2459	rBV2	178	229	0.04%	0.004%
60	9.364	2506	2511	2513	rBV2	291	278	0.04%	0.005%
61	9.412	2513	2526	2563	rVV	367993	632960	100.00%	11.778%
62	9.611	2585	2588	2595	rVB2	289	307	0.05%	0.006%
63	9.766	2631	2636	2639	rBV	392	394	0.06%	0.007%
64	9.843	2656	2660	2663	rBV2	372	318	0.05%	0.006%
65	9.888	2669	2674	2678	rBV2	306	308	0.05%	0.006%
66	10.106	2738	2742	2748	rVB2	492	473	0.07%	0.009%
67	10.187	2764	2767	2771	rBV2	267	251	0.04%	0.005%
68	10.650	2905	2911	2913	rBV3	484	451	0.07%	0.008%
69	10.688	2917	2923	2927	rBV2	373	410	0.06%	0.008%
70	10.750	2929	2942	2961	rBV	242744	395128	62.43%	7.352%
71	10.888	2978	2985	2996	rVB3	4063	5432	0.86%	0.101%
72	11.090	3043	3048	3049	rBV	201	182	0.03%	0.003%
73	11.235	3090	3093	3096	rBV	406	289	0.05%	0.005%
74	11.283	3105	3108	3110	rBV	427	244	0.04%	0.005%
75	11.364	3129	3133	3137	rBV	295	271	0.04%	0.005%
76	11.505	3174	3177	3181	rBV2	298	201	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059165.D
 Acq On : 06 Jun 2024 15:12
 Operator : MD/SY
 Sample : P2696-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4D66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.534	3181	3186	3189	rBV2	286	315	0.05%	0.006%
78	11.807	3259	3271	3299	rBV	318299	533458	84.28%	9.926%
79	11.959	3315	3318	3322	rBV3	388	262	0.04%	0.005%
80	12.074	3351	3354	3356	rBV2	454	280	0.04%	0.005%
81	12.090	3357	3359	3361	rBV2	436	254	0.04%	0.005%
82	12.190	3378	3390	3417	rBV	234543	400010	63.20%	7.443%
83	12.335	3433	3435	3439	rVV3	512	305	0.05%	0.006%
84	12.367	3443	3445	3449	rVB3	642	401	0.06%	0.007%
85	12.473	3470	3478	3483	rBV	335	556	0.09%	0.010%
86	12.540	3492	3499	3503	rBV5	1784	1865	0.29%	0.035%
87	12.647	3529	3532	3535	rBV2	242	171	0.03%	0.003%
88	12.753	3561	3565	3566	rBV2	518	371	0.06%	0.007%
89	12.859	3595	3598	3602	rBV2	223	183	0.03%	0.003%
90	12.904	3609	3612	3615	rBV	502	267	0.04%	0.005%
91	13.460	3782	3785	3792	rBV2	495	453	0.07%	0.008%
92	13.621	3831	3835	3840	rBV2	446	427	0.07%	0.008%
93	13.865	3908	3911	3915	rVB2	470	291	0.05%	0.005%
94	13.949	3931	3937	3940	rBV	329	387	0.06%	0.007%
95	14.119	3986	3990	3992	rBV3	499	428	0.07%	0.008%
96	14.772	4191	4193	4197	rBV2	358	249	0.04%	0.005%
97	14.946	4243	4247	4249	rBV	407	366	0.06%	0.007%
98	14.962	4250	4252	4254	rBV2	346	199	0.03%	0.004%
99	15.106	4294	4297	4300	rVB2	631	384	0.06%	0.007%
100	15.823	4518	4520	4523	rBV2	406	303	0.05%	0.006%




Sum of corrected areas: 5374235

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059165.D
Acq On : 06 Jun 2024 15:12
Operator : MD/SY
Sample : P2696-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4D66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

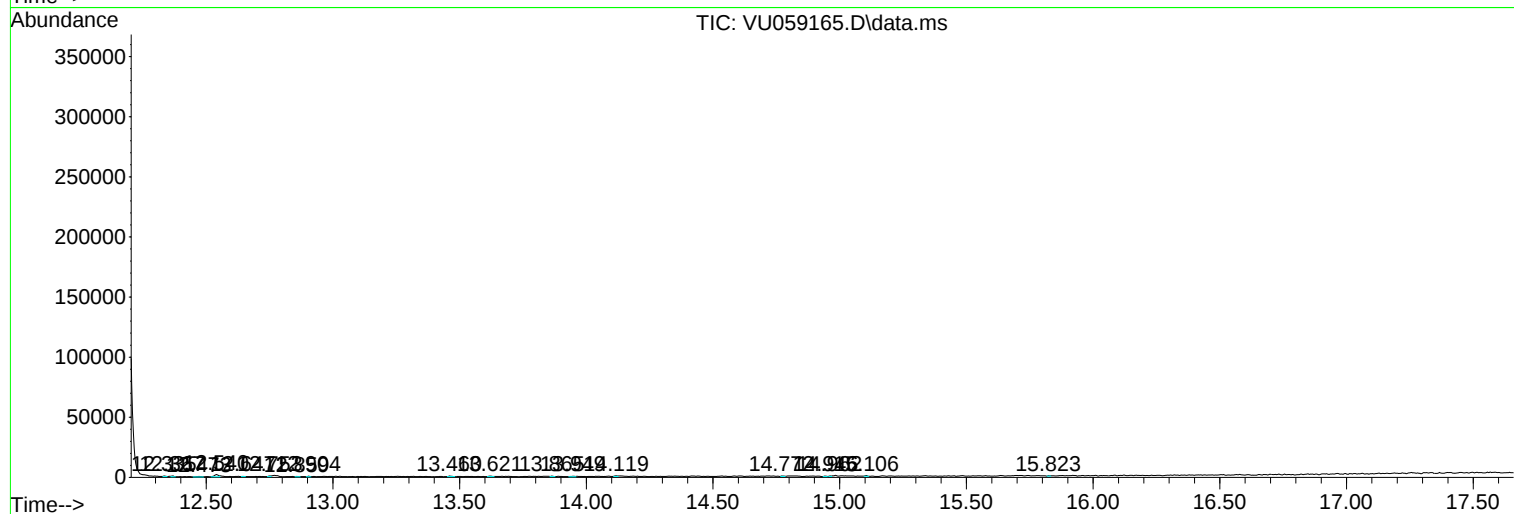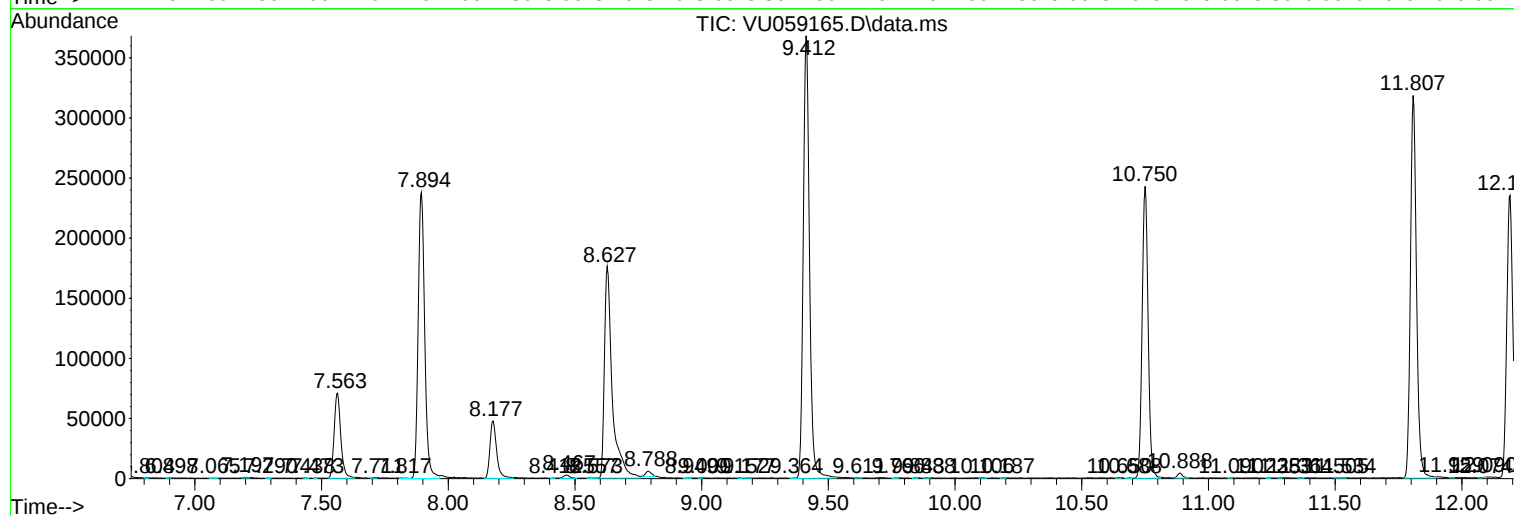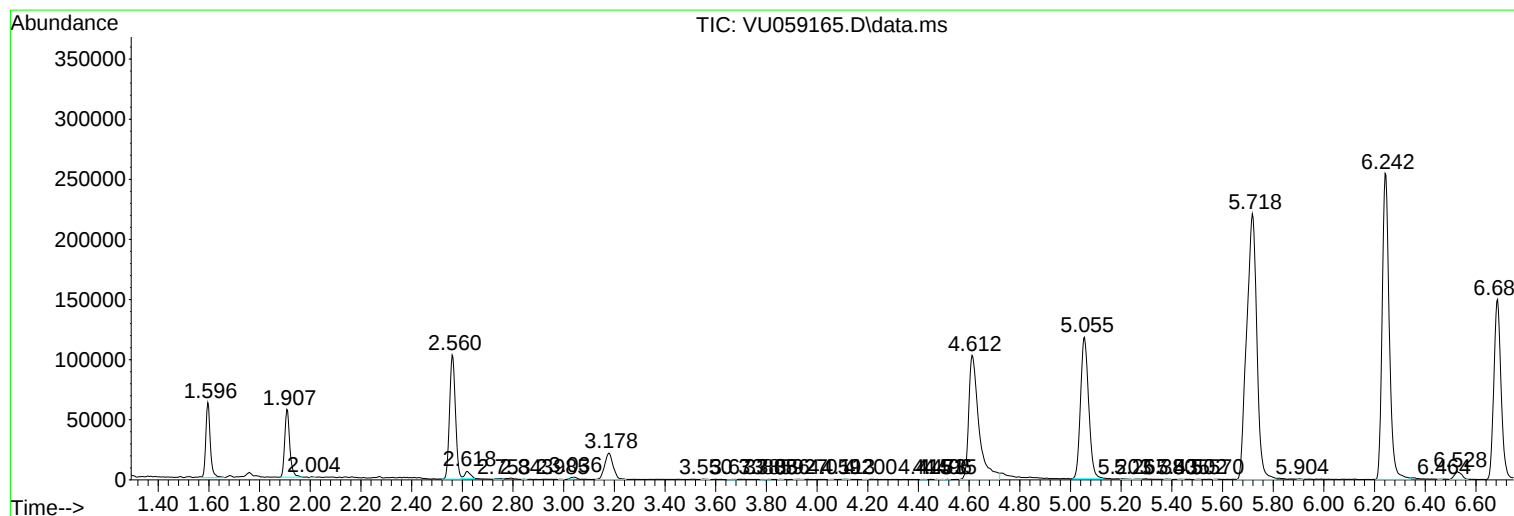

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059165.D
Acq On : 06 Jun 2024 15:12
Operator : MD/SY
Sample : P2696-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4D66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059165.D
Acq On : 06 Jun 2024 15:12
Operator : MD/SY
Sample : P2696-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4D66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc