

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059168.D
 Acq On : 06 Jun 2024 16:22
 Operator : MD/SY
 Sample : P2693-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059168.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.518	67	71	78	rBV3	1238	1631	0.25%	0.032%
2	1.595	87	95	108	rBV	58565	69159	10.80%	1.338%
3	1.763	141	147	158	rVB3	9118	11317	1.77%	0.219%
4	1.907	184	192	208	rVB	53612	73725	11.51%	1.426%
5	2.158	266	270	272	rBV3	947	851	0.13%	0.016%
6	2.560	384	395	410	rBV	98965	161665	25.24%	3.127%
7	2.724	443	446	448	rBV	216	140	0.02%	0.003%
8	2.763	456	458	460	rBV	449	194	0.03%	0.004%
9	3.039	534	544	553	rBV3	2452	4370	0.68%	0.085%
10	3.136	564	574	582	rBV3	2976	6227	0.97%	0.120%
11	3.348	637	640	642	rVB2	263	157	0.02%	0.003%
12	3.531	695	697	699	rBV	215	147	0.02%	0.003%
13	3.589	712	715	719	rVB2	221	187	0.03%	0.004%
14	3.692	743	747	752	rVB2	287	280	0.04%	0.005%
15	3.926	814	820	822	rBV2	223	234	0.04%	0.005%
16	3.994	838	841	845	rVB2	339	246	0.04%	0.005%
17	4.023	845	850	852	rBV2	276	295	0.05%	0.006%
18	4.039	852	855	858	rBV	245	167	0.03%	0.003%
19	4.480	987	992	997	rVB2	222	269	0.04%	0.005%
20	4.515	1000	1003	1008	rVB2	214	205	0.03%	0.004%
21	4.611	1023	1033	1066	rBV	81814	207671	32.42%	4.017%
22	4.997	1147	1153	1155	rBV2	368	449	0.07%	0.009%
23	5.055	1155	1171	1193	rVV	115567	257279	40.16%	4.977%
24	5.213	1218	1220	1223	rVB2	521	310	0.05%	0.006%
25	5.242	1223	1229	1232	rBV2	385	434	0.07%	0.008%
26	5.316	1250	1252	1255	rVB	372	185	0.03%	0.004%
27	5.341	1255	1260	1262	rBV2	407	329	0.05%	0.006%
28	5.505	1306	1311	1313	rBV2	225	206	0.03%	0.004%
29	5.608	1340	1343	1348	rVB	271	271	0.04%	0.005%
30	5.634	1348	1351	1354	rBV2	248	228	0.04%	0.004%
31	5.717	1358	1377	1404	rBV2	210424	590633	92.20%	11.426%
32	5.978	1455	1458	1460	rBV2	213	175	0.03%	0.003%
33	6.020	1467	1471	1474	rVB3	315	291	0.05%	0.006%
34	6.061	1482	1484	1488	rVV2	197	167	0.03%	0.003%
35	6.242	1528	1540	1562	rBV	257158	493861	77.09%	9.554%
36	6.393	1584	1587	1591	rBV3	406	362	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059168.D
 Acq On : 06 Jun 2024 16:22
 Operator : MD/SY
 Sample : P2693-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.528	1620	1629	1642	rVB4	6403	11974	1.87%	0.232%
38	6.576	1642	1644	1648	rVB	319	195	0.03%	0.004%
39	6.685	1665	1678	1700	rBV	147604	292395	45.64%	5.656%
40	6.804	1710	1715	1718	rBV3	678	603	0.09%	0.012%
41	6.823	1718	1721	1725	rVV3	398	345	0.05%	0.007%
42	6.846	1725	1728	1729	rVV2	287	141	0.02%	0.003%
43	7.055	1789	1793	1796	rBV	277	283	0.04%	0.005%
44	7.097	1803	1806	1811	rVB2	218	259	0.04%	0.005%
45	7.245	1848	1852	1854	rBV2	251	243	0.04%	0.005%
46	7.270	1857	1860	1864	rVV2	160	161	0.03%	0.003%
47	7.338	1878	1881	1886	rVB	227	187	0.03%	0.004%
48	7.428	1905	1909	1913	rBV2	176	219	0.03%	0.004%
49	7.563	1940	1951	1970	rBV2	69046	126152	19.69%	2.440%
50	7.711	1993	1997	2000	rBV2	274	257	0.04%	0.005%
51	7.894	2041	2054	2080	rBV	224590	404216	63.10%	7.820%
52	8.065	2104	2107	2114	rBV3	318	409	0.06%	0.008%
53	8.177	2131	2142	2163	rBV	47741	83996	13.11%	1.625%
54	8.312	2181	2184	2187	rBV2	247	177	0.03%	0.003%
55	8.450	2223	2227	2228	rBV2	420	279	0.04%	0.005%
56	8.470	2229	2233	2243	rVB2	1359	1708	0.27%	0.033%
57	8.592	2263	2271	2272	rBV2	198	226	0.04%	0.004%
58	8.627	2272	2282	2320	rBV2	184303	392647	61.29%	7.596%
59	8.991	2393	2395	2398	rVB2	241	138	0.02%	0.003%
60	9.010	2398	2401	2404	rBV	222	163	0.03%	0.003%
61	9.100	2425	2429	2431	rBV2	302	204	0.03%	0.004%
62	9.164	2446	2449	2453	rBV	203	142	0.02%	0.003%
63	9.412	2514	2526	2553	rBV	377657	640624	100.00%	12.393%
64	9.618	2587	2590	2594	rVB2	255	241	0.04%	0.005%
65	9.679	2606	2609	2613	rVB2	245	184	0.03%	0.004%
66	9.708	2613	2618	2625	rBV2	302	409	0.06%	0.008%
67	9.897	2672	2677	2679	rBV	175	197	0.03%	0.004%
68	10.103	2738	2741	2744	rVB2	265	150	0.02%	0.003%
69	10.280	2794	2796	2808	rVB2	331	525	0.08%	0.010%
70	10.331	2808	2812	2817	rBV2	384	482	0.08%	0.009%
71	10.479	2855	2858	2861	rBV2	353	275	0.04%	0.005%
72	10.701	2923	2927	2930	rBV	189	204	0.03%	0.004%
73	10.749	2930	2942	2961	rVV	236758	387617	60.51%	7.499%
74	10.884	2977	2984	2994	rVB3	1932	2790	0.44%	0.054%
75	10.974	3010	3012	3015	rBV	291	212	0.03%	0.004%
76	10.994	3015	3018	3021	rVV	252	164	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059168.D
 Acq On : 06 Jun 2024 16:22
 Operator : MD/SY
 Sample : P2693-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.016	3021	3025	3031	rVV2	270	315	0.05%	0.006%
78	11.129	3057	3060	3063	rBV	185	160	0.02%	0.003%
79	11.807	3259	3271	3299	rBV	318097	537037	83.83%	10.389%
80	11.952	3313	3316	3319	rBV	483	289	0.05%	0.006%
81	12.000	3329	3331	3336	rBV2	207	140	0.02%	0.003%
82	12.190	3377	3390	3407	rBV	230146	389667	60.83%	7.538%
83	12.765	3561	3569	3570	rBV2	645	704	0.11%	0.014%
84	13.698	3856	3859	3862	rBV2	305	243	0.04%	0.005%
85	13.762	3876	3879	3881	rBV	260	135	0.02%	0.003%
86	13.794	3885	3889	3892	rBV2	288	251	0.04%	0.005%
87	13.817	3892	3896	3899	rBV2	417	412	0.06%	0.008%
88	13.881	3913	3916	3918	rBV2	392	163	0.03%	0.003%
89	13.952	3935	3938	3943	rBV2	297	305	0.05%	0.006%
90	14.097	3980	3983	3985	rBV	434	303	0.05%	0.006%
91	14.206	4015	4017	4019	rBV	284	159	0.02%	0.003%
92	14.543	4119	4122	4126	rBV	359	341	0.05%	0.007%
93	14.608	4140	4142	4147	rBV3	321	222	0.03%	0.004%
94	14.646	4151	4154	4157	rBV3	436	329	0.05%	0.006%
95	14.707	4171	4173	4174	rBV	339	160	0.02%	0.003%
96	15.257	4341	4344	4346	rBV2	437	276	0.04%	0.005%
97	15.392	4383	4386	4389	rBV	400	319	0.05%	0.006%
98	16.055	4589	4592	4597	rBV3	569	641	0.10%	0.012%
99	16.112	4608	4610	4613	rVB	559	250	0.04%	0.005%
100	16.174	4626	4629	4630	rBV2	494	265	0.04%	0.005%




Sum of corrected areas: 5169196

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059168.D
Acq On : 06 Jun 2024 16:22
Operator : MD/SY
Sample : P2693-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

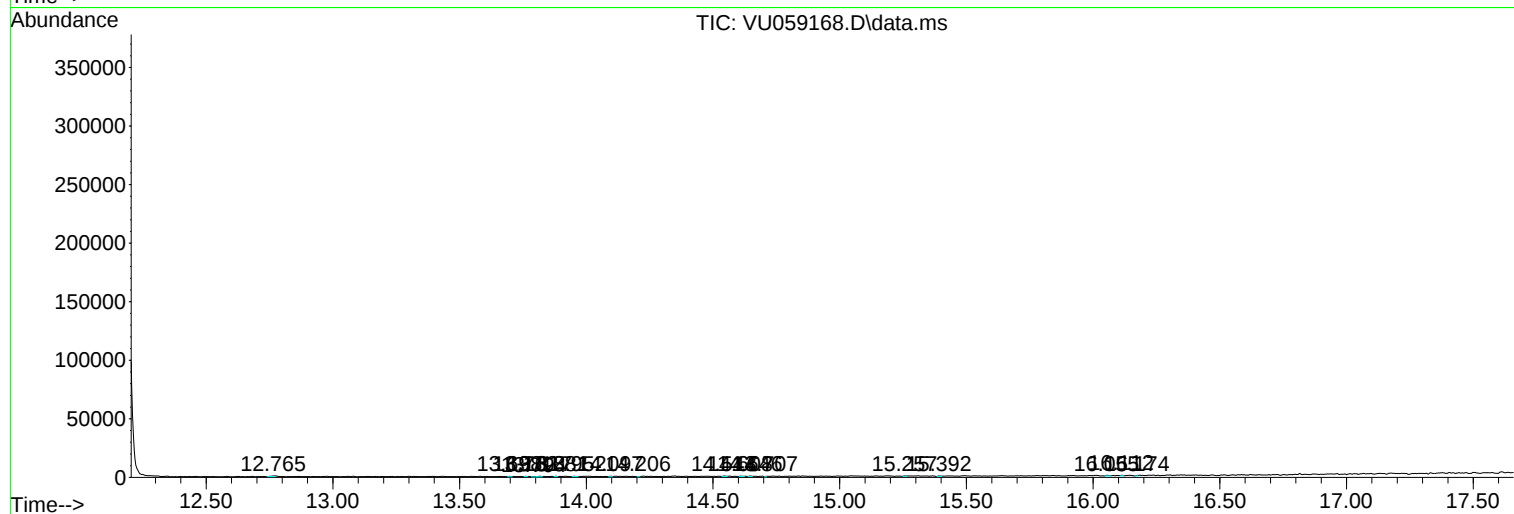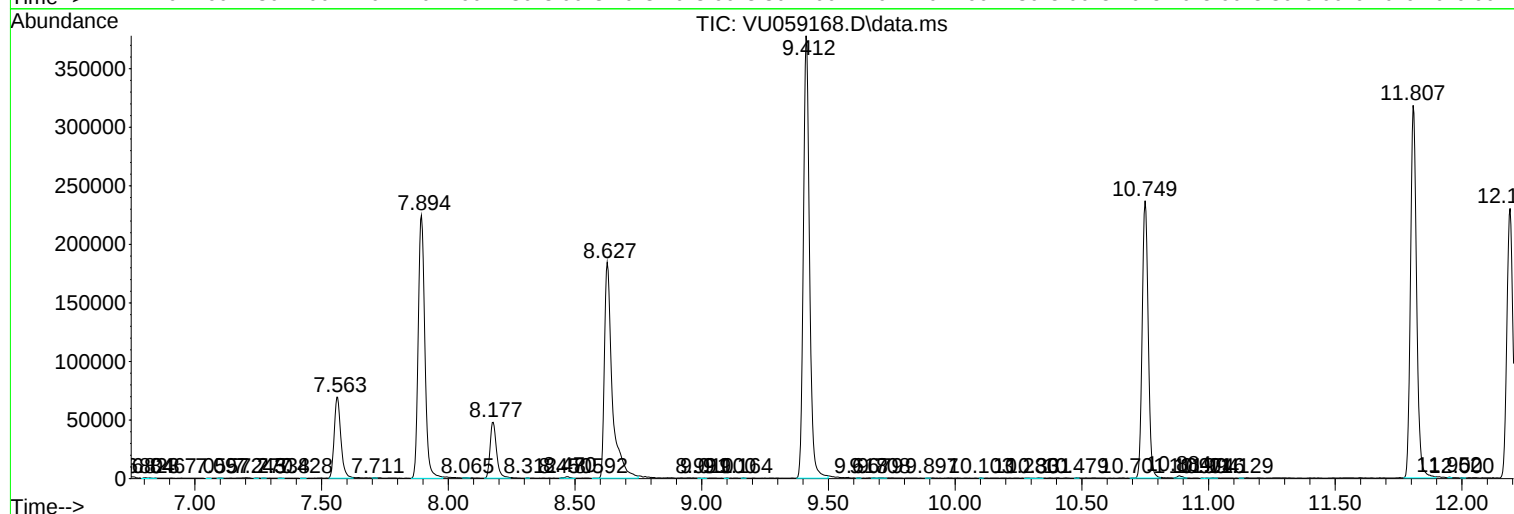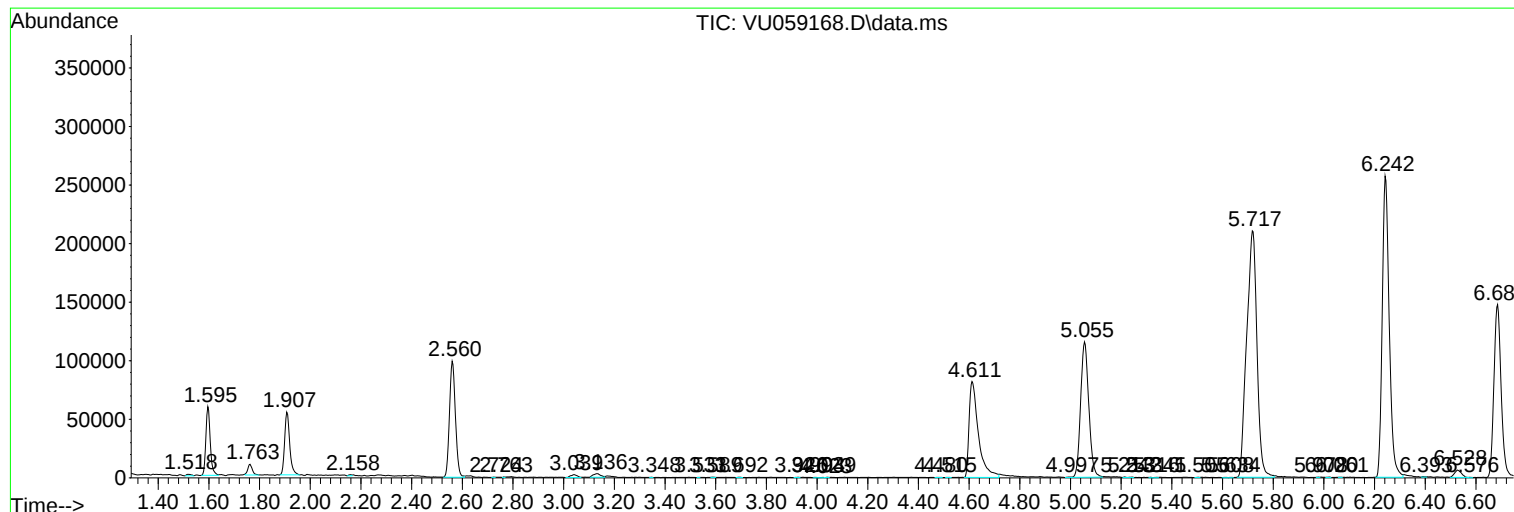

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059168.D
Acq On : 06 Jun 2024 16:22
Operator : MD/SY
Sample : P2693-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059168.D
Acq On : 06 Jun 2024 16:22
Operator : MD/SY
Sample : P2693-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------