

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059169.D
 Acq On : 06 Jun 2024 16:45
 Operator : MD/SY
 Sample : P2693-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059169.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.518	68	71	74	rBV2	1039	753	0.12%	0.015%
2	1.595	88	95	110	rVB	57699	67540	10.62%	1.310%
3	1.763	143	147	156	rVB4	7988	8420	1.32%	0.163%
4	1.907	184	192	210	rVB	52619	73252	11.52%	1.420%
5	2.406	344	347	350	rBV2	834	697	0.11%	0.014%
6	2.560	378	395	411	rBV	99490	163004	25.63%	3.161%
7	2.666	425	428	431	rBV2	356	242	0.04%	0.005%
8	2.785	461	465	470	rBV2	485	513	0.08%	0.010%
9	2.846	481	484	488	rBV	251	221	0.03%	0.004%
10	2.936	506	512	517	rVB2	340	419	0.07%	0.008%
11	2.981	521	526	531	rBV2	417	543	0.09%	0.011%
12	3.039	535	544	557	rVB6	2424	4624	0.73%	0.090%
13	3.094	557	561	562	rBV2	255	209	0.03%	0.004%
14	3.129	562	572	579	rBV4	2636	4084	0.64%	0.079%
15	3.255	608	611	614	rVB2	275	178	0.03%	0.003%
16	3.290	614	622	627	rBV2	262	418	0.07%	0.008%
17	3.525	690	695	698	rBV2	323	351	0.06%	0.007%
18	3.608	718	721	723	rBV	182	152	0.02%	0.003%
19	3.711	748	753	758	rBV2	199	244	0.04%	0.005%
20	4.052	856	859	866	rVB2	191	164	0.03%	0.003%
21	4.277	925	929	932	rBV	270	257	0.04%	0.005%
22	4.412	966	971	976	rBV2	287	357	0.06%	0.007%
23	4.570	1018	1020	1023	rVB	334	215	0.03%	0.004%
24	4.611	1023	1033	1074	rBV	79995	207167	32.57%	4.017%
25	4.978	1144	1147	1154	rVB3	387	402	0.06%	0.008%
26	5.055	1154	1171	1196	rBV	115353	260189	40.91%	5.045%
27	5.200	1213	1216	1219	rBV2	274	176	0.03%	0.003%
28	5.238	1225	1228	1231	rBV2	317	247	0.04%	0.005%
29	5.309	1245	1250	1257	rBV2	212	255	0.04%	0.005%
30	5.361	1263	1266	1271	rBV	266	294	0.05%	0.006%
31	5.441	1284	1291	1298	rVB2	303	510	0.08%	0.010%
32	5.586	1332	1336	1340	rBV	164	184	0.03%	0.004%
33	5.717	1357	1377	1398	rBV2	219387	591102	92.94%	11.461%
34	5.914	1434	1438	1443	rBV2	311	367	0.06%	0.007%
35	6.029	1468	1474	1475	rBV2	221	203	0.03%	0.004%
36	6.132	1503	1506	1509	rBV	335	280	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059169.D
 Acq On : 06 Jun 2024 16:45
 Operator : MD/SY
 Sample : P2693-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.164	1513	1516	1520	rVB2	366	273	0.04%	0.005%
38	6.245	1528	1541	1561	rBV	249129	489170	76.91%	9.485%
39	6.528	1620	1629	1643	rVB4	6067	12771	2.01%	0.248%
40	6.582	1645	1646	1651	rVB	251	150	0.02%	0.003%
41	6.685	1664	1678	1699	rBV2	144491	291082	45.77%	5.644%
42	6.820	1718	1720	1728	rVB3	412	422	0.07%	0.008%
43	7.007	1773	1778	1780	rBV2	195	159	0.02%	0.003%
44	7.168	1824	1828	1831	rBV	284	264	0.04%	0.005%
45	7.203	1831	1839	1840	rBV	505	648	0.10%	0.013%
46	7.351	1879	1885	1888	rBV2	236	247	0.04%	0.005%
47	7.512	1931	1935	1938	rBV	184	161	0.03%	0.003%
48	7.563	1939	1951	1970	rBV	70191	126788	19.93%	2.458%
49	7.766	2009	2014	2019	rBV2	163	206	0.03%	0.004%
50	7.788	2019	2021	2024	rVB	263	164	0.03%	0.003%
51	7.807	2024	2027	2028	rBV2	271	163	0.03%	0.003%
52	7.894	2041	2054	2076	rBV	227773	402979	63.36%	7.813%
53	8.094	2113	2116	2118	rVB2	305	197	0.03%	0.004%
54	8.113	2118	2122	2125	rBV	436	426	0.07%	0.008%
55	8.177	2132	2142	2164	rBV2	46042	82588	12.99%	1.601%
56	8.322	2185	2187	2190	rBV	336	218	0.03%	0.004%
57	8.376	2200	2204	2206	rBV	303	209	0.03%	0.004%
58	8.425	2215	2219	2222	rBV	333	347	0.05%	0.007%
59	8.466	2224	2232	2241	rVB2	1097	2035	0.32%	0.039%
60	8.627	2271	2282	2320	rBV2	184157	387119	60.87%	7.506%
61	8.913	2366	2371	2375	rBV2	292	252	0.04%	0.005%
62	9.042	2408	2411	2414	rVB2	279	156	0.02%	0.003%
63	9.360	2505	2510	2513	rBV	274	308	0.05%	0.006%
64	9.412	2514	2526	2556	rBV	371268	636023	100.00%	12.332%
65	9.807	2642	2649	2653	rVB2	287	413	0.06%	0.008%
66	9.913	2679	2682	2685	rBV2	247	175	0.03%	0.003%
67	10.110	2740	2743	2748	rBV	283	219	0.03%	0.004%
68	10.148	2752	2755	2756	rBV	269	175	0.03%	0.003%
69	10.421	2835	2840	2842	rBV2	436	375	0.06%	0.007%
70	10.624	2899	2903	2908	rBV	224	273	0.04%	0.005%
71	10.749	2930	2942	2962	rVV	240804	390577	61.41%	7.573%
72	10.888	2980	2985	2995	rVB2	2064	2866	0.45%	0.056%
73	11.193	3076	3080	3086	rBV	368	391	0.06%	0.008%
74	11.367	3127	3134	3138	rBV	353	429	0.07%	0.008%
75	11.515	3177	3180	3182	rBV	255	154	0.02%	0.003%
76	11.695	3233	3236	3241	rVB	314	231	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059169.D
 Acq On : 06 Jun 2024 16:45
 Operator : MD/SY
 Sample : P2693-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.724	3241	3245	3249	rBV2	262	264	0.04%	0.005%
78	11.746	3249	3252	3257	rVB2	302	231	0.04%	0.004%
79	11.807	3259	3271	3294	rBV	320782	536942	84.42%	10.411%
80	11.920	3303	3306	3311	rVB3	450	346	0.05%	0.007%
81	12.035	3340	3342	3346	rBV	201	174	0.03%	0.003%
82	12.190	3377	3390	3416	rBV	228413	392735	61.75%	7.615%
83	12.309	3424	3427	3428	rBV2	336	197	0.03%	0.004%
84	12.360	3439	3443	3446	rBV	254	264	0.04%	0.005%
85	12.415	3457	3460	3463	rBV2	284	190	0.03%	0.004%
86	12.769	3562	3570	3576	rBV2	787	1271	0.20%	0.025%
87	12.933	3618	3621	3623	rBV2	301	178	0.03%	0.003%
88	13.113	3674	3677	3681	rBV	256	225	0.04%	0.004%
89	13.331	3742	3745	3750	rBV2	272	247	0.04%	0.005%
90	13.724	3864	3867	3871	rVB2	341	291	0.05%	0.006%
91	14.386	4068	4073	4076	rBV3	435	486	0.08%	0.009%
92	14.553	4123	4125	4129	rBV2	348	241	0.04%	0.005%
93	14.579	4129	4133	4134	rBV	425	307	0.05%	0.006%
94	14.701	4169	4171	4174	rVB	415	204	0.03%	0.004%
95	14.723	4175	4178	4180	rBV2	405	302	0.05%	0.006%
96	14.894	4228	4231	4234	rBV	329	289	0.05%	0.006%
97	15.196	4321	4325	4328	rBV2	411	393	0.06%	0.008%
98	16.183	4629	4632	4633	rBV2	596	341	0.05%	0.007%
99	16.595	4757	4760	4768	rBV5	802	929	0.15%	0.018%
100	16.842	4834	4837	4838	rBV2	764	453	0.07%	0.009%




Sum of corrected areas: 5157536

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059169.D
Acq On : 06 Jun 2024 16:45
Operator : MD/SY
Sample : P2693-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

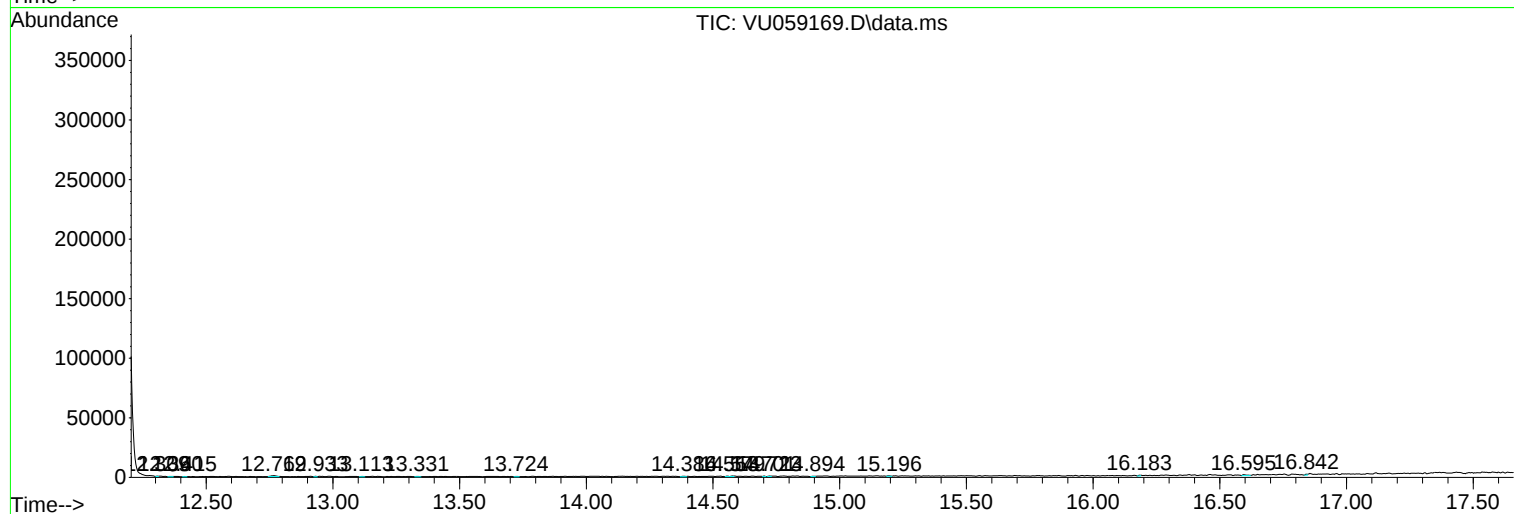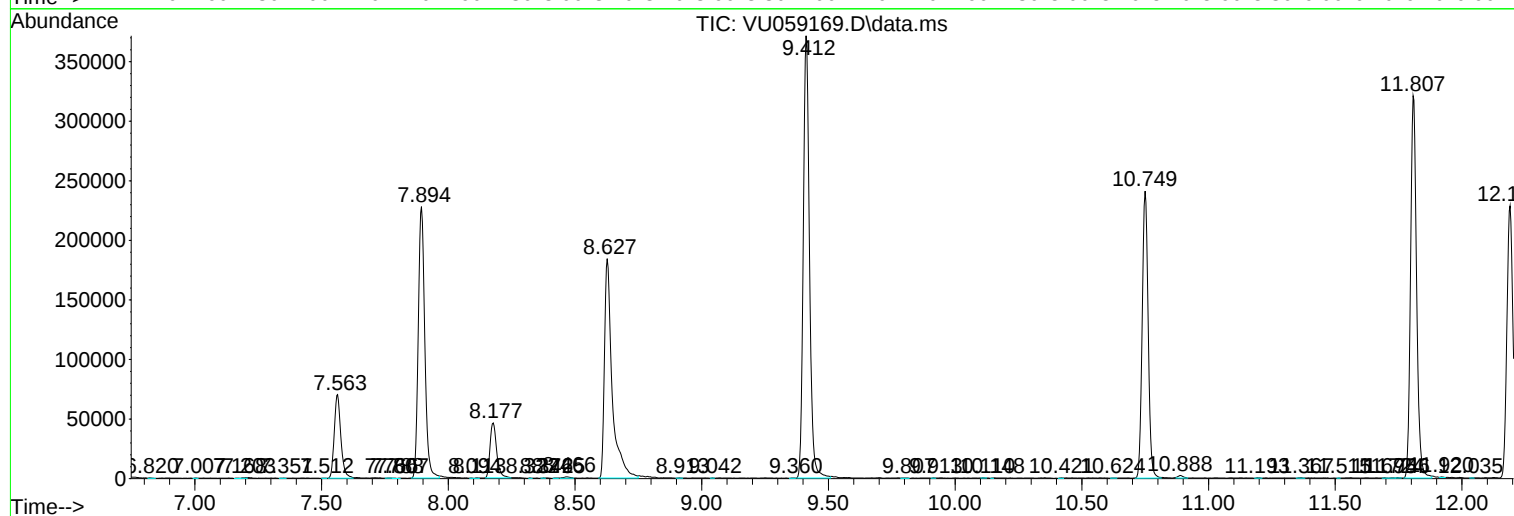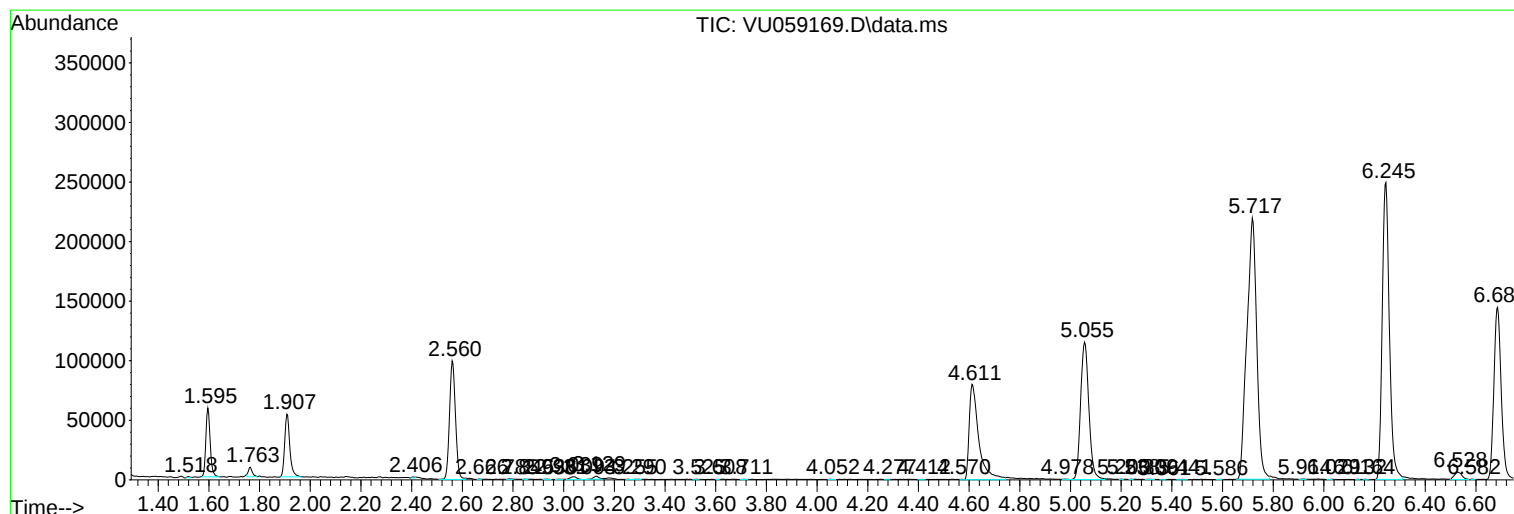

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059169.D
Acq On : 06 Jun 2024 16:45
Operator : MD/SY
Sample : P2693-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059169.D
Acq On : 06 Jun 2024 16:45
Operator : MD/SY
Sample : P2693-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------