

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059170.D
 Acq On : 06 Jun 2024 17:08
 Operator : MD/SY
 Sample : P2693-01 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.483	58	60	66	rBV2	857	628	0.10%	0.012%
2	1.595	87	95	116	rVB	60765	73017	11.80%	1.419%
3	1.763	141	147	153	rBV3	6238	7345	1.19%	0.143%
4	1.907	183	192	211	rBV	55032	77008	12.44%	1.496%
5	2.560	383	395	415	rBV	100857	164520	26.58%	3.197%
6	2.711	437	442	445	rVV2	158	190	0.03%	0.004%
7	2.756	454	456	460	rBV2	240	158	0.03%	0.003%
8	2.785	460	465	470	rBV2	532	699	0.11%	0.014%
9	2.843	481	483	487	rBV2	202	187	0.03%	0.004%
10	3.039	532	544	557	rVV2	5992	11608	1.88%	0.226%
11	3.174	578	586	593	rBV3	738	1196	0.19%	0.023%
12	3.300	619	625	626	rBV	253	214	0.03%	0.004%
13	3.354	637	642	645	rBV3	456	372	0.06%	0.007%
14	3.509	684	690	694	rBV2	455	594	0.10%	0.012%
15	3.592	714	716	724	rVB	245	292	0.05%	0.006%
16	3.682	738	744	748	rBV2	127	186	0.03%	0.004%
17	3.865	798	801	811	rVB2	322	495	0.08%	0.010%
18	4.020	843	849	851	rBV2	139	160	0.03%	0.003%
19	4.283	927	931	937	rVB2	235	273	0.04%	0.005%
20	4.322	937	943	947	rBV2	206	215	0.03%	0.004%
21	4.348	948	951	956	rBV2	220	200	0.03%	0.004%
22	4.406	966	969	974	rBV2	199	192	0.03%	0.004%
23	4.447	979	982	986	rVB	316	209	0.03%	0.004%
24	4.611	1023	1033	1061	rBV2	78975	199187	32.18%	3.871%
25	5.055	1155	1171	1193	rBV	115011	257648	41.63%	5.007%
26	5.168	1204	1206	1209	rVB2	299	178	0.03%	0.003%
27	5.187	1209	1212	1214	rBV3	255	166	0.03%	0.003%
28	5.232	1222	1226	1230	rBV3	276	228	0.04%	0.004%
29	5.399	1275	1278	1283	rVB2	213	202	0.03%	0.004%
30	5.528	1312	1318	1319	rBV2	356	316	0.05%	0.006%
31	5.595	1336	1339	1345	rBV2	176	195	0.03%	0.004%
32	5.647	1352	1355	1357	rBV2	256	164	0.03%	0.003%
33	5.717	1358	1377	1409	rBV2	213027	599179	96.82%	11.643%
34	6.107	1496	1498	1503	rVB2	255	244	0.04%	0.005%
35	6.145	1503	1510	1512	rBV2	229	316	0.05%	0.006%
36	6.158	1512	1514	1520	rVB2	173	174	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059170.D
 Acq On : 06 Jun 2024 17:08
 Operator : MD/SY
 Sample : P2693-01 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.190	1520	1524	1528	rBV2	167	152	0.02%	0.003%
38	6.242	1528	1540	1569	rBV	246761	483179	78.07%	9.389%
39	6.531	1619	1630	1643	rVB5	6323	13075	2.11%	0.254%
40	6.685	1665	1678	1701	rBV2	146925	290531	46.94%	5.645%
41	6.804	1712	1715	1720	rVB3	584	526	0.08%	0.010%
42	6.862	1729	1733	1738	rBV2	271	220	0.04%	0.004%
43	6.898	1741	1744	1748	rVB2	202	155	0.03%	0.003%
44	6.962	1756	1764	1767	rBV	402	408	0.07%	0.008%
45	7.100	1804	1807	1810	rBV2	209	182	0.03%	0.004%
46	7.142	1814	1820	1824	rVB	232	294	0.05%	0.006%
47	7.164	1824	1827	1832	rBV	231	251	0.04%	0.005%
48	7.193	1832	1836	1842	rBV4	540	813	0.13%	0.016%
49	7.396	1894	1899	1901	rBV	188	167	0.03%	0.003%
50	7.431	1906	1910	1914	rVV2	172	151	0.02%	0.003%
51	7.560	1939	1950	1974	rBV2	70269	127942	20.67%	2.486%
52	7.711	1990	1997	2000	rBV4	408	565	0.09%	0.011%
53	7.750	2007	2009	2015	rVB3	326	200	0.03%	0.004%
54	7.894	2038	2054	2074	rBV	231028	410745	66.37%	7.981%
55	8.078	2109	2111	2119	rVB2	339	376	0.06%	0.007%
56	8.135	2125	2129	2132	rVB3	170	152	0.02%	0.003%
57	8.177	2132	2142	2157	rBV	46967	83858	13.55%	1.629%
58	8.370	2199	2202	2206	rVB2	398	264	0.04%	0.005%
59	8.402	2206	2212	2216	rBV3	470	532	0.09%	0.010%
60	8.463	2226	2231	2238	rBV2	557	764	0.12%	0.015%
61	8.547	2255	2257	2260	rVB2	293	203	0.03%	0.004%
62	8.566	2260	2263	2267	rBV2	226	228	0.04%	0.004%
63	8.627	2272	2282	2319	rBV2	181629	390900	63.16%	7.596%
64	9.348	2503	2506	2509	rBV2	181	194	0.03%	0.004%
65	9.412	2513	2526	2555	rBV	359568	618889	100.00%	12.026%
66	9.692	2608	2613	2616	rBV2	291	318	0.05%	0.006%
67	9.711	2616	2619	2622	rVB	484	355	0.06%	0.007%
68	9.782	2638	2641	2644	rBV	289	244	0.04%	0.005%
69	9.836	2655	2658	2659	rBV	290	188	0.03%	0.004%
70	9.933	2682	2688	2690	rBV2	271	313	0.05%	0.006%
71	10.026	2714	2717	2721	rBV	365	231	0.04%	0.004%
72	10.103	2735	2741	2743	rBV2	341	340	0.05%	0.007%
73	10.261	2787	2790	2792	rBV	274	184	0.03%	0.004%
74	10.383	2821	2828	2832	rVB2	400	514	0.08%	0.010%
75	10.444	2843	2847	2851	rVB	286	219	0.04%	0.004%
76	10.470	2851	2855	2856	rBV	219	166	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059170.D
 Acq On : 06 Jun 2024 17:08
 Operator : MD/SY
 Sample : P2693-01 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

77	10.749	2929	2942	2962	rBV	246190	395165	63.85%	7.679%
78	10.849	2970	2973	2978	rBV2	434	457	0.07%	0.009%
79	10.881	2978	2983	2987	rVV2	490	497	0.08%	0.010%
80	11.479	3166	3169	3173	rVB2	369	273	0.04%	0.005%
81	11.560	3191	3194	3196	rBV	307	224	0.04%	0.004%
82	11.740	3247	3250	3251	rBV2	343	213	0.03%	0.004%
83	11.807	3260	3271	3288	rBV	313378	520156	84.05%	10.107%
84	11.936	3309	3311	3315	rVB2	480	297	0.05%	0.006%
85	12.029	3338	3340	3343	rVB2	315	158	0.03%	0.003%
86	12.113	3363	3366	3369	rBV	360	213	0.03%	0.004%
87	12.190	3378	3390	3415	rBV	230874	396739	64.11%	7.709%
88	12.672	3531	3540	3544	rBV2	377	636	0.10%	0.012%
89	12.765	3564	3569	3575	rVB3	642	793	0.13%	0.015%
90	13.200	3701	3704	3707	rVB	362	195	0.03%	0.004%
91	13.296	3729	3734	3739	rBV2	370	492	0.08%	0.010%
92	13.341	3744	3748	3750	rBV	355	310	0.05%	0.006%
93	13.511	3797	3801	3803	rBV	314	247	0.04%	0.005%
94	14.132	3992	3994	3996	rBV	389	189	0.03%	0.004%
95	14.174	4002	4007	4012	rBV2	312	393	0.06%	0.008%
96	14.273	4036	4038	4043	rBV2	315	252	0.04%	0.005%
97	14.299	4043	4046	4052	rVV3	309	300	0.05%	0.006%
98	14.582	4130	4134	4135	rBV	276	199	0.03%	0.004%
99	14.884	4224	4228	4230	rBV2	403	331	0.05%	0.006%
100	15.823	4518	4520	4524	rBV2	443	394	0.06%	0.008%




Sum of corrected areas: 5146266

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059170.D
Acq On : 06 Jun 2024 17:08
Operator : MD/SY
Sample : P2693-01 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

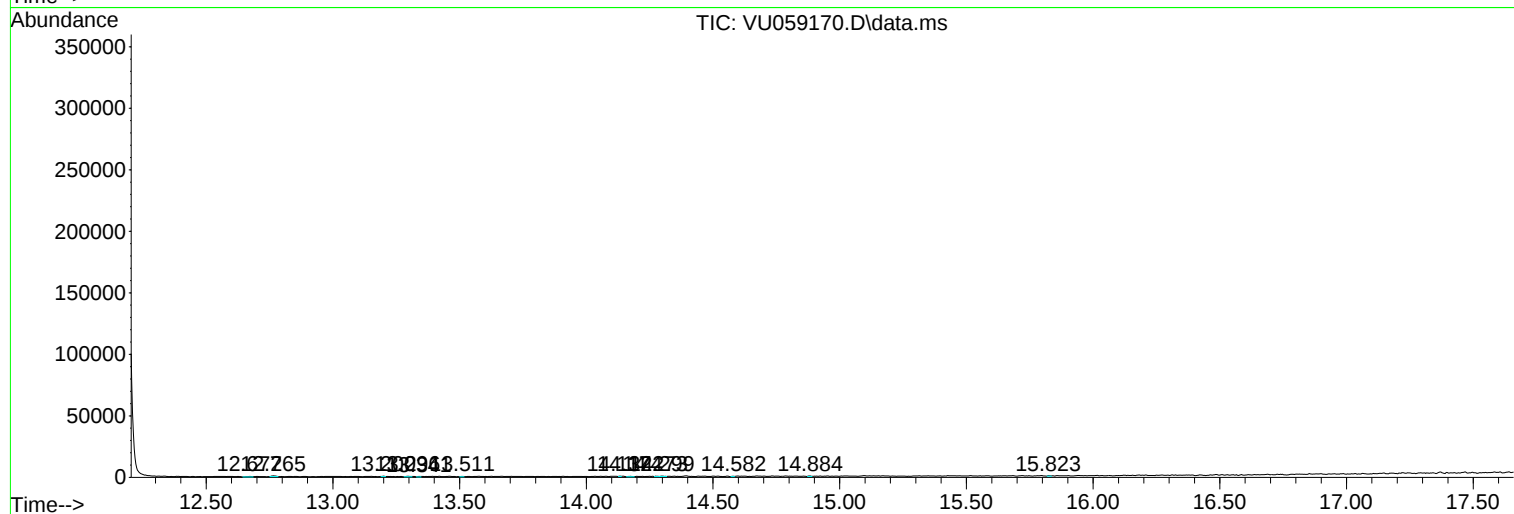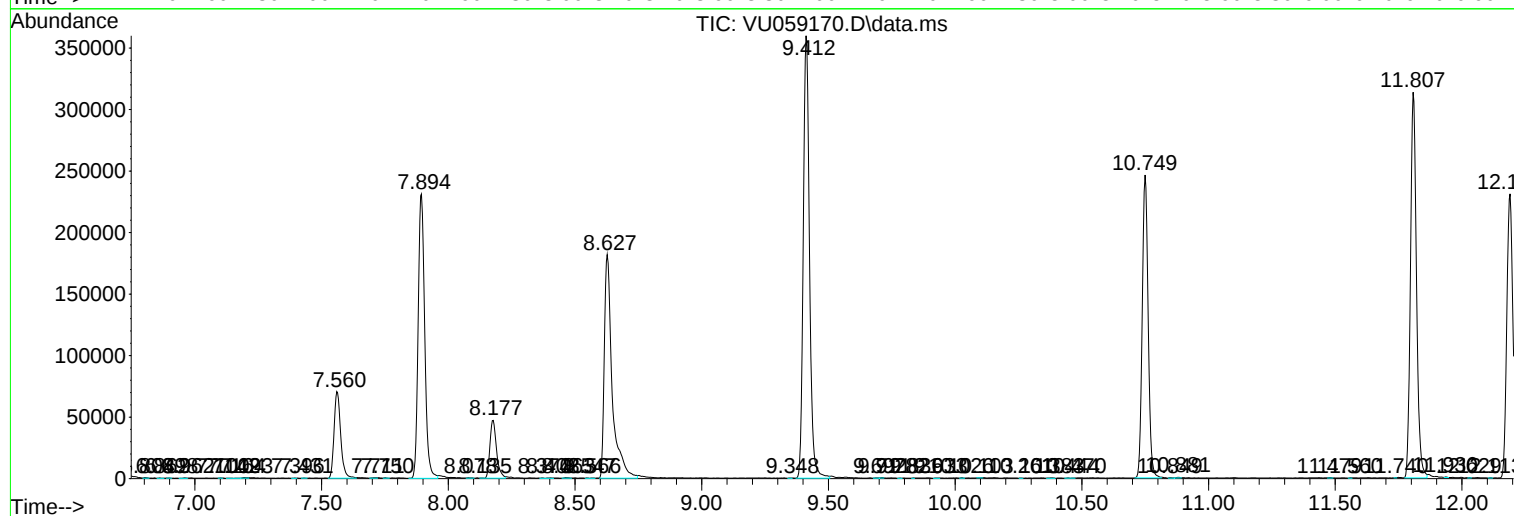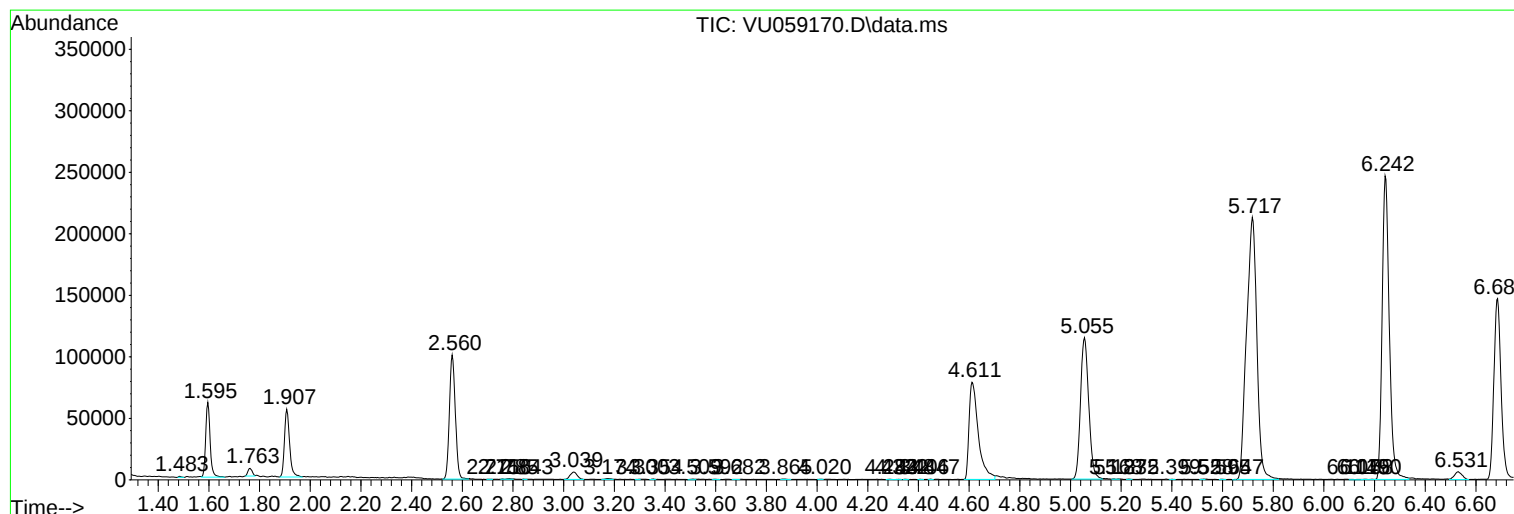

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059170.D
Acq On : 06 Jun 2024 17:08
Operator : MD/SY
Sample : P2693-01 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059170.D
Acq On : 06 Jun 2024 17:08
Operator : MD/SY
Sample : P2693-01 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------