

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059174.D
 Acq On : 06 Jun 2024 18:41
 Operator : MD/SY
 Sample : P2693-02 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059174.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	110	rBV	57735	68931	11.02%	1.337%
2	1.907	184	192	211	rVB	53305	72526	11.60%	1.407%
3	2.290	309	311	316	rBV2	556	417	0.07%	0.008%
4	2.560	383	395	409	rBV	98641	159025	25.43%	3.085%
5	2.750	450	454	458	rBV	361	356	0.06%	0.007%
6	2.769	458	460	465	rVB2	293	203	0.03%	0.004%
7	2.981	523	526	532	rVB2	227	242	0.04%	0.005%
8	3.039	532	544	561	rVB2	11318	20654	3.30%	0.401%
9	3.107	561	565	570	rBV	302	323	0.05%	0.006%
10	3.145	574	577	581	rVB2	226	167	0.03%	0.003%
11	3.171	581	585	587	rBV	512	423	0.07%	0.008%
12	3.296	621	624	631	rVB2	215	208	0.03%	0.004%
13	3.332	631	635	640	rVB2	255	275	0.04%	0.005%
14	3.432	664	666	670	rVB	235	181	0.03%	0.004%
15	3.454	670	673	675	rBV	323	211	0.03%	0.004%
16	3.493	679	685	688	rBV2	211	241	0.04%	0.005%
17	3.795	774	779	782	rBV	167	202	0.03%	0.004%
18	3.856	793	798	801	rBV2	221	172	0.03%	0.003%
19	4.116	876	879	883	rBV	252	234	0.04%	0.005%
20	4.152	887	890	893	rVV	304	267	0.04%	0.005%
21	4.171	893	896	902	rVB2	257	335	0.05%	0.006%
22	4.200	902	905	911	rBV2	271	301	0.05%	0.006%
23	4.239	911	917	922	rVV2	246	387	0.06%	0.008%
24	4.284	926	931	934	rBV	282	326	0.05%	0.006%
25	4.309	934	939	941	rVV2	187	196	0.03%	0.004%
26	4.374	956	959	967	rVV2	206	242	0.04%	0.005%
27	4.531	1004	1008	1012	rVV2	170	189	0.03%	0.004%
28	4.612	1023	1033	1076	rBV2	85017	214429	34.29%	4.159%
29	5.055	1154	1171	1195	rBV	114610	256104	40.95%	4.968%
30	5.177	1206	1209	1215	rVB3	479	473	0.08%	0.009%
31	5.210	1217	1219	1224	rVB3	331	217	0.03%	0.004%
32	5.242	1224	1229	1234	rBV2	453	367	0.06%	0.007%
33	5.284	1237	1242	1245	rBV2	251	276	0.04%	0.005%
34	5.390	1272	1275	1281	rVB2	194	174	0.03%	0.003%
35	5.425	1282	1286	1289	rBV2	180	178	0.03%	0.003%
36	5.476	1295	1302	1306	rBV2	295	370	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059174.D
 Acq On : 06 Jun 2024 18:41
 Operator : MD/SY
 Sample : P2693-02 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	5.541	1318	1322	1326	rBV2	213	271	0.04%	0.005%
38	5.611	1341	1344	1347	rBV2	193	180	0.03%	0.003%
39	5.718	1357	1377	1410	rVV3	211894	594301	95.03%	11.527%
40	5.907	1434	1436	1441	rVB3	386	246	0.04%	0.005%
41	5.952	1447	1450	1454	rBV2	349	285	0.05%	0.006%
42	6.242	1528	1540	1566	rBV	249109	483877	77.37%	9.386%
43	6.525	1620	1628	1629	rBV5	5912	5948	0.95%	0.115%
44	6.682	1665	1677	1703	rBV	146735	291560	46.62%	5.655%
45	6.808	1715	1716	1721	rVB2	480	172	0.03%	0.003%
46	6.840	1721	1726	1733	rVB3	387	593	0.09%	0.012%
47	6.894	1740	1743	1746	rVB	211	166	0.03%	0.003%
48	6.984	1768	1771	1775	rBV	253	221	0.04%	0.004%
49	7.116	1808	1812	1815	rBV	278	268	0.04%	0.005%
50	7.193	1831	1836	1838	rBV2	754	581	0.09%	0.011%
51	7.238	1846	1850	1853	rVB2	285	234	0.04%	0.005%
52	7.560	1936	1950	1978	rBV	68265	125435	20.06%	2.433%
53	7.660	1978	1981	1984	rVB	483	294	0.05%	0.006%
54	7.711	1992	1997	2003	rVB3	599	763	0.12%	0.015%
55	7.894	2041	2054	2077	rBV	225449	399685	63.91%	7.752%
56	8.177	2127	2142	2162	rBV	46411	84478	13.51%	1.639%
57	8.380	2200	2205	2206	rBV	282	182	0.03%	0.004%
58	8.627	2271	2282	2321	rVV	193903	404235	64.64%	7.841%
59	8.885	2360	2362	2367	rVB2	289	212	0.03%	0.004%
60	8.994	2393	2396	2399	rVV2	231	168	0.03%	0.003%
61	9.020	2401	2404	2410	rVB2	257	207	0.03%	0.004%
62	9.139	2437	2441	2444	rVB2	265	205	0.03%	0.004%
63	9.412	2513	2526	2555	rBV	368589	625395	100.00%	12.130%
64	9.753	2629	2632	2634	rBV2	300	195	0.03%	0.004%
65	10.299	2797	2802	2804	rBV2	226	227	0.04%	0.004%
66	10.399	2830	2833	2836	rBV2	282	199	0.03%	0.004%
67	10.496	2860	2863	2867	rBV	344	328	0.05%	0.006%
68	10.521	2867	2871	2874	rVB2	306	225	0.04%	0.004%
69	10.672	2911	2918	2921	rBV2	242	280	0.04%	0.005%
70	10.750	2929	2942	2962	rBV	241182	395794	63.29%	7.677%
71	11.023	3018	3027	3035	rBV	439	708	0.11%	0.014%
72	11.081	3042	3045	3048	rBV2	222	171	0.03%	0.003%
73	11.258	3096	3100	3103	rBV	263	187	0.03%	0.004%
74	11.332	3119	3123	3127	rBV2	267	297	0.05%	0.006%
75	11.450	3157	3160	3163	rBV2	264	192	0.03%	0.004%
76	11.495	3171	3174	3180	rVB2	380	356	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
 Data File : VU059174.D
 Acq On : 06 Jun 2024 18:41
 Operator : MD/SY
 Sample : P2693-02 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.528	3180	3184	3187	rVB2	361	316	0.05%	0.006%
78	11.547	3187	3190	3193	rBV	368	306	0.05%	0.006%
79	11.807	3259	3271	3295	rBV	324748	535361	85.60%	10.384%
80	11.987	3325	3327	3331	rBV	317	213	0.03%	0.004%
81	12.103	3359	3363	3366	rBV	277	229	0.04%	0.004%
82	12.190	3377	3390	3408	rBV	233035	393471	62.92%	7.632%
83	12.479	3477	3480	3483	rBV2	335	232	0.04%	0.004%
84	12.608	3515	3520	3523	rBV	358	403	0.06%	0.008%
85	12.647	3529	3532	3535	rBV2	261	208	0.03%	0.004%
86	12.769	3563	3570	3574	rBV2	640	741	0.12%	0.014%
87	12.820	3583	3586	3590	rBV	303	220	0.04%	0.004%
88	12.859	3595	3598	3602	rBV2	313	281	0.04%	0.005%
89	12.997	3638	3641	3645	rBV2	226	217	0.03%	0.004%
90	13.499	3793	3797	3804	rBV	284	360	0.06%	0.007%
91	13.531	3804	3807	3809	rBV	324	221	0.04%	0.004%
92	13.688	3850	3856	3859	rBV	442	444	0.07%	0.009%
93	13.923	3925	3929	3931	rBV2	421	316	0.05%	0.006%
94	14.039	3963	3965	3968	rVB	433	241	0.04%	0.005%
95	14.190	4006	4012	4017	rBV6	937	1262	0.20%	0.024%
96	14.601	4137	4140	4144	rBV2	338	307	0.05%	0.006%
97	14.711	4170	4174	4175	rBV2	299	238	0.04%	0.005%
98	15.614	4453	4455	4458	rVB3	591	295	0.05%	0.006%
99	15.913	4546	4548	4549	rBV	421	190	0.03%	0.004%
100	16.556	4746	4748	4750	rBV	606	351	0.06%	0.007%




Sum of corrected areas: 5155566

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059174.D
Acq On : 06 Jun 2024 18:41
Operator : MD/SY
Sample : P2693-02 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

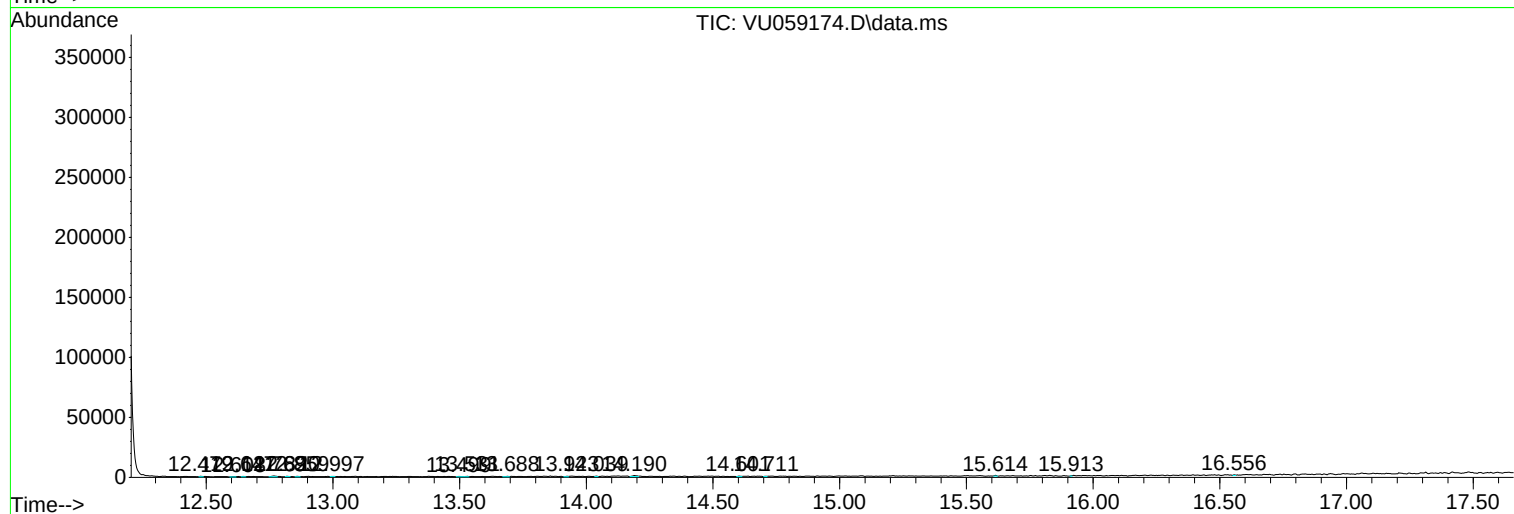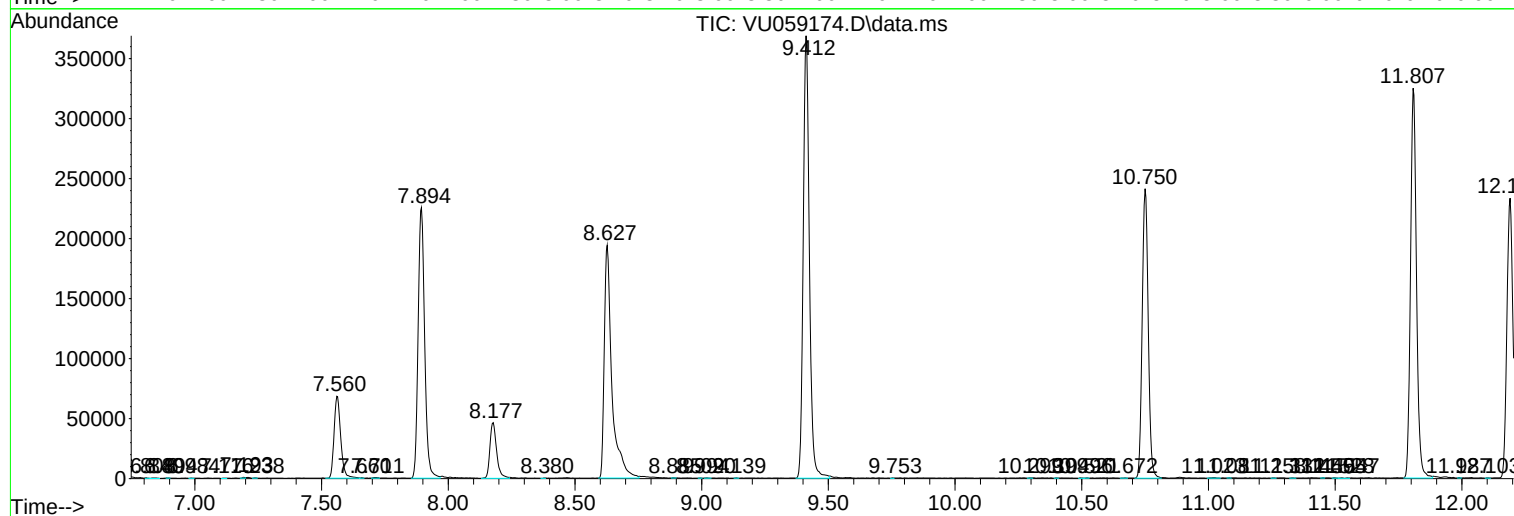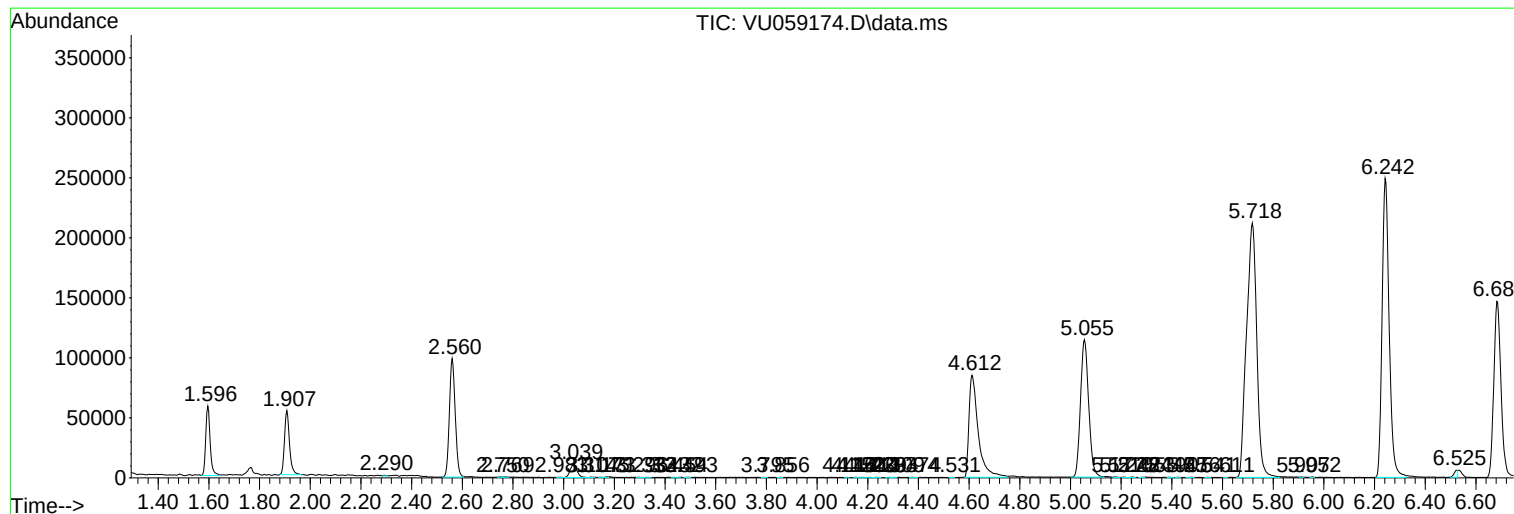

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059174.D
Acq On : 06 Jun 2024 18:41
Operator : MD/SY
Sample : P2693-02 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060624\
Data File : VU059174.D
Acq On : 06 Jun 2024 18:41
Operator : MD/SY
Sample : P2693-02 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------