

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061024\
 Data File : VU059197.D
 Acq On : 10 Jun 2024 10:25
 Operator : MD/SY
 Sample : VU0610MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jun 11 06:01:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 11 05:56:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	304239	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	289138	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	137280	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	87578	48.077	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	96.160%		
7) Chloroethane-d5	1.882	69	83042	53.218	ug/L	-0.03
Spiked Amount 50.000	Range 70 - 130		Recovery =	106.440%		
11) 1,1-Dichloroethene-d2	2.554	63	119222	33.158	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	66.320%		
21) 2-Butanone-d5	4.611	46	133849	77.956	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	77.960%		
24) Chloroform-d	5.052	84	163469	45.078	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.160%		
26) 1,2-Dichloroethane-d4	5.692	65	105297	47.375	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.760%		
32) Benzene-d6	5.717	84	345592	52.077	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	104.160%		
36) 1,2-Dichloropropane-d6	6.682	67	109942	48.049	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	96.100%		
41) Toluene-d8	7.891	98	299346	53.137	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.280%		
43) trans-1,3-Dichloroprop...	8.174	79	43540	47.075	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.160%		
47) 2-Hexanone-d5	8.627	63	93965	88.805	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	88.810%		
56) 1,1,2,2-Tetrachloroeth...	10.749	84	165934	42.849	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	85.700%		
66) 1,2-Dichlorobenzene-d4	12.187	152	111360	54.357	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.720%		
Target Compounds						Qvalue
37) 1,2-Dichloropropane	6.679	63	11218	3.784	ug/L	# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061024\
Data File : VU059197.D
Acq On : 10 Jun 2024 10:25
Operator : MD/SY
Sample : VU0610MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jun 11 06:01:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 11 05:56:14 2024
Response via : Initial Calibration

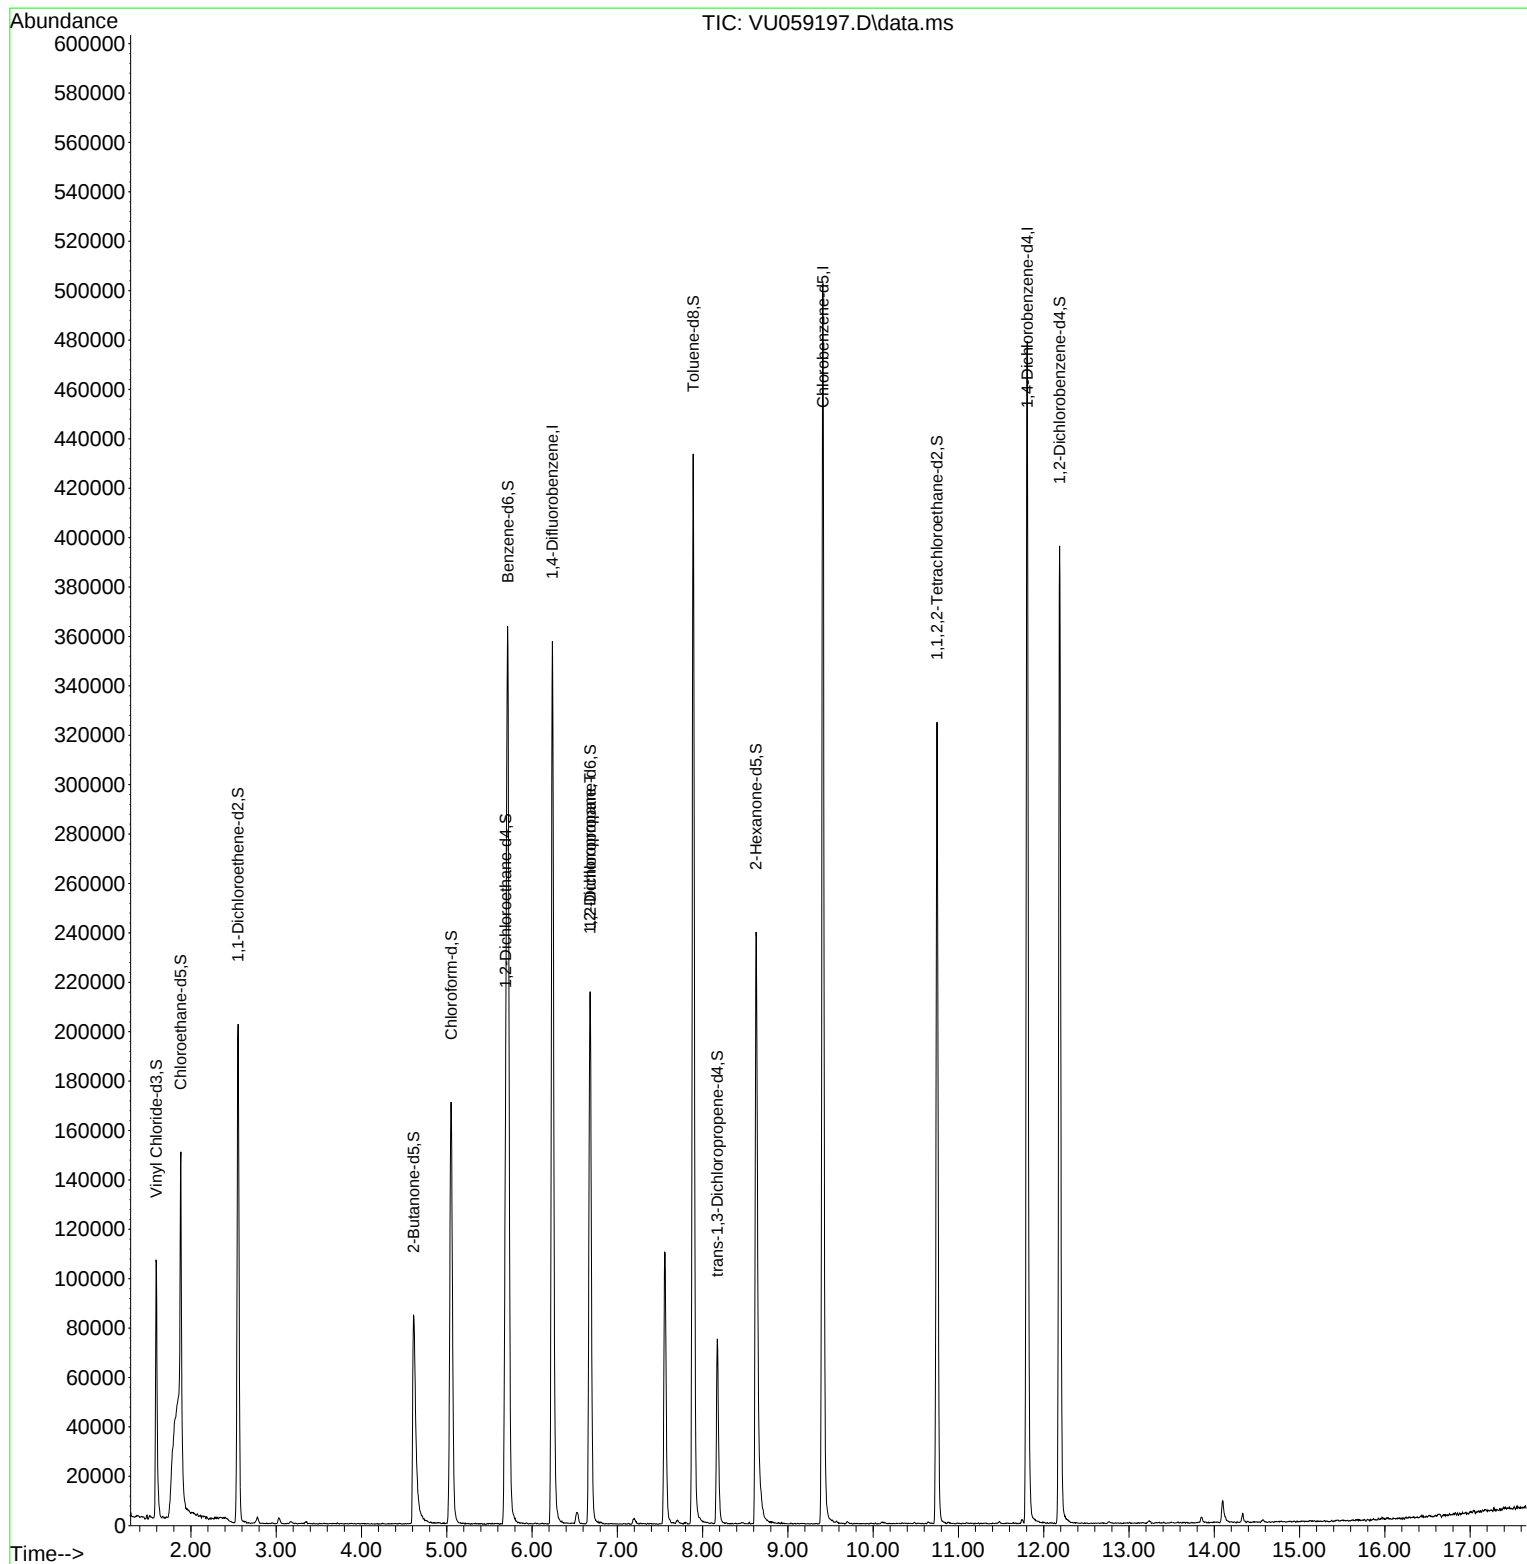

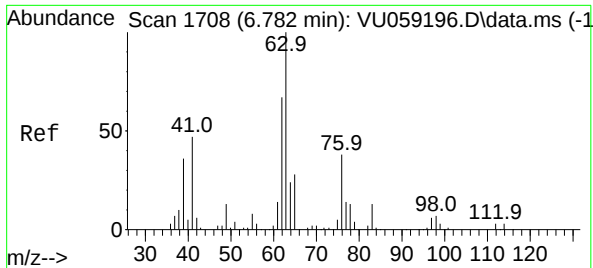

#37
 1,2-Dichloropropane
 Concen: 3.784 ug/L
 RT: 6.679 min Scan# 1
 Delta R.T. -0.103 min
 Lab File: VU059197.D
 Acq: 10 Jun 2024 10:25

Instrument :
 MSVOA_U
 ClientSampleId :

Tgt Ion: 63 Resp: 11218
 Ion Ratio Lower Upper
 63 100
 112 0.0 2.6 4.0#

