

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061024\
 Data File : VU059200.D
 Acq On : 10 Jun 2024 11:36
 Operator : MD/SY
 Sample : P2754-03ME
 Misc : 3.32g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jun 11 06:02:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 11 05:56:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	310947	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	305996	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	142052	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	51118	27.457	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	54.920%#
7) Chloroethane-d5	1.911	69	51798	32.479	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	64.960%#
11) 1,1-Dichloroethene-d2	2.563	63	78955	21.485	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	42.960%#
21) 2-Butanone-d5	4.611	46	130698	74.479	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	74.480%
24) Chloroform-d	5.055	84	147859	39.894	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.780%
26) 1,2-Dichloroethane-d4	5.695	65	90927	40.027	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.060%
32) Benzene-d6	5.721	84	266684	37.972	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.940%
36) 1,2-Dichloropropane-d6	6.685	67	94720	39.116	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	78.240%
41) Toluene-d8	7.894	98	225611	37.842	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	75.680%#
43) trans-1,3-Dichloroprop...	8.177	79	37956	38.777	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.560%
47) 2-Hexanone-d5	8.627	63	80703	72.070	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	72.070%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	163217	39.826	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	79.660%
66) 1,2-Dichlorobenzene-d4	12.187	152	98244	46.344	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.680%
Target Compounds						
					Qvalue	
60) 1,2,3-Trichloropropane	11.807	75	16731	4.235	ug/L #	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061024\
Data File : VU059200.D
Acq On : 10 Jun 2024 11:36
Operator : MD/SY
Sample : P2754-03ME
Misc : 3.32g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Jun 11 06:02:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 11 05:56:14 2024
Response via : Initial Calibration

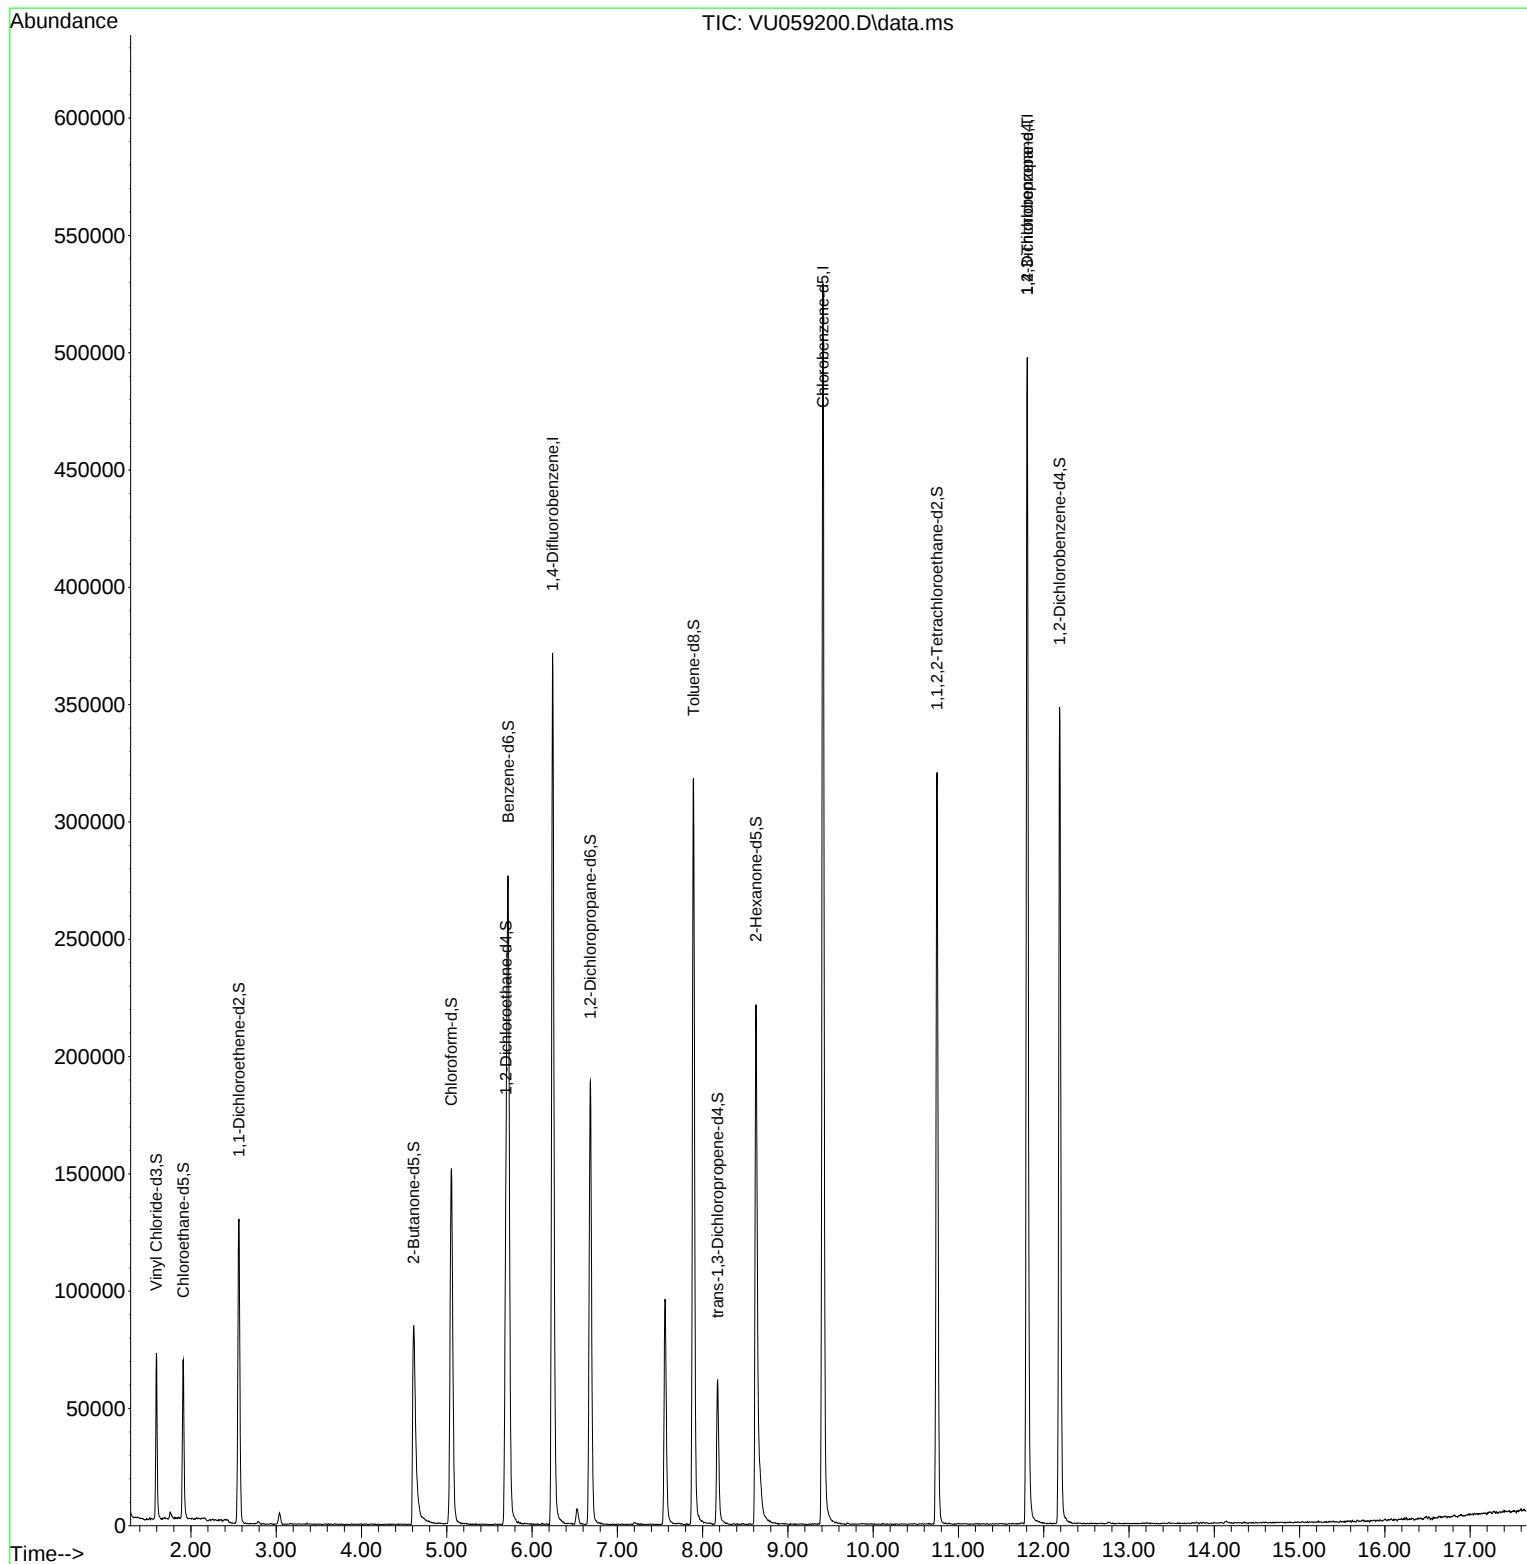

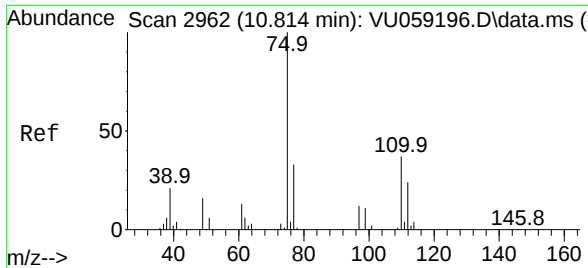

#60
 1,2,3-Trichloropropane
 Concen: 4.235 ug/L
 RT: 11.807 min Scan# 31
 Delta R.T. 0.993 min
 Lab File: VU059200.D
 Acq: 10 Jun 2024 11:36

Instrument :
 MSVOA_U
 ClientSampleId :

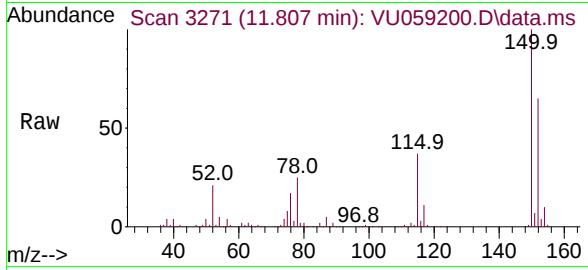

Tgt Ion: 75 Resp: 16731

Ion	Ratio	Lower	Upper
75	100		
77	36.2	26.2	39.2
110	1.7	28.4	42.6#

