

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061024\
 Data File : VU059203.D
 Acq On : 10 Jun 2024 13:35
 Operator : MD/SY
 Sample : P2754-18ME
 Misc : 4.91g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jun 11 06:02:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 11 05:56:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	277956	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	281023	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	128291	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	44568	26.780	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	53.560%#		
7) Chloroethane-d5	1.911	69	46310	32.484	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	64.960%#		
11) 1,1-Dichloroethene-d2	2.563	63	68439	20.834	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	41.660%#		
21) 2-Butanone-d5	4.615	46	129683	82.672	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	82.670%		
24) Chloroform-d	5.055	84	134780	40.682	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.360%		
26) 1,2-Dichloroethane-d4	5.695	65	86565	42.630	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.260%		
32) Benzene-d6	5.721	84	243778	37.796	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	75.600%		
36) 1,2-Dichloropropane-d6	6.685	67	88317	39.712	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	79.420%		
41) Toluene-d8	7.894	98	203908	37.241	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	74.480%#		
43) trans-1,3-Dichloroprop...	8.177	79	36120	40.180	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.360%		
47) 2-Hexanone-d5	8.627	63	78819	76.642	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	76.640%		
56) 1,1,2,2-Tetrachloroeth...	10.750	84	156994	41.711	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	83.420%		
66) 1,2-Dichlorobenzene-d4	12.190	152	90950	47.505	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.020%		
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	6.682	63	9295	3.226	ug/L #	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061024\
Data File : VU059203.D
Acq On : 10 Jun 2024 13:35
Operator : MD/SY
Sample : P2754-18ME
Misc : 4.91g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jun 11 06:02:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 11 05:56:14 2024
Response via : Initial Calibration

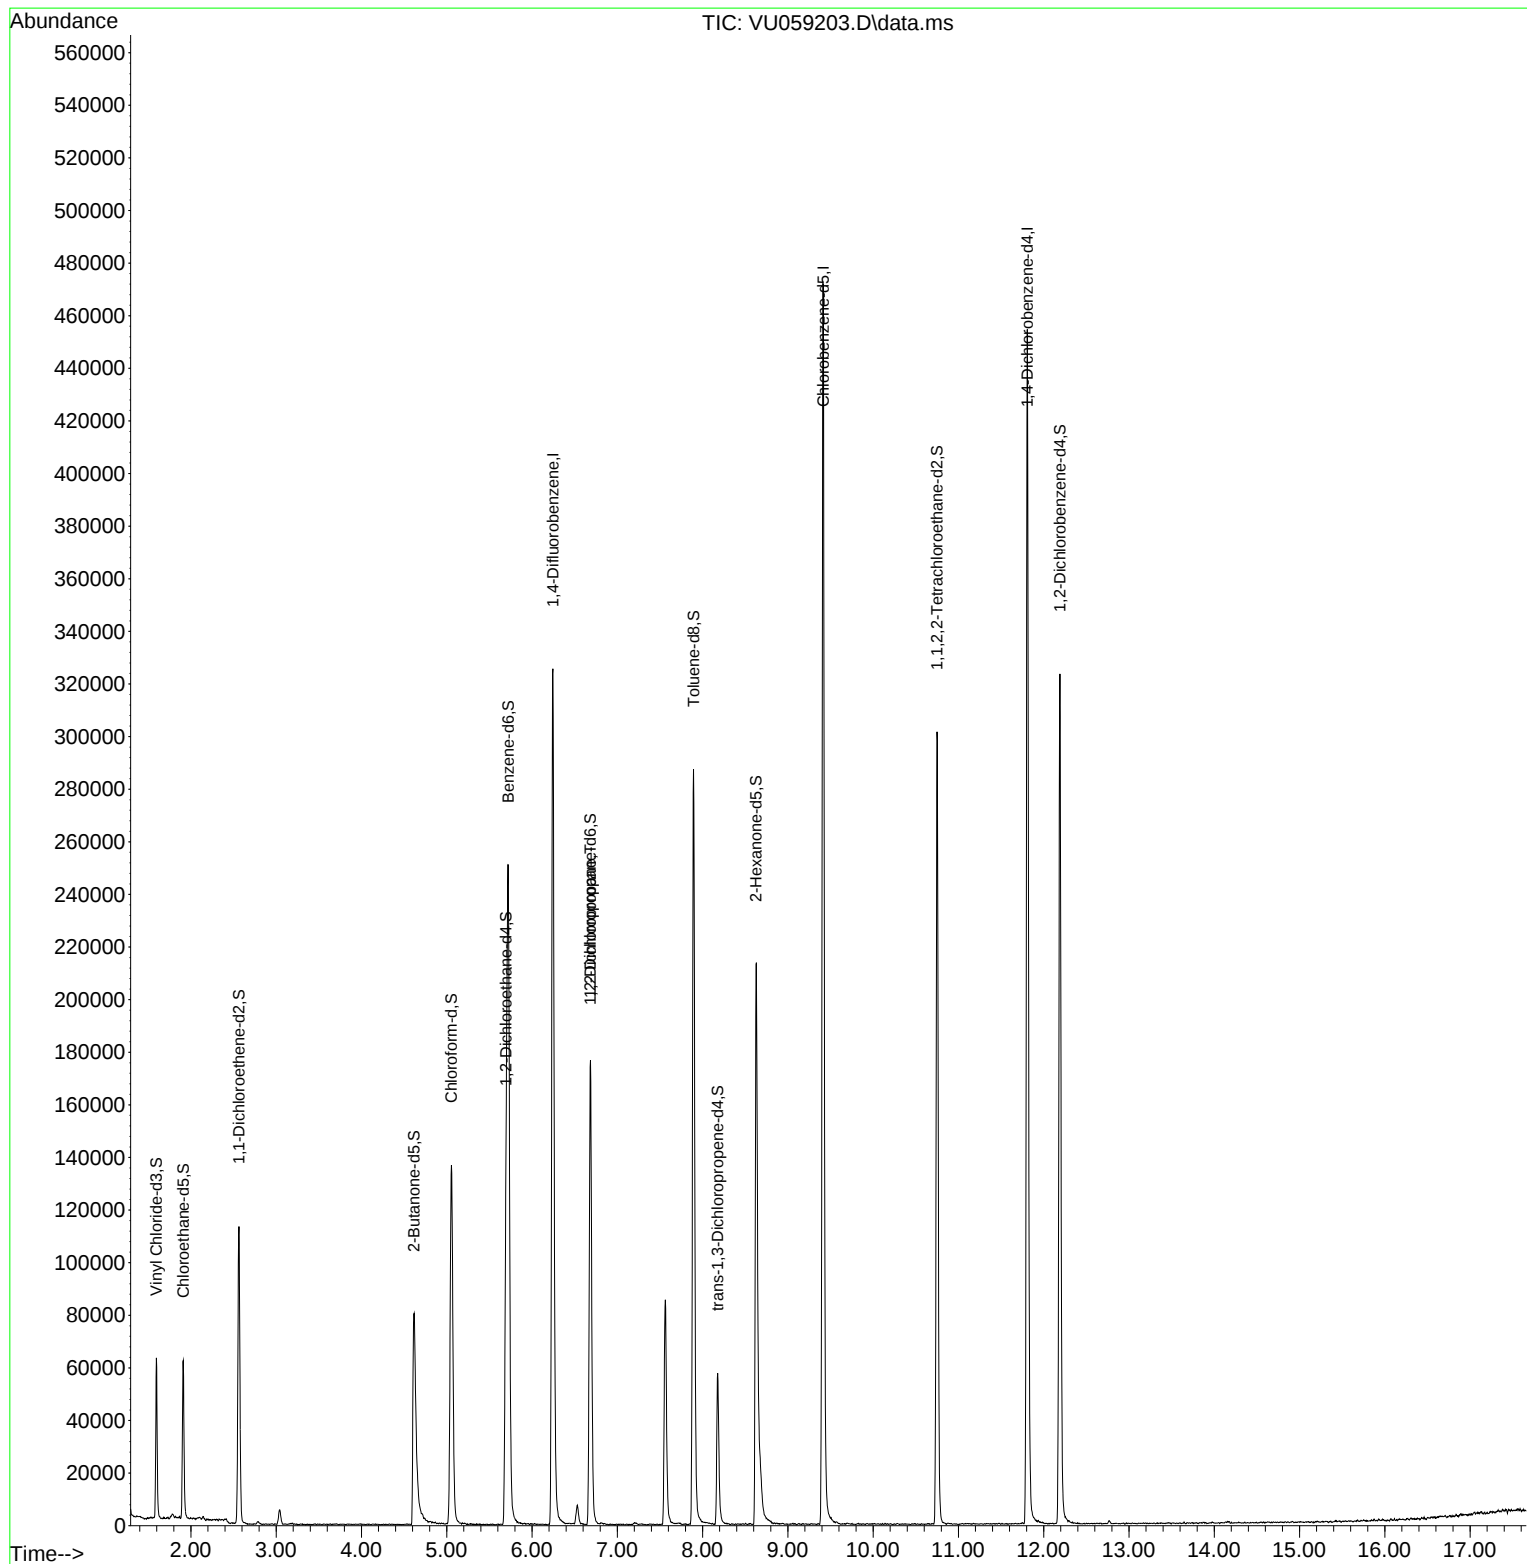

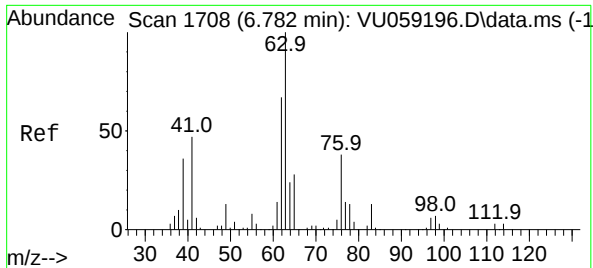

#37
 1,2-Dichloropropane
 Concen: 3.226 ug/L
 RT: 6.682 min Scan# 1
 Delta R.T. -0.100 min
 Lab File: VU059203.D
 Acq: 10 Jun 2024 13:35

Instrument :
 MSVOA_U
 ClientSampleId :

Tgt Ion: 63 Resp: 9295
 Ion Ratio Lower Upper
 63 100
 112 0.0 2.6 4.0#

