

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061024\
 Data File : VU059199.D
 Acq On : 10 Jun 2024 11:11
 Operator : MD/SY
 Sample : P2693-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059199.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	115	rVB	118608	139858	14.43%	1.848%
2	1.911	184	193	213	rVB	100116	133962	13.82%	1.770%
3	2.563	383	396	415	rBV	190631	317380	32.75%	4.194%
4	2.698	434	438	443	rVV	318	267	0.03%	0.004%
5	2.753	452	455	458	rBV2	302	243	0.03%	0.003%
6	2.792	458	467	475	rVV3	1689	2764	0.29%	0.037%
7	2.849	482	485	489	rVB	382	252	0.03%	0.003%
8	2.882	489	495	498	rBV2	406	429	0.04%	0.006%
9	2.962	515	520	523	rBV2	398	411	0.04%	0.005%
10	3.039	536	544	556	rVB4	2597	5272	0.54%	0.070%
11	3.107	560	565	569	rBV2	347	402	0.04%	0.005%
12	3.158	575	581	582	rBV	195	214	0.02%	0.003%
13	3.264	613	614	619	rVB	291	201	0.02%	0.003%
14	3.303	623	626	633	rVV	331	383	0.04%	0.005%
15	3.348	636	640	645	rVV3	498	500	0.05%	0.007%
16	3.386	647	652	657	rBV2	193	262	0.03%	0.003%
17	3.441	666	669	674	rVB2	289	193	0.02%	0.003%
18	3.611	719	722	724	rBV	292	187	0.02%	0.002%
19	3.782	769	775	778	rBV2	249	278	0.03%	0.004%
20	3.833	785	791	794	rBV2	281	325	0.03%	0.004%
21	3.862	798	800	802	rBV2	339	176	0.02%	0.002%
22	3.904	810	813	817	rVB	234	194	0.02%	0.003%
23	3.972	830	834	835	rBV	306	248	0.03%	0.003%
24	4.103	872	875	883	rVB2	324	362	0.04%	0.005%
25	4.229	909	914	916	rBV2	367	317	0.03%	0.004%
26	4.261	920	924	930	rVB2	448	478	0.05%	0.006%
27	4.309	933	939	942	rBV	432	407	0.04%	0.005%
28	4.425	971	975	979	rVB2	263	208	0.02%	0.003%
29	4.447	979	982	985	rBV	233	186	0.02%	0.002%
30	4.528	1003	1007	1013	rBV2	309	323	0.03%	0.004%
31	4.611	1024	1033	1068	rBV	74269	195355	20.16%	2.582%
32	4.984	1145	1149	1154	rBV2	527	487	0.05%	0.006%
33	5.055	1154	1171	1197	rVV	168303	379299	39.14%	5.012%
34	5.508	1308	1312	1317	rVV3	152	174	0.02%	0.002%
35	5.605	1339	1342	1348	rBV	258	268	0.03%	0.004%
36	5.717	1354	1377	1411	rBV2	352648	969167	100.00%	12.808%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061024\
 Data File : VU059199.D
 Acq On : 10 Jun 2024 11:11
 Operator : MD/SY
 Sample : P2693-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.081	1487	1490	1492	rVB	331	190	0.02%	0.003%
38	6.100	1492	1496	1499	rBV3	287	211	0.02%	0.003%
39	6.242	1526	1540	1570	rBV	342551	672597	69.40%	8.888%
40	6.489	1613	1617	1619	rBV2	301	260	0.03%	0.003%
41	6.531	1619	1630	1641	rVB7	5616	12157	1.25%	0.161%
42	6.682	1664	1677	1708	rBV	214911	430171	44.39%	5.685%
43	6.846	1725	1728	1733	rBV2	271	253	0.03%	0.003%
44	6.881	1736	1739	1742	rVB3	294	212	0.02%	0.003%
45	6.923	1749	1752	1756	rBV	235	172	0.02%	0.002%
46	7.068	1793	1797	1806	rVB2	406	494	0.05%	0.007%
47	7.103	1806	1808	1814	rVB2	342	328	0.03%	0.004%
48	7.132	1814	1817	1819	rBV	317	201	0.02%	0.003%
49	7.200	1831	1838	1843	rBV5	1312	2305	0.24%	0.030%
50	7.361	1886	1888	1892	rVB2	299	200	0.02%	0.003%
51	7.386	1892	1896	1902	rBV2	390	517	0.05%	0.007%
52	7.560	1937	1950	1973	rBV	109020	198797	20.51%	2.627%
53	7.714	1989	1998	2002	rBV3	1203	1570	0.16%	0.021%
54	7.791	2017	2022	2026	rBV2	439	457	0.05%	0.006%
55	7.891	2041	2053	2082	rBV	421738	741896	76.55%	9.804%
56	8.126	2123	2126	2128	rVB2	366	198	0.02%	0.003%
57	8.174	2131	2141	2163	rBV	73039	131497	13.57%	1.738%
58	8.290	2173	2177	2180	rVV2	418	367	0.04%	0.005%
59	8.434	2218	2222	2226	rVB2	397	382	0.04%	0.005%
60	8.460	2226	2230	2234	rBV2	562	536	0.06%	0.007%
61	8.553	2256	2259	2263	rVB3	611	416	0.04%	0.005%
62	8.627	2271	2282	2317	rBV2	204437	418918	43.22%	5.536%
63	8.907	2366	2369	2371	rVV3	319	207	0.02%	0.003%
64	8.939	2376	2379	2382	rBV2	303	200	0.02%	0.003%
65	9.077	2417	2422	2430	rBV2	264	415	0.04%	0.005%
66	9.161	2446	2448	2452	rVB2	399	221	0.02%	0.003%
67	9.286	2484	2487	2490	rBV3	329	181	0.02%	0.002%
68	9.309	2490	2494	2496	rBV2	267	189	0.02%	0.002%
69	9.412	2512	2526	2567	rBV	493855	857895	88.52%	11.337%
70	9.685	2605	2611	2613	rBV3	552	592	0.06%	0.008%
71	9.714	2618	2620	2623	rVV3	472	249	0.03%	0.003%
72	9.801	2644	2647	2649	rBV	254	202	0.02%	0.003%
73	9.942	2685	2691	2697	rBV	429	572	0.06%	0.008%
74	10.074	2729	2732	2735	rBV2	233	242	0.02%	0.003%
75	10.100	2736	2740	2743	rVV2	535	464	0.05%	0.006%
76	10.135	2749	2751	2753	rVV3	316	183	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061024\
 Data File : VU059199.D
 Acq On : 10 Jun 2024 11:11
 Operator : MD/SY
 Sample : P2693-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	10.190	2763	2768	2771	rBV2	271	295	0.03%	0.004%
78	10.396	2829	2832	2835	rVB2	296	187	0.02%	0.002%
79	10.486	2855	2860	2864	rVB2	346	341	0.04%	0.005%
80	10.505	2864	2866	2869	rBV	255	170	0.02%	0.002%
81	10.624	2899	2903	2907	rBV2	277	244	0.03%	0.003%
82	10.653	2909	2912	2914	rBV	473	252	0.03%	0.003%
83	10.749	2928	2942	2962	rBV	305625	499960	51.59%	6.607%
84	10.878	2979	2982	2983	rBV	429	224	0.02%	0.003%
85	11.473	3165	3167	3171	rVB2	268	206	0.02%	0.003%
86	11.746	3246	3252	3258	rBV3	892	1026	0.11%	0.014%
87	11.807	3258	3271	3302	rBV	464350	780324	80.51%	10.312%
88	12.068	3348	3352	3355	rBV2	328	327	0.03%	0.004%
89	12.106	3361	3364	3366	rBV	337	242	0.02%	0.003%
90	12.187	3375	3389	3415	rBV	385703	651090	67.18%	8.604%
91	12.457	3469	3473	3476	rBV	318	292	0.03%	0.004%
92	12.714	3550	3553	3557	rVB2	362	231	0.02%	0.003%
93	12.769	3565	3570	3577	rVB3	875	1114	0.11%	0.015%
94	13.135	3681	3684	3687	rBV2	397	310	0.03%	0.004%
95	13.180	3694	3698	3701	rBV	433	385	0.04%	0.005%
96	13.637	3836	3840	3842	rBV	276	269	0.03%	0.004%
97	13.810	3891	3894	3897	rBV	332	293	0.03%	0.004%
98	13.862	3907	3910	3912	rBV	523	351	0.04%	0.005%
99	13.891	3917	3919	3924	rVB2	366	218	0.02%	0.003%
100	15.585	4444	4446	4448	rBV3	458	177	0.02%	0.002%




Sum of corrected areas: 7567074

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061024\
Data File : VU059199.D
Acq On : 10 Jun 2024 11:11
Operator : MD/SY
Sample : P2693-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

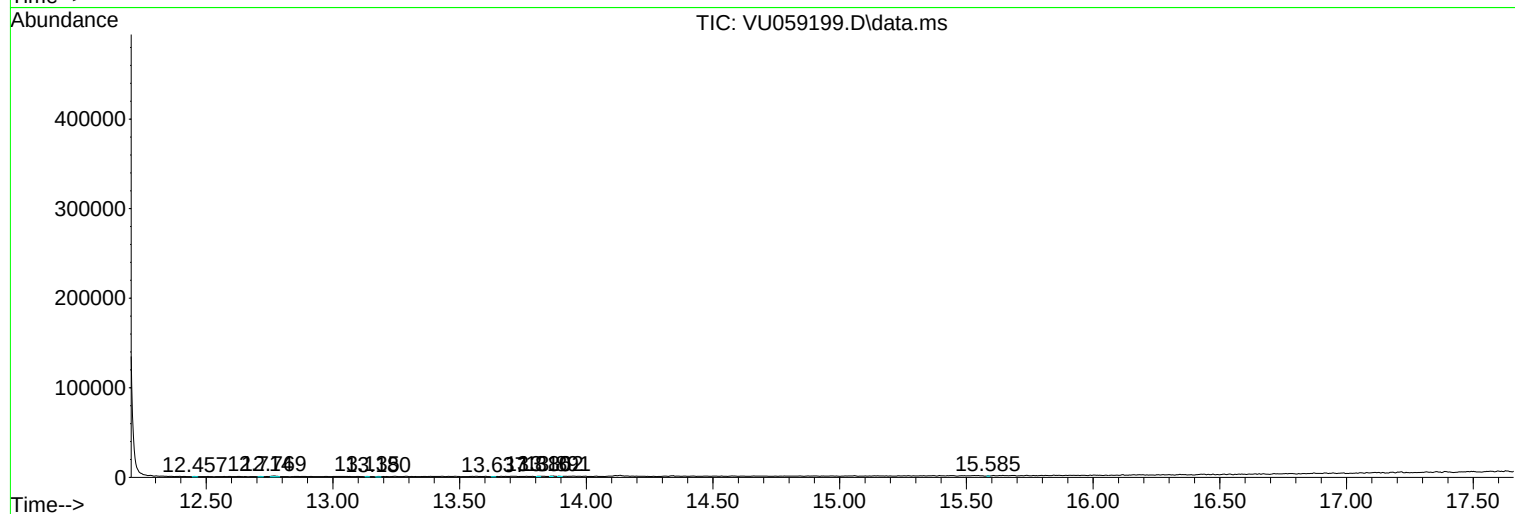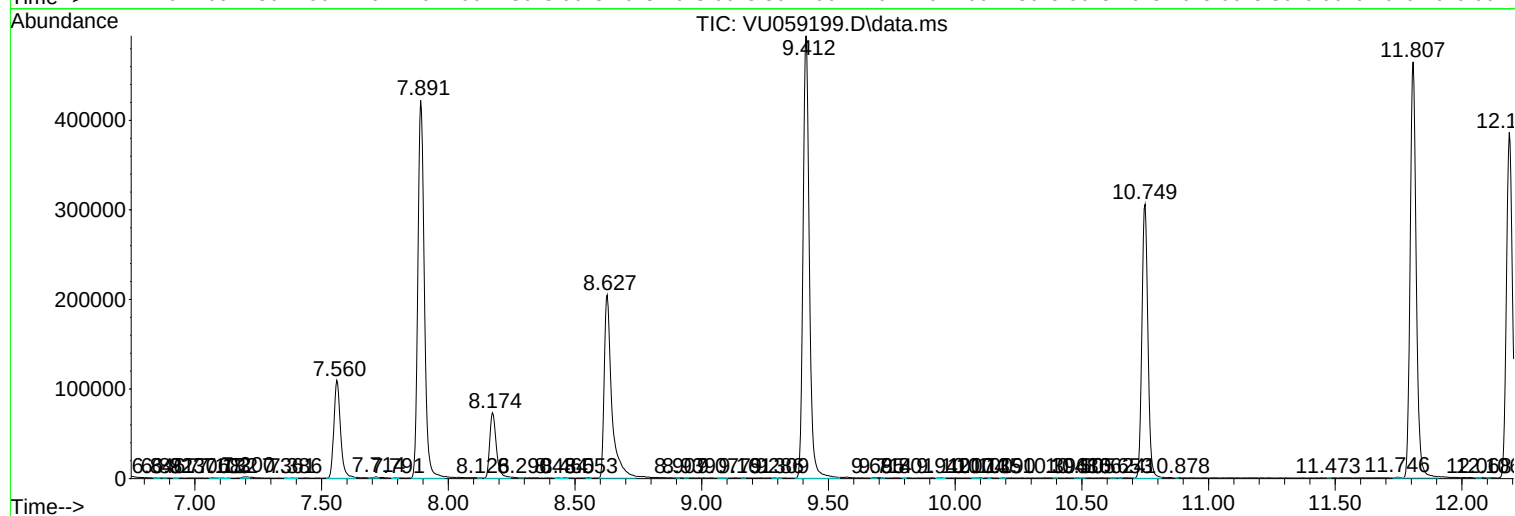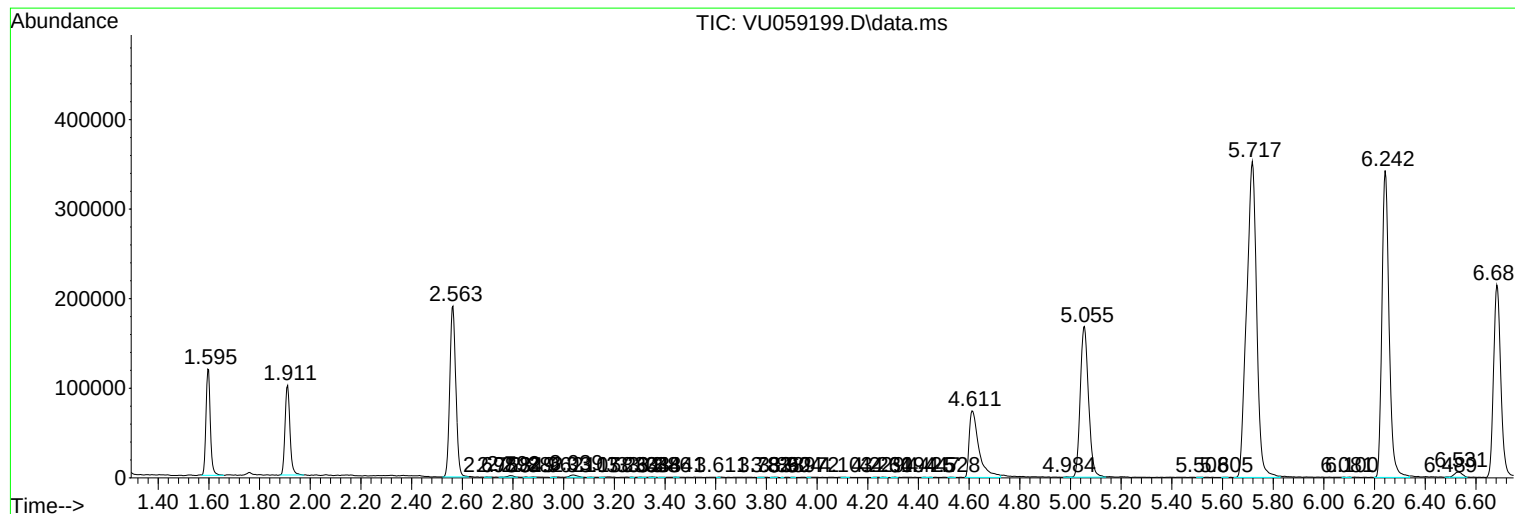

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061024\
Data File : VU059199.D
Acq On : 10 Jun 2024 11:11
Operator : MD/SY
Sample : P2693-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061024\
Data File : VU059199.D
Acq On : 10 Jun 2024 11:11
Operator : MD/SY
Sample : P2693-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc