




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061324\
Data File : VU059229.D
Acq On : 13 Jun 2024 11:01
Operator : MD/SY
Sample : P2850-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHB87

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2024
Supervised By :Mahesh Dadoda 06/14/2024

Quant Time: Jun 14 06:55:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 14 06:53:55 2024
Response via : Initial Calibration

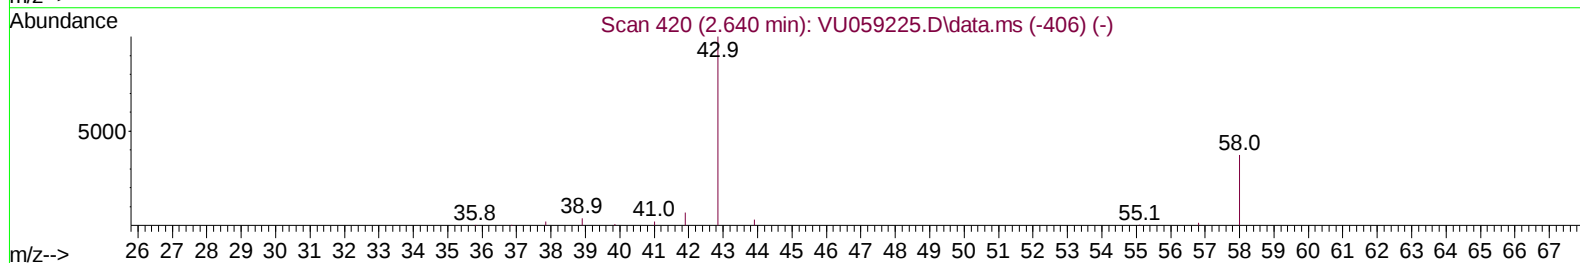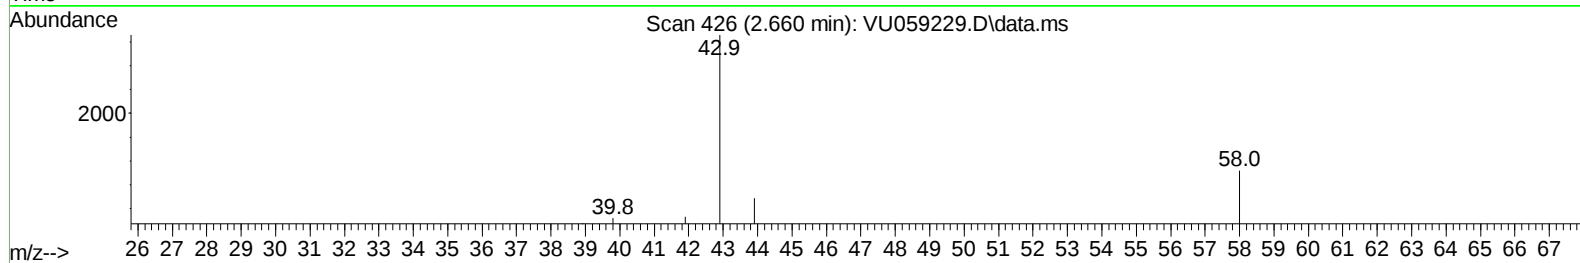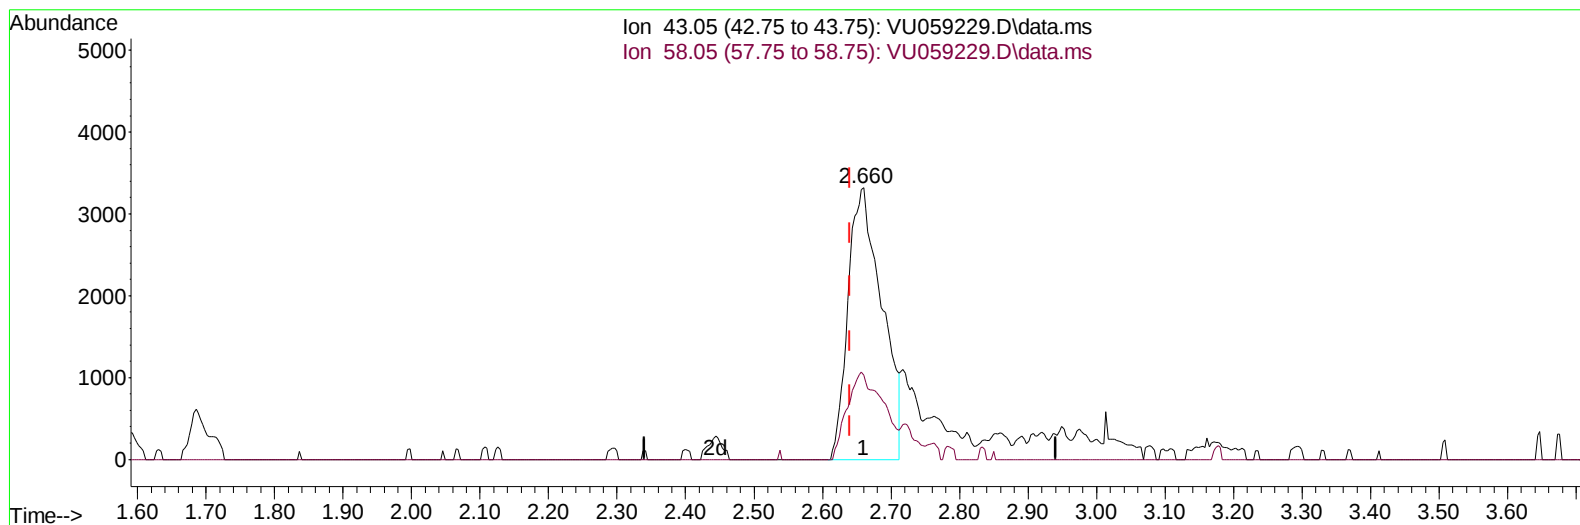

TIC: VU059229.D\data.ms

(13) Acetone (T)

2.660min (+ 0.019) 7.01 ug/L

response 11335

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	34.43
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061324\
Data File : VU059229.D
Acq On : 13 Jun 2024 11:01
Operator : MD/SY
Sample : P2850-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHB87

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2024
Supervised By :Mahesh Dadoda 06/14/2024

Quant Time: Jun 14 06:55:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 14 06:53:55 2024
Response via : Initial Calibration

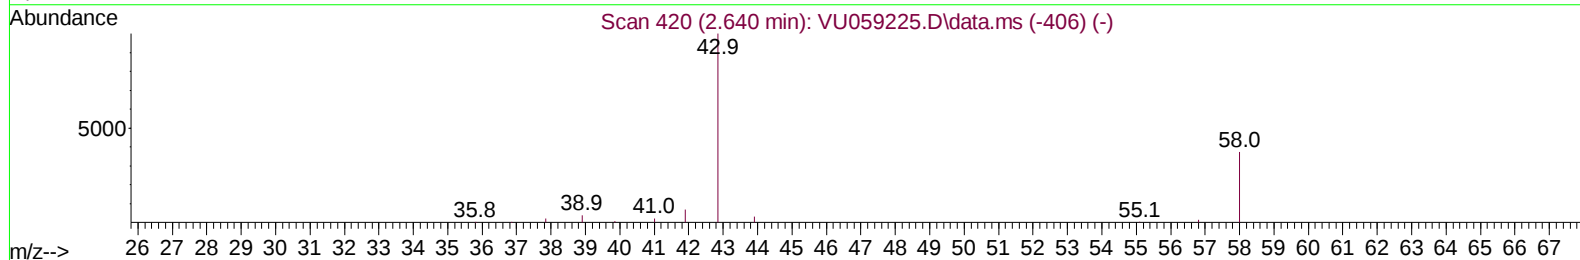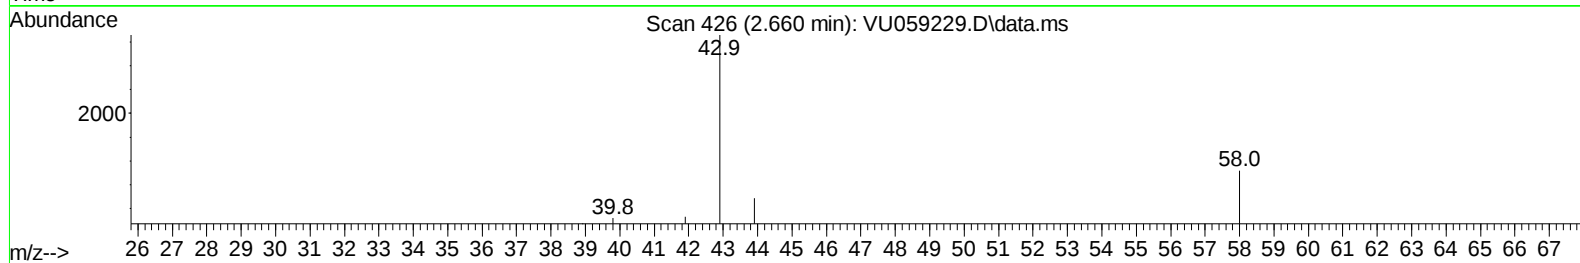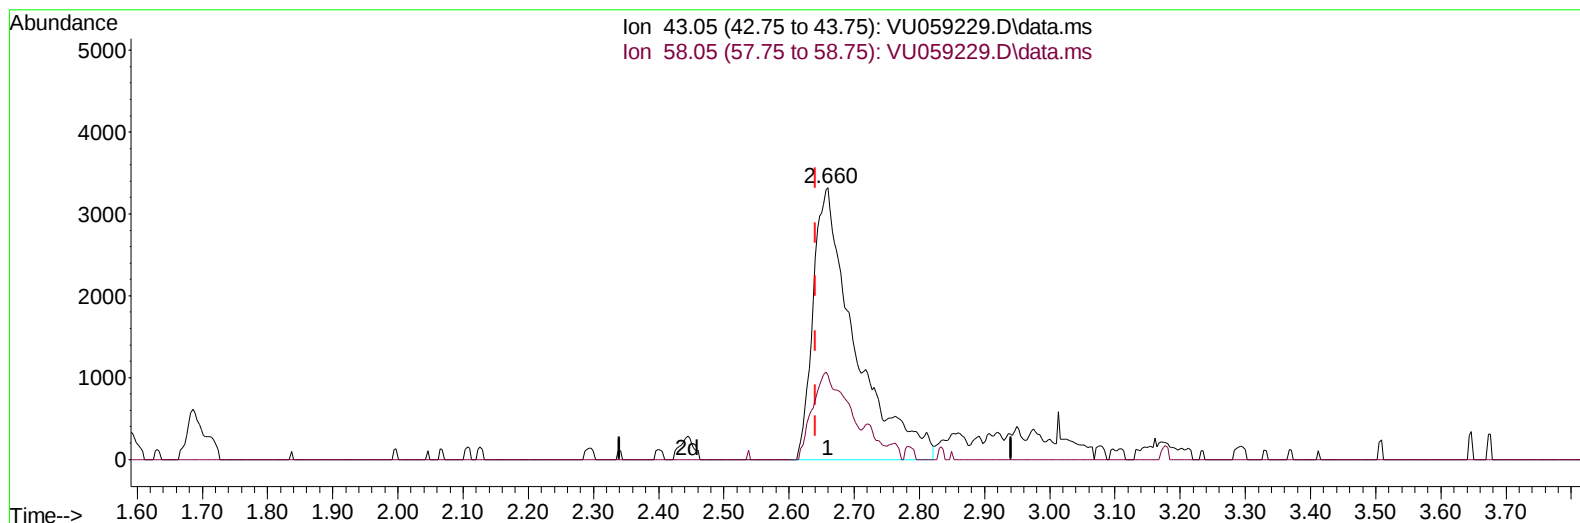

TIC: VU059229.D\data.ms

(13) Acetone (T)

2.660min (+ 0.019) 9.12 ug/L m

response 14740

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	26.48
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061324\
 Data File : VU059229.D
 Acq On : 13 Jun 2024 11:01
 Operator : MD/SY
 Sample : P2850-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHB87

Manual IntegrationsAPPROVED

Quant Time: Jun 14 06:55:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 14 06:53:55 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/14/2024
 Supervised By :Mahesh Dadoda 06/14/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		148450	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		150406	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		63582	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.589	65		32977	3.667	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	73.400%	
7) Chloroethane-d5	1.904	69		36020	4.432	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	88.600%	
11) 1,1-Dichloroethene-d2	2.557	65		14435	3.939	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	78.800%	
20) 2-Butanone-d5	4.640	46		126114	53.943	ug/L	0.01
Spiked Amount 50.000	Range 40	- 130		Recovery	=	107.880%	
24) Chloroform-d	5.052	84		90939	5.008	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	100.200%	
26) 1,2-Dichloroethane-d4	5.695	65		47560	5.096	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	102.000%	
32) Benzene-d6	5.717	84		163477	4.735	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	94.800%	
36) 1,2-Dichloropropane-d6	6.682	67		58746	5.107	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	102.200%	
41) Toluene-d8	7.891	98		126139	4.014	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	80.200%	
43) trans-1,3-Dichloroprop...	8.177	79		16097	4.078	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	81.600%	
46) 2-Hexanone-d5	8.631	63		86661	45.743	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	91.480%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		50613	5.095	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	101.800%	
66) 1,2-Dichlorobenzene-d4	12.187	152		49972	5.226	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	104.600%	
Target Compounds							
13) Acetone	2.660	43		14740m	9.122	ug/L	
14) Carbon disulfide	2.782	76		129509	4.420	ug/L	98
16) Methylene chloride	3.036	84		2280	0.182	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061324\
Data File : VU059229.D
Acq On : 13 Jun 2024 11:01
Operator : MD/SY
Sample : P2850-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHB87

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2024
Supervised By :Mahesh Dadoda 06/14/2024

Quant Time: Jun 14 06:55:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 14 06:53:55 2024
Response via : Initial Calibration

