




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061324\
Data File : VU059230.D
Acq On : 13 Jun 2024 11:25
Operator : MD/SY
Sample : P2850-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAZ6

Manual IntegrationsAPPROVED

Quant Time: Jun 14 06:55:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 14 06:53:55 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/14/2024
Supervised By :Mahesh Dadoda 06/14/2024

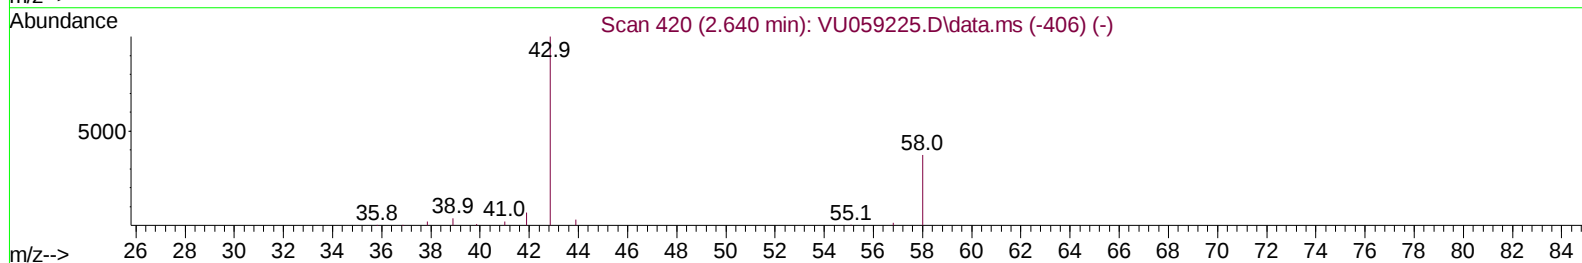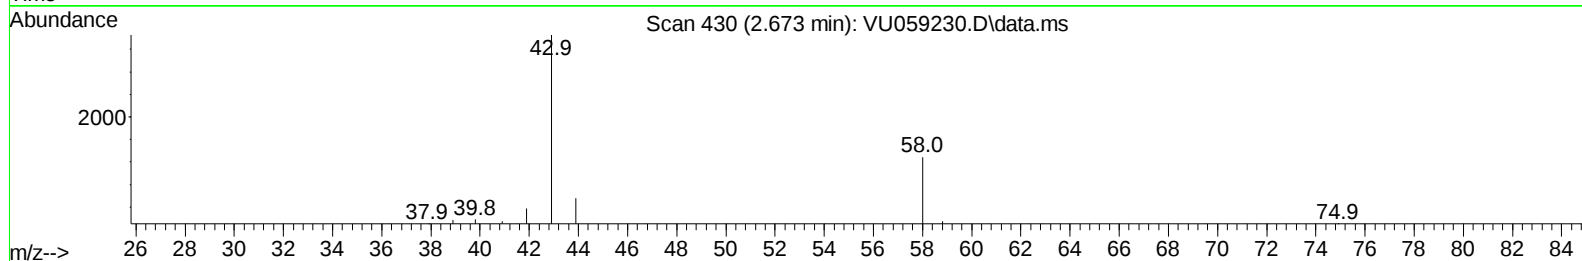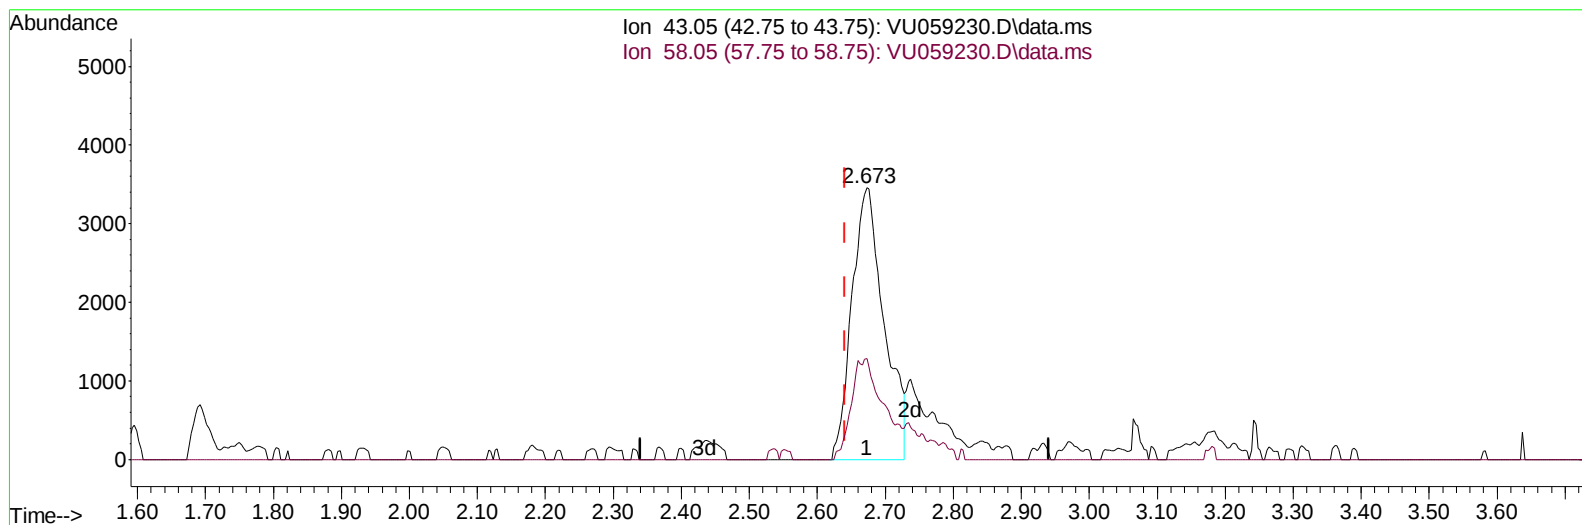

TIC: VU059230.D\data.ms

(13) Acetone (T)

2.673min (+ 0.032) 6.66 ug/L

response 11375

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	37.78
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061324\
Data File : VU059230.D
Acq On : 13 Jun 2024 11:25
Operator : MD/SY
Sample : P2850-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAZ6

Manual IntegrationsAPPROVED

Quant Time: Jun 14 06:55:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 14 06:53:55 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/14/2024
Supervised By :Mahesh Dadoda 06/14/2024

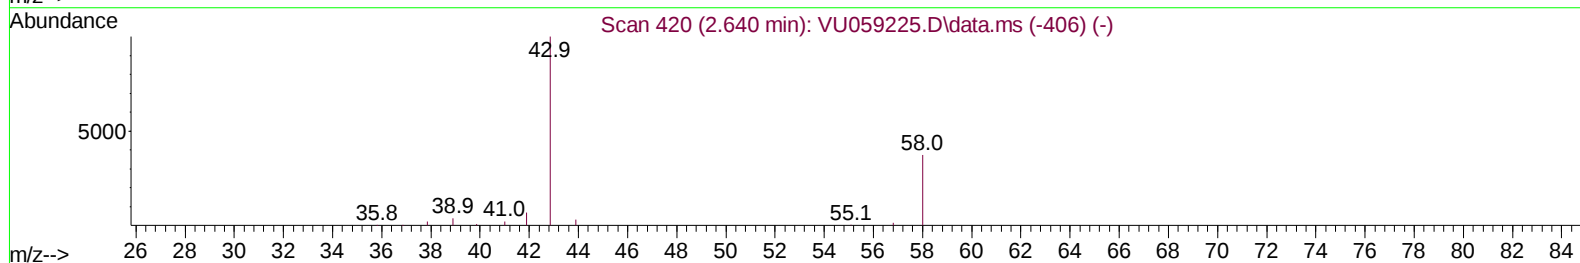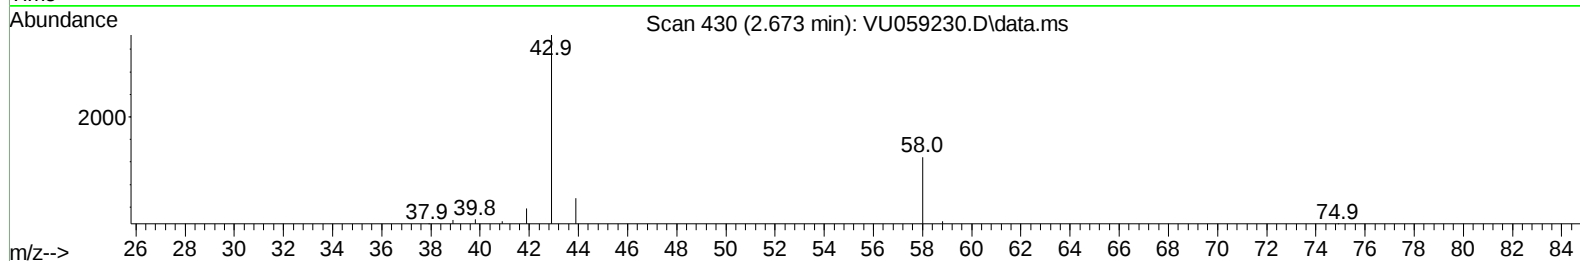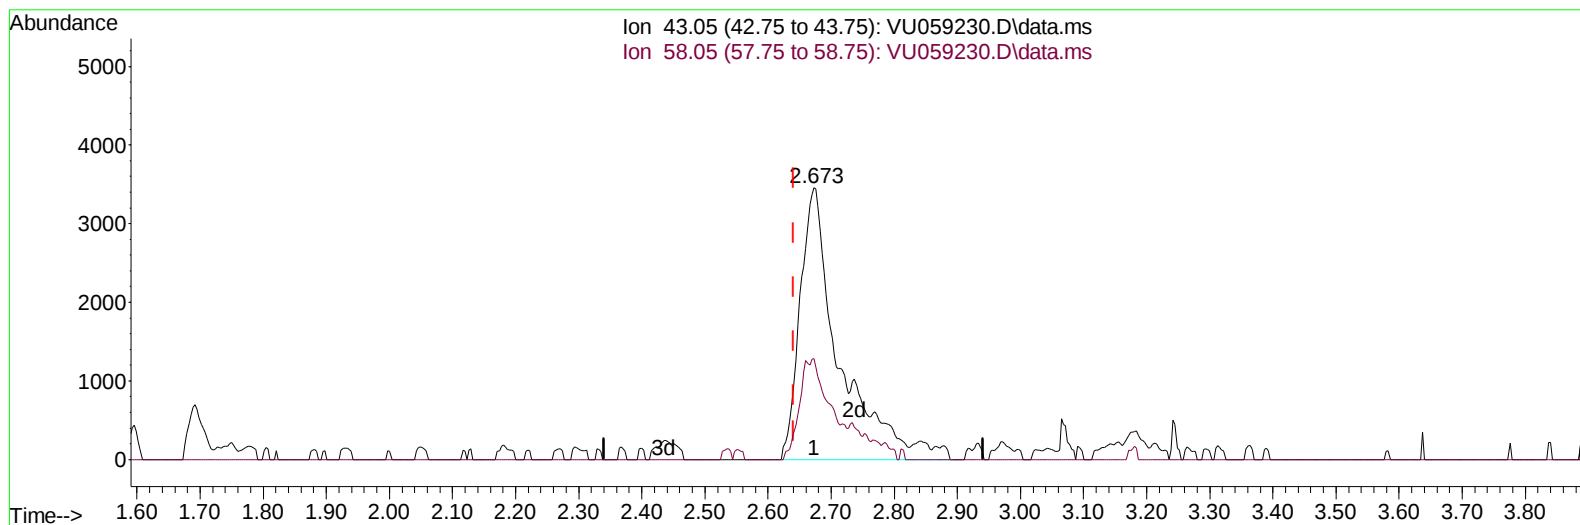

TIC: VU059230.D\data.ms

(13) Acetone (T)

2.673min (+ 0.032) 8.80 ug/L m

response 15031

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	28.59
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061324\
 Data File : VU059230.D
 Acq On : 13 Jun 2024 11:25
 Operator : MD/SY
 Sample : P2850-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHAZ6

Manual IntegrationsAPPROVED

Quant Time: Jun 14 06:55:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 14 06:53:55 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/14/2024
 Supervised By :Mahesh Dadoda 06/14/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		156988	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		161098	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		68387	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.592	65		33151	3.486	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	69.800%	
7) Chloroethane-d5	1.907	69		37767	4.394	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.800%	
11) 1,1-Dichloroethene-d2	2.560	65		15759	4.066	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.400%	
20) 2-Butanone-d5	4.644	46		139456	56.406	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.820%	
24) Chloroform-d	5.055	84		93741	4.881	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%	
26) 1,2-Dichloroethane-d4	5.698	65		49522	5.018	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.400%	
32) Benzene-d6	5.718	84		171119	4.627	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.600%	
36) 1,2-Dichloropropane-d6	6.682	67		62069	5.038	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.800%	
41) Toluene-d8	7.894	98		130210	3.869	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.400%	
43) trans-1,3-Dichloroprop...	8.177	79		17936	4.242	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.800%	
46) 2-Hexanone-d5	8.631	63		89211	43.964	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.920%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		53030	4.984	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.600%	
66) 1,2-Dichlorobenzene-d4	12.187	152		52065	5.062	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.200%	
Target Compounds							
13) Acetone	2.673	43		15031m	8.796	ug/L	
16) Methylene chloride	3.036	84		2461	0.185	ug/L	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061324\
Data File : VU059230.D
Acq On : 13 Jun 2024 11:25
Operator : MD/SY
Sample : P2850-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAZ6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/14/2024
Supervised By :Mahesh Dadoda 06/14/2024

Quant Time: Jun 14 06:55:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 14 06:53:55 2024
Response via : Initial Calibration

