

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061324\
 Data File : VU059227.D
 Acq On : 13 Jun 2024 10:14
 Operator : MD/SY
 Sample : P2850-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHB64

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU059227.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	108	rVB	52821	61999	10.95%	1.362%
2	1.907	183	192	208	rVB	56827	76354	13.49%	1.677%
3	2.560	384	395	409	rBV	87532	142050	25.10%	3.119%
4	2.634	409	418	438	rVB	8585	17986	3.18%	0.395%
5	2.792	456	467	470	rBV4	4574	6943	1.23%	0.152%
6	3.039	535	544	554	rVB3	4969	9065	1.60%	0.199%
7	3.174	575	586	602	rBV	5001	11715	2.07%	0.257%
8	4.621	1019	1036	1080	rBV	94163	285693	50.48%	6.274%
9	4.811	1086	1095	1110	rBV2	11849	25670	4.54%	0.564%
10	5.055	1156	1171	1196	rBV	114181	255625	45.17%	5.614%
11	5.718	1358	1377	1401	rBV2	198873	528588	93.40%	11.608%
12	6.242	1525	1540	1567	rBV	185438	368139	65.05%	8.084%
13	6.685	1665	1678	1699	rBV	131914	264470	46.73%	5.808%
14	7.563	1940	1951	1973	rBV2	53712	98121	17.34%	2.155%
15	7.894	2042	2054	2074	rBV	211061	374321	66.14%	8.220%
16	8.177	2133	2142	2164	rBV3	31473	56972	10.07%	1.251%
17	8.631	2271	2283	2326	rBV2	261774	565968	100.00%	12.429%
18	9.412	2514	2526	2556	rBV	272753	474964	83.92%	10.430%
19	10.753	2931	2943	2962	rBV	107663	180294	31.86%	3.959%
20	11.807	3260	3271	3296	rBV	232380	398183	70.35%	8.744%
21	12.190	3378	3390	3416	rBV	204357	350533	61.94%	7.698%




Sum of corrected areas: 4553653

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061324\
Data File : VU059227.D
Acq On : 13 Jun 2024 10:14
Operator : MD/SY
Sample : P2850-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHB64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

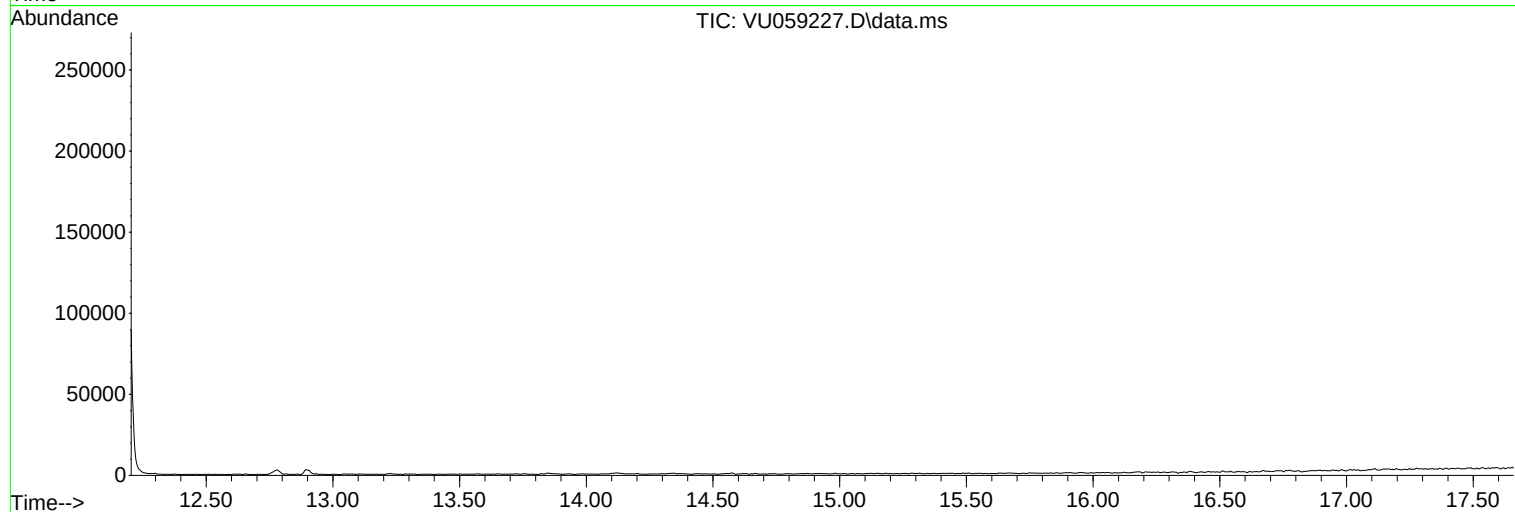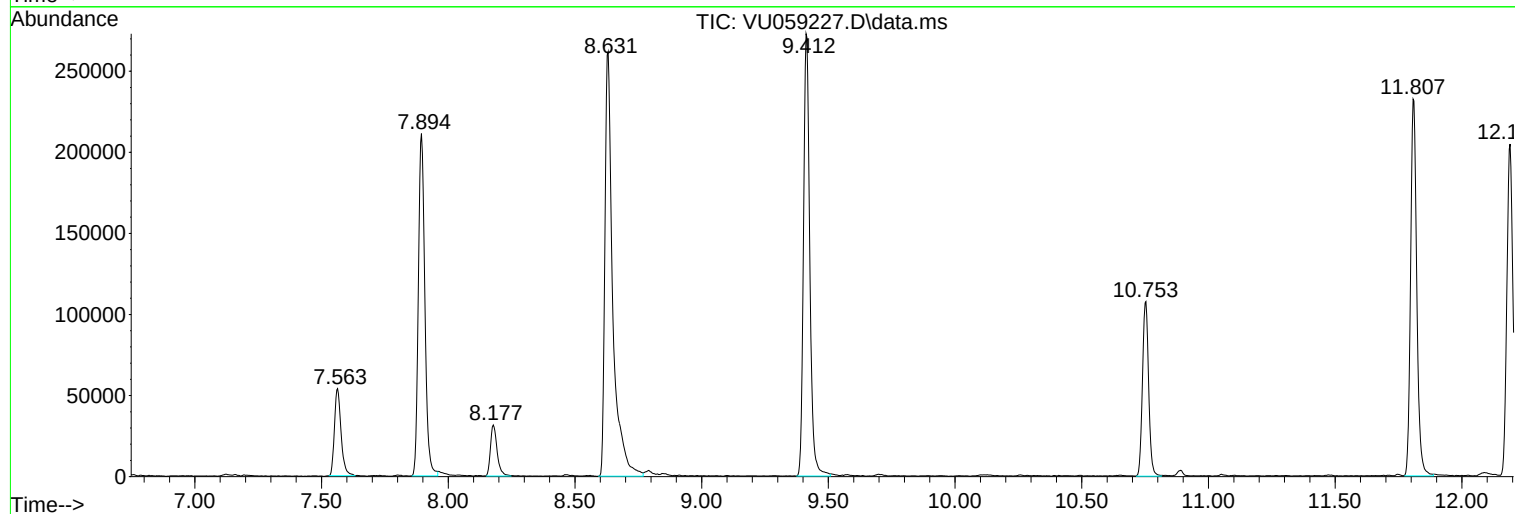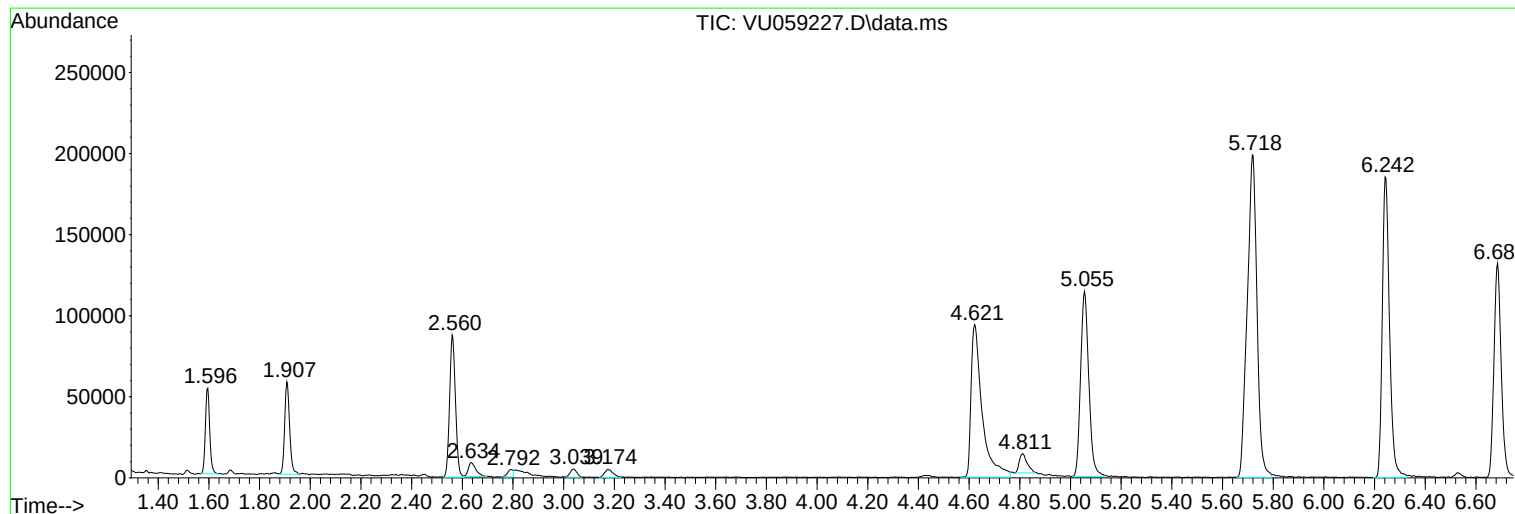

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061324\
Data File : VU059227.D
Acq On : 13 Jun 2024 10:14
Operator : MD/SY
Sample : P2850-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHB64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061324\
Data File : VU059227.D
Acq On : 13 Jun 2024 10:14
Operator : MD/SY
Sample : P2850-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHB64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
