

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061324\
 Data File : VU059235.D
 Acq On : 13 Jun 2024 15:25
 Operator : MD/SY
 Sample : P2850-01 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHAW0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU059235.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	108	rVB	47479	54648	7.85%	1.139%
2	1.907	184	192	204	rVB	47698	63566	9.14%	1.325%
3	2.560	383	395	411	rBV	75241	121355	17.44%	2.530%
4	3.039	530	544	565	rVB2	47938	92602	13.31%	1.931%
5	4.657	1024	1047	1084	rBV4	207920	695729	100.00%	14.505%
6	5.055	1156	1171	1192	rBV	98853	219192	31.51%	4.570%
7	5.721	1359	1378	1404	rBV3	176972	476307	68.46%	9.931%
8	6.245	1527	1541	1566	rBV2	201503	391715	56.30%	8.167%
9	6.534	1621	1631	1648	rVB8	6666	14559	2.09%	0.304%
10	6.685	1664	1678	1696	rBV	122617	242084	34.80%	5.047%
11	7.563	1938	1951	1970	rBV2	50029	92251	13.26%	1.923%
12	7.894	2040	2054	2074	rBV	185047	328630	47.24%	6.852%
13	8.177	2133	2142	2160	rBV	29619	51631	7.42%	1.076%
14	8.547	2251	2257	2268	rBV6	4535	7318	1.05%	0.153%
15	8.627	2272	2282	2319	rBV2	266413	555987	79.91%	11.592%
16	9.412	2515	2526	2569	rBV	290942	500580	71.95%	10.437%
17	10.753	2931	2943	2963	rBV	103099	170473	24.50%	3.554%
18	11.807	3260	3271	3296	rBV	238339	406760	58.47%	8.481%
19	12.190	3378	3390	3412	rBV2	183629	310944	44.69%	6.483%




Sum of corrected areas: 4796331

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061324\
Data File : VU059235.D
Acq On : 13 Jun 2024 15:25
Operator : MD/SY
Sample : P2850-01 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

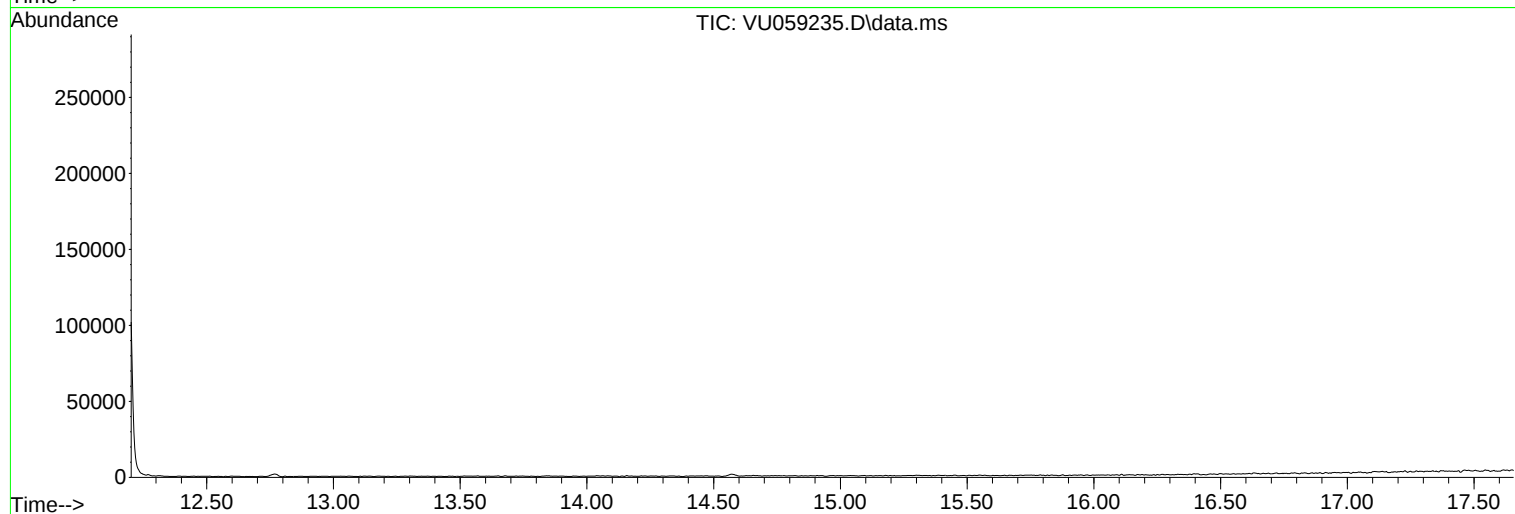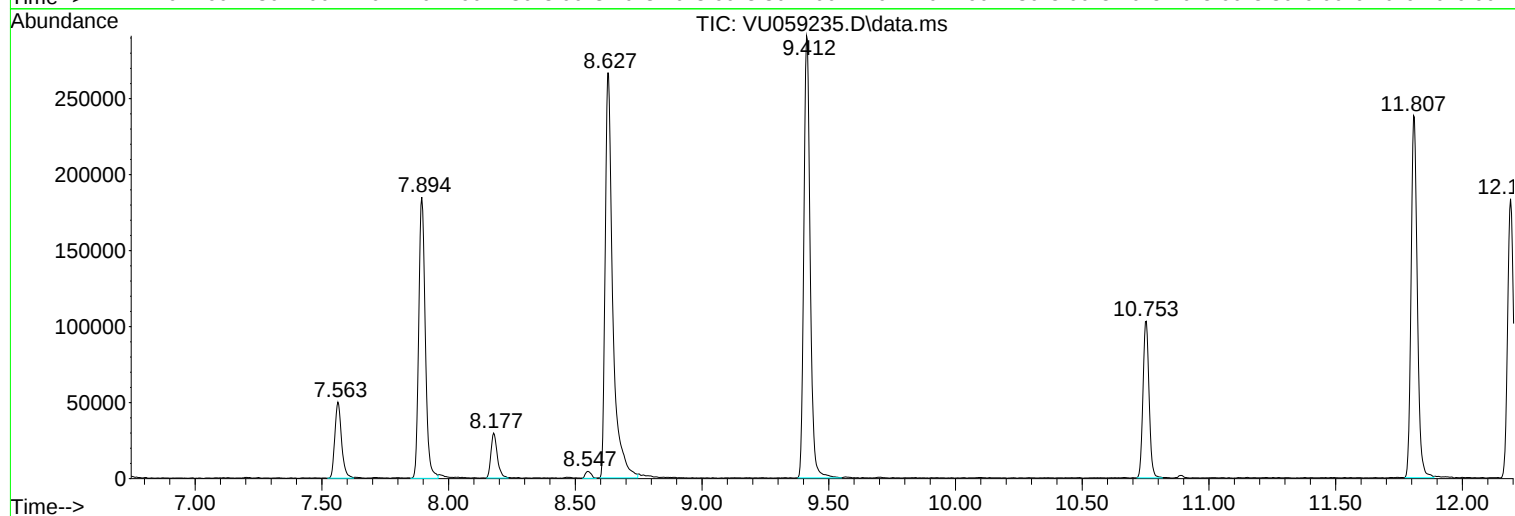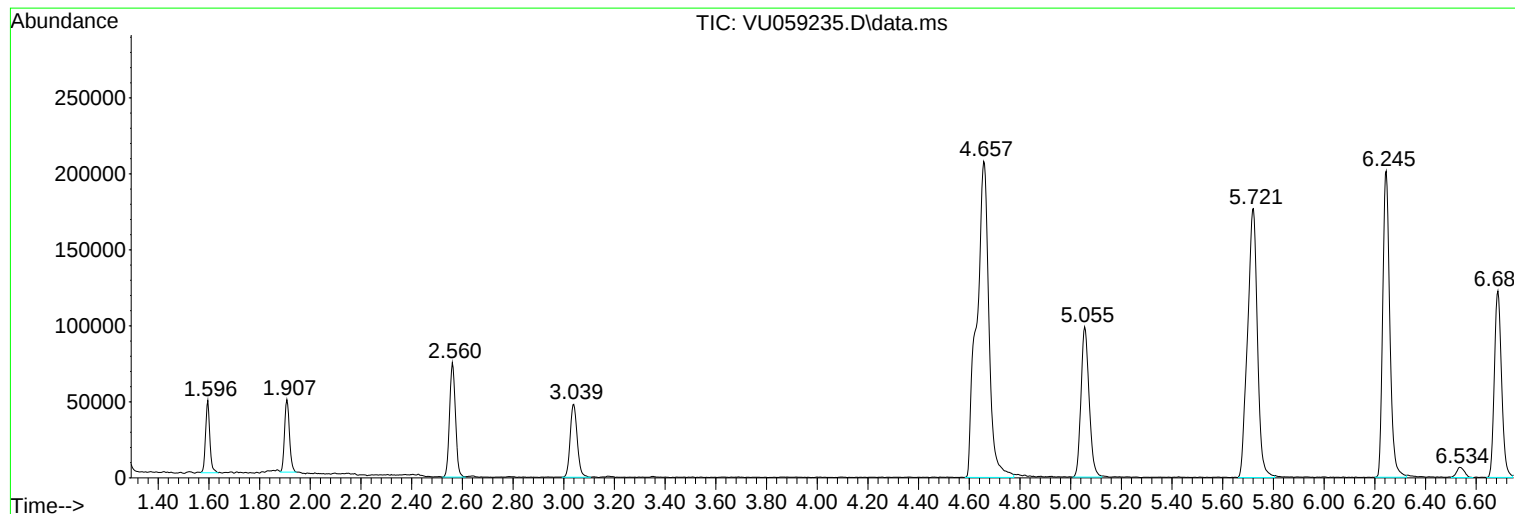

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061324\
Data File : VU059235.D
Acq On : 13 Jun 2024 15:25
Operator : MD/SY
Sample : P2850-01 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061324\
Data File : VU059235.D
Acq On : 13 Jun 2024 15:25
Operator : MD/SY
Sample : P2850-01 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAW0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc