

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061418\
 Data File : VU024545.D
 Acq On : 14 Jun 2018 17:16
 Operator : MD/SY
 Sample : J3443-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jun 15 01:37:00 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 13 13:55:26 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.99	168	170305	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.89	114	289993	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	286448	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.49	152	168449	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.31	65	132472	47.65	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.30%	
35) Dibromofluoromethane	4.89	113	118337	49.17	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.34%	
50) Toluene-d8	7.57	98	435769	49.64	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.28%	
62) 4-Bromofluorobenzene	10.31	95	169887	48.74	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.48%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.33	50	539	0.247	ug/l	95
6) Chloroethane	1.70	64	554	Below Cal	#	52
8) Diethyl Ether	1.85	74	86	Below Cal		82
11) Tert butyl alcohol	2.82	59	4005	5.923	ug/l #	72
13) Acrolein	2.24	56	107	0.301	ug/l #	1
14) Allyl chloride	2.71	41	817	0.227	ug/l #	25
16) Acetone	2.33	43	9519	6.372	ug/l	93
19) Methyl tert-butyl Ether	3.00	73	19244	2.640	ug/l #	69
20) Methylene Chloride	2.70	84	879	0.375	ug/l #	66
25) 2-Butanone	4.30	43	438	0.218	ug/l #	51
31) Cyclohexane	5.00	56	14012	1.946	ug/l #	75
36) 1,1-Dichloropropene	4.99	75	11828	3.471	ug/l #	51
38) Carbon Tetrachloride	4.99	117	16269	4.342	ug/l #	16
39) Methylcyclohexane	6.42	83	5761	1.355	ug/l #	92
52) Toluene	7.64	92	2464	0.394	ug/l	92
55) 1,1,2-Trichloroethane	8.05	97	1161	0.457	ug/l #	14
68) m/p-Xylenes	9.38	106	4887	0.992	ug/l	97
73) Isopropylbenzene	10.17	105	65800	5.088	ug/l	99
76) 1,2,3-Trichloropropane	10.31	75	84064	22.667	ug/l #	36
78) n-propylbenzene	10.59	91	32828	2.155	ug/l	98
79) 2-Chlorotoluene	10.59	91	32828	3.654	ug/l #	41
81) trans-1,4-Dichloro-2-buten	10.31	75	84064	52.461	ug/l #	100
82) 4-Chlorotoluene	10.59	91	32828	3.139	ug/l #	45
83) tert-Butylbenzene	11.10	119	18905	1.753	ug/l	88
84) 1,2,4-Trimethylbenzene	10.98	105	16042	1.404	ug/l	79
85) sec-Butylbenzene	11.33	105	57518	4.262	ug/l	98
86) p-Isopropyltoluene	11.69	119	36331	3.006	ug/l	93
89) n-Butylbenzene	11.90	91	11463	1.068	ug/l	93
90) Hexachloroethane	12.26	117	9438	4.002	ug/l #	8
92) 1,2-Dibromo-3-Chloropropan	12.65	75	1521	1.272	ug/l #	3
95) Naphthalene	13.75	128	3495	0.958	ug/l #	58

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061418\
Data File : VU024545.D
Acq On : 14 Jun 2018 17:16
Operator : MD/SY
Sample : J3443-09
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jun 15 01:37:00 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 13 13:55:26 2018
Response via : Initial Calibration

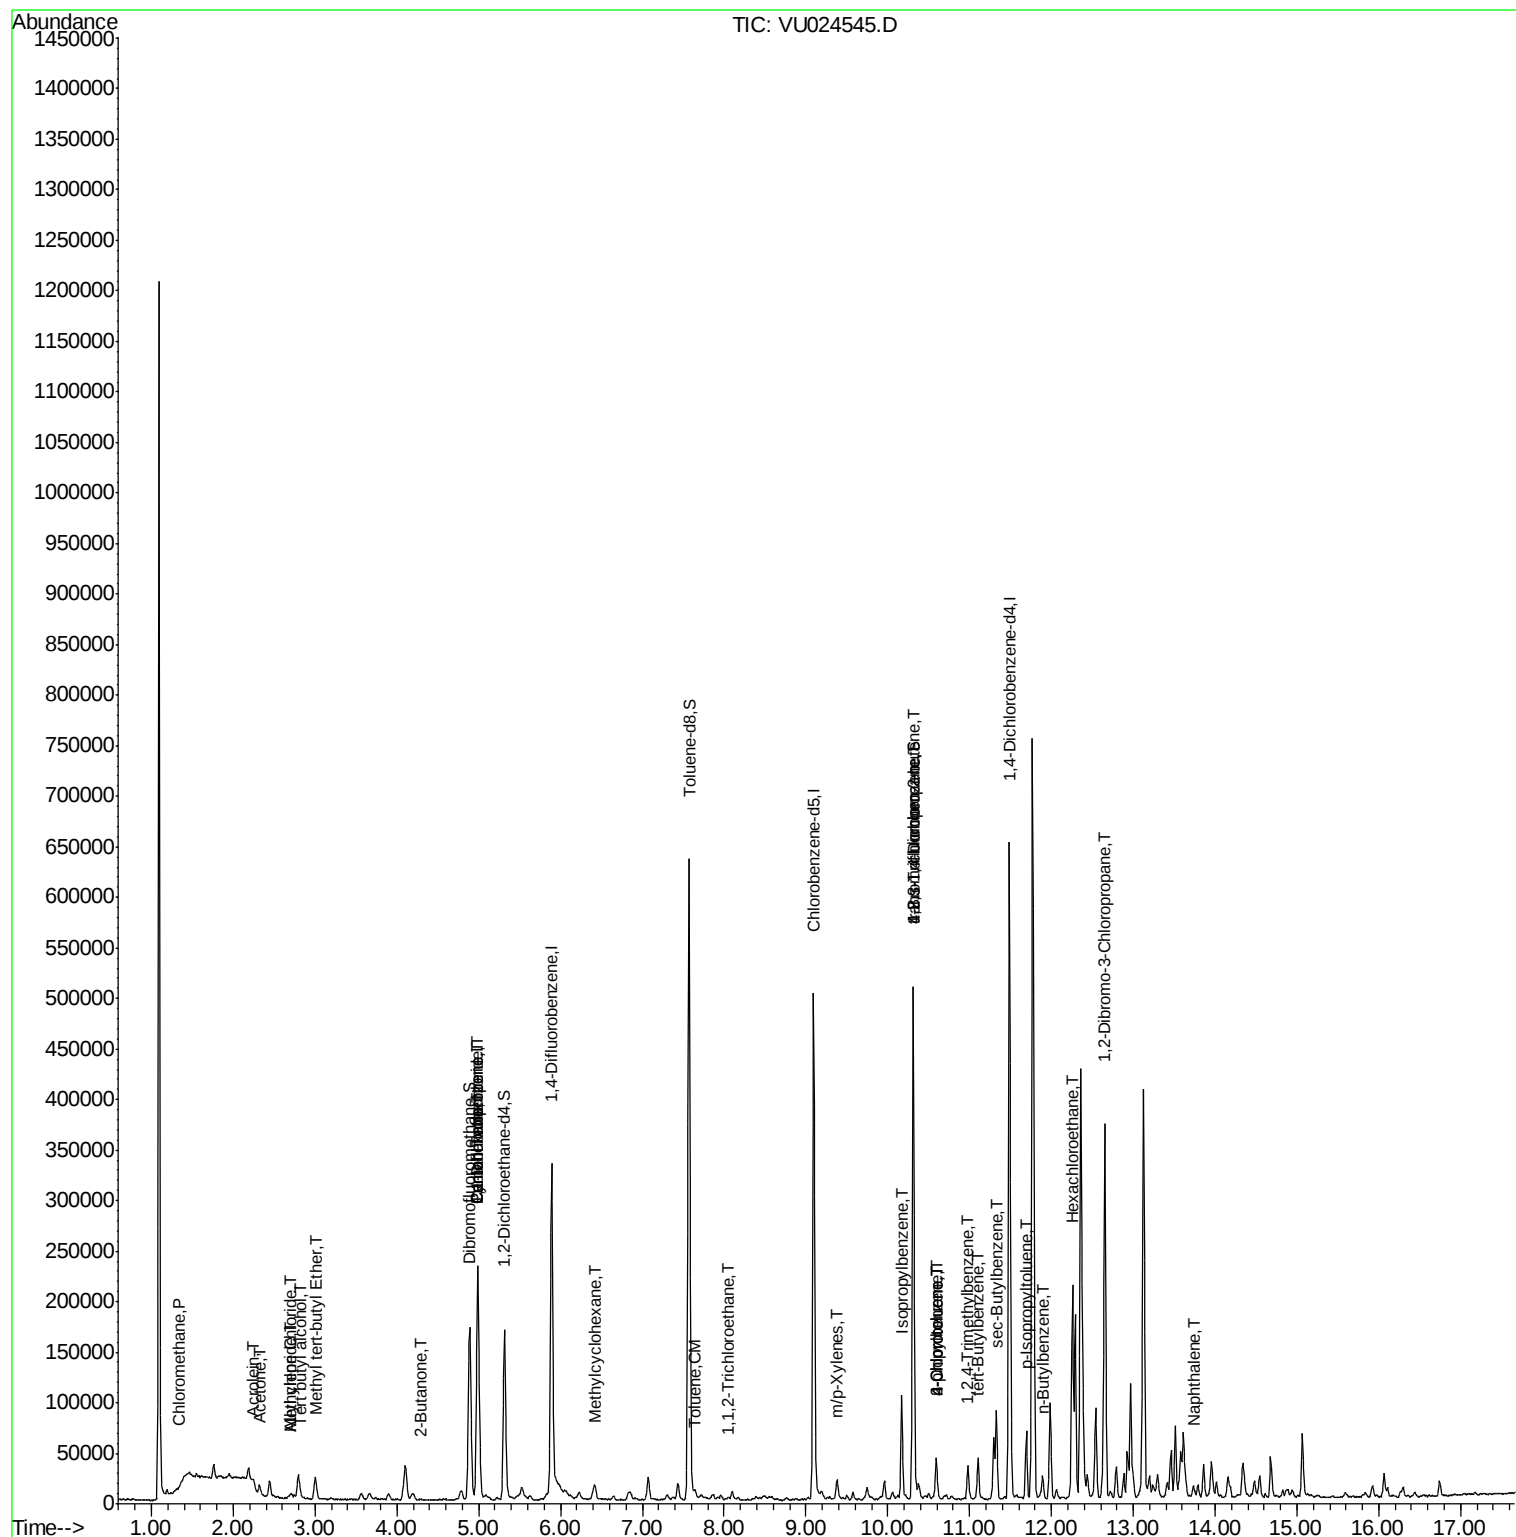



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.99 min Scan# 1368

Delta R.T. -0.00 min

Lab File: VU024545.D

Acq: 14 Jun 2018 17:16


Instrument :
MSVOA_U
ClientSampleId :

Tot Ion:168 Resp: 170305




Ion Ratio Lower Upper

168 100

99 54.2 43.2 64.8

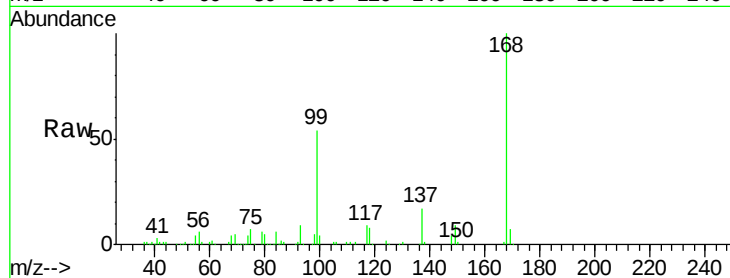

Abundance Ion 167.90 (167.60 to 168.60): VU024545.D (-1275) (-)

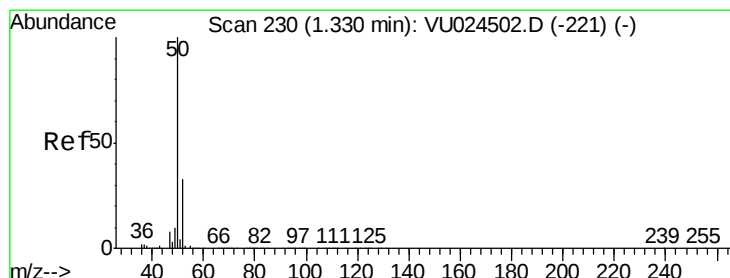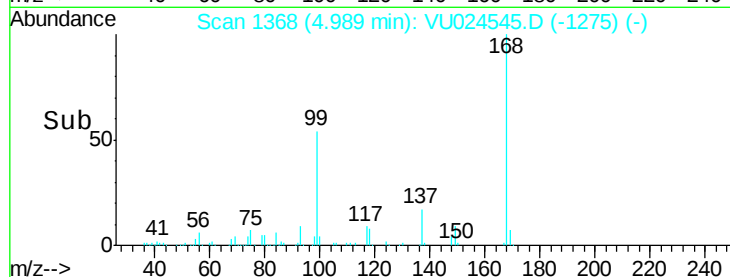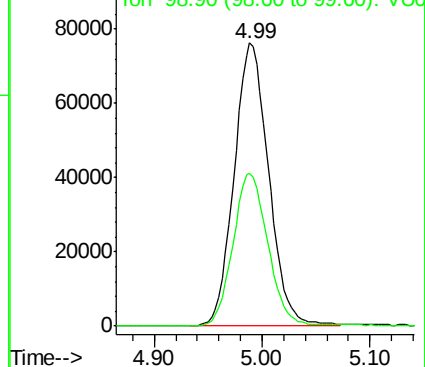

#3

Chloromethane

Concen: 0.247 ug/l

RT: 1.33 min Scan# 230

Delta R.T. -0.00 min

Lab File: VU024545.D


Acq: 14 Jun 2018 17:16

Tgt Ion: 50 Resp: 539



Ion Ratio Lower Upper


50 100

52 35.6 26.4 39.6

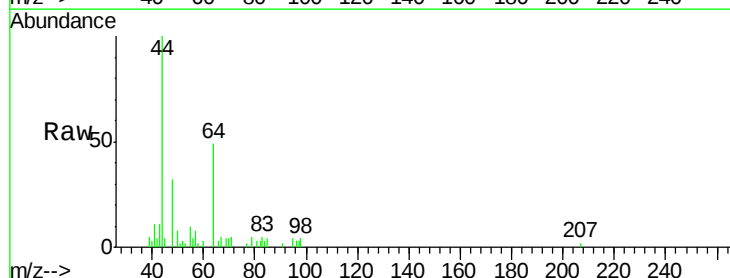

Abundance Ion 49.90 (49.60 to 50.60): VU024545.D (-137) (-)

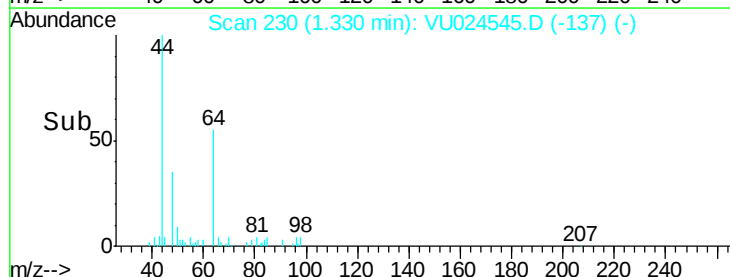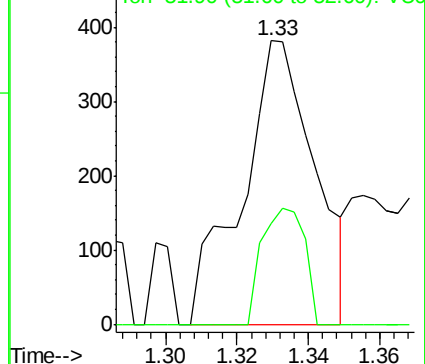

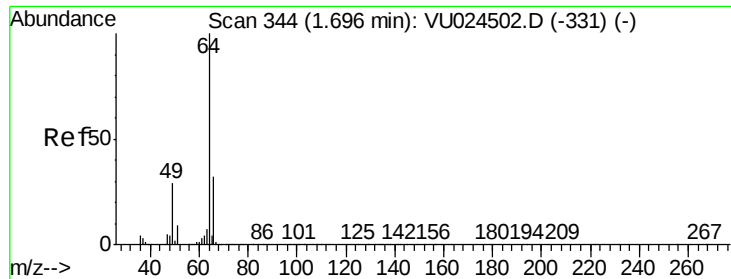

#6

Chloroethane

Concen: Below Cal

RT: 1.70 min Scan# 346

Delta R.T. 0.01 min

Lab File: VU024545.D

Acq: 14 Jun 2018 17:16

Instrument :

MSVOA_U





ClientSampleId :

Tot Ion: 64 Resp: 554

Ion Ratio Lower Upper

64 100

66 5.2 25.5 38.3#

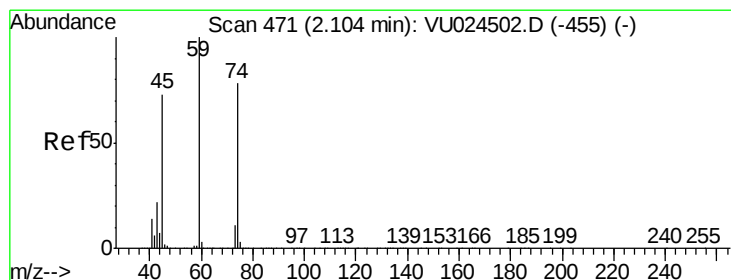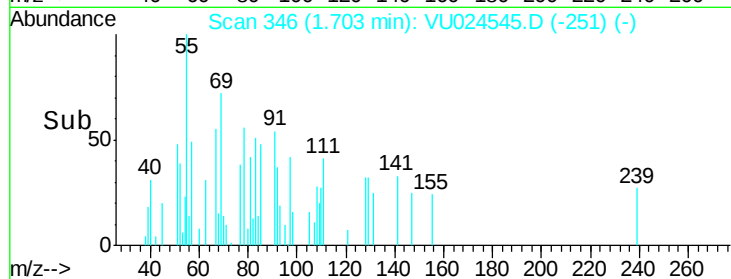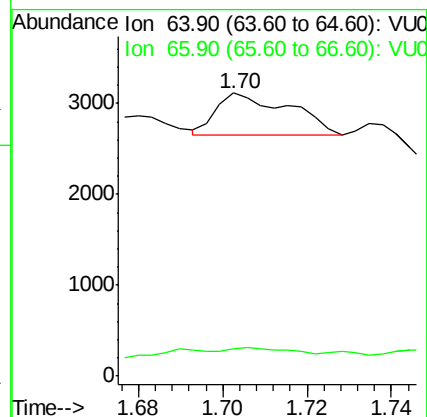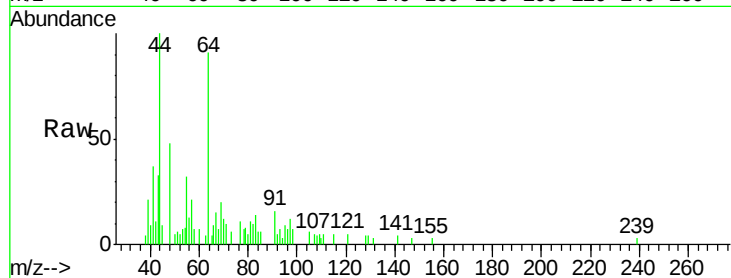

#8

Diethyl Ether

Concen: Below Cal

RT: 1.85 min Scan# 391

Delta R.T. -0.26 min

Lab File: VU024545.D




Acq: 14 Jun 2018 17:16


Tgt Ion: 74 Resp: 86

Ion Ratio Lower Upper

74 100

45 90.7 55.0 165.0

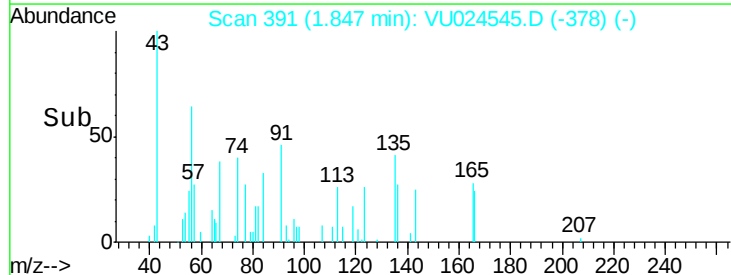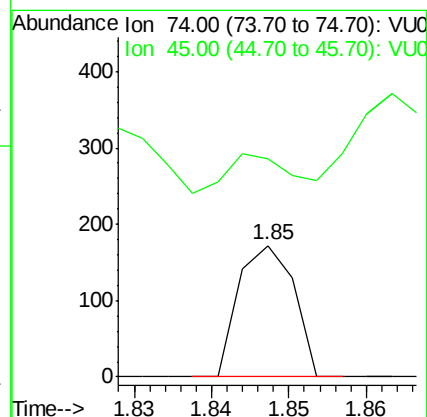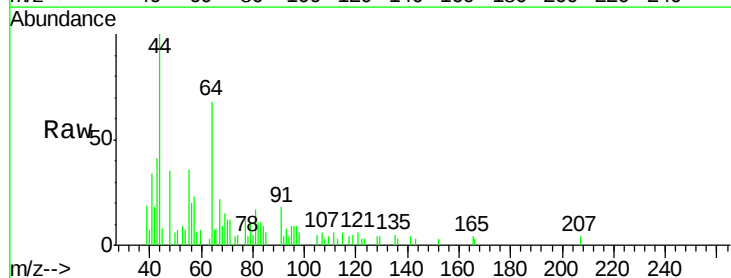




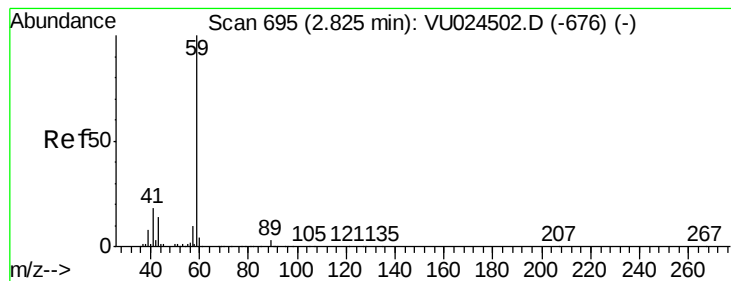


#11

Tert butyl alcohol
Concen: 5.923 ug/l
RT: 2.82 min Scan# 695
Delta R.T. -0.00 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16

Instrument :
MSVOA_U
ClientSampleId :




Tot Ion: 59 Resp: 4005
Ion Ratio Lower Upper
59 100
57 0.0 8.5 12.7#

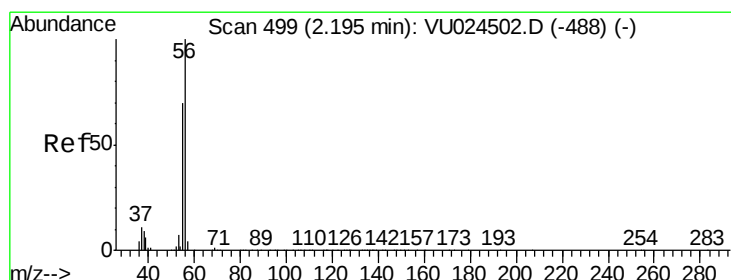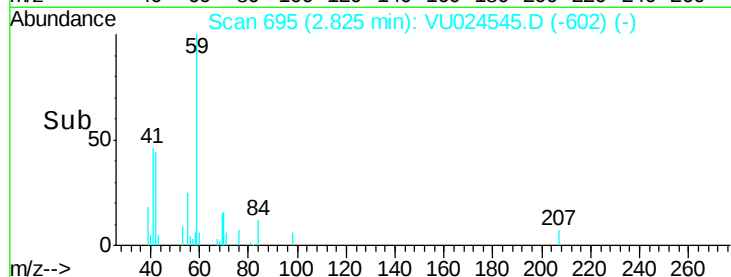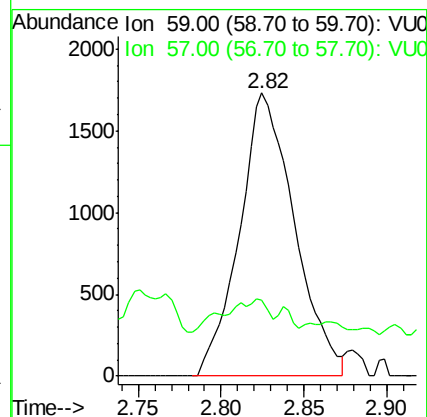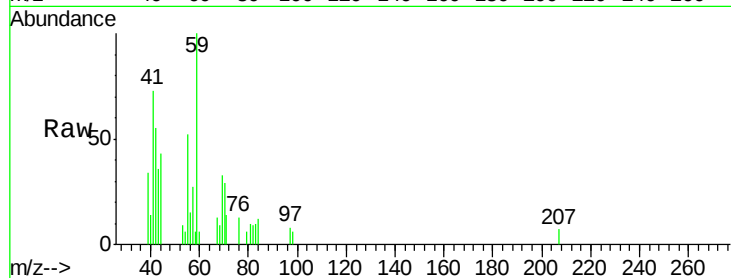


#13

Acrolein
Concen: 0.301 ug/l
RT: 2.24 min Scan# 512
Delta R.T. 0.04 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16

Tgt Ion: 56 Resp: 107
Ion Ratio Lower Upper
56 100
55 1042.1 58.4 87.6#


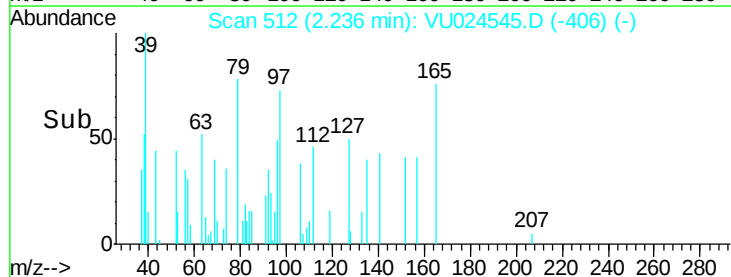
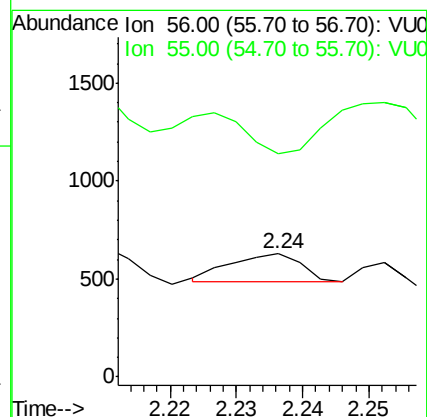
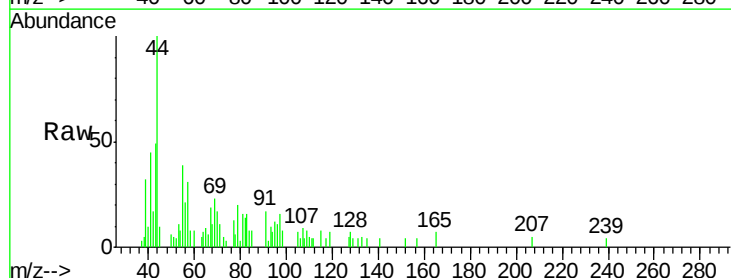




#14
 Allyl chloride
 Concen: 0.227 ug/l
 RT: 2.71 min Scan# 658
 Delta R.T. 0.11 min
 Lab File: VU024545.D
 Acq: 14 Jun 2018 17:16




Instrument :
 MSVOA_U
 ClientSampleId :


Tot Ion: 41 Resp: 817
 Ion Ratio Lower Upper
 41 100
 39 0.0 61.6 92.4#
 76 10.0 29.7 44.5#

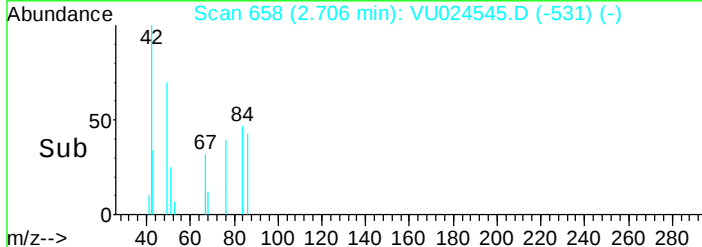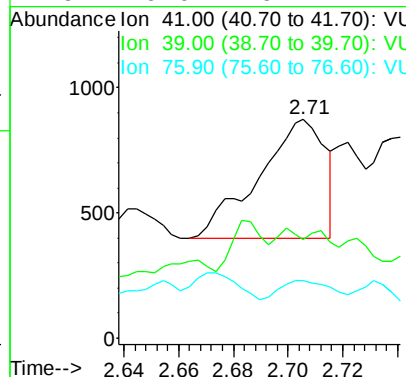

#16
 Acetone
 Concen: 6.372 ug/l
 RT: 2.33 min Scan# 540
 Delta R.T. 0.00 min
 Lab File: VU024545.D
 Acq: 14 Jun 2018 17:16

Tgt Ion: 43 Resp: 9519
 Ion Ratio Lower Upper
 43 100



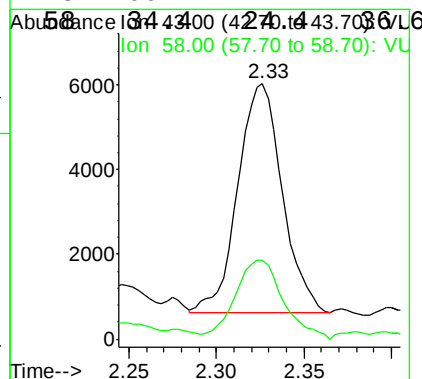





#19
Methyl tert-butyl Ether
Concen: 2.640 ug/l
RT: 3.00 min Scan# 751
Delta R.T. 0.00 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16




Instrument :
MSVOA_U
ClientSampleId :


Tot Ion: 73 Resp: 19244
Ion Ratio Lower Upper
73 100
57 38.6 18.8 28.2#

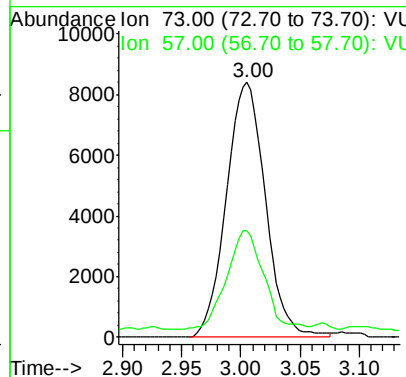

#20
Methylene Chloride
Concen: 0.375 ug/l
RT: 2.70 min Scan# 657
Delta R.T. -0.00 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16

Tgt Ion: 84 Resp: 879
Ion Ratio Lower Upper
84 100



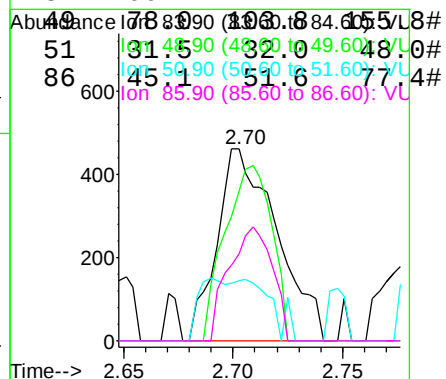



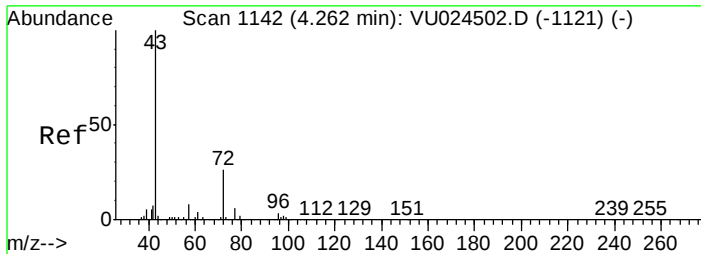

#25
2-Butanone
Concen: 0.218 ug/l
RT: 4.30 min Scan# 1154
Delta R.T. 0.04 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16




Instrument :
MSVOA_U
ClientSampleId :


Tot Ion: 43 Resp: 438
Ion Ratio Lower Upper
43 100
72 0.0 19.6 29.4#

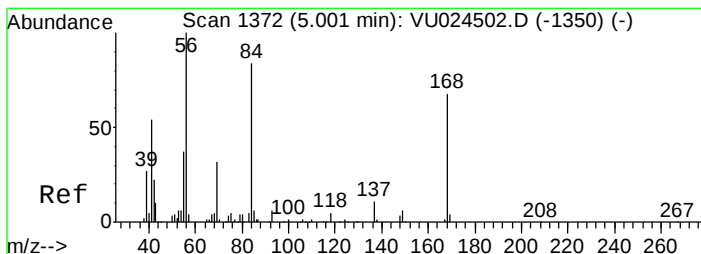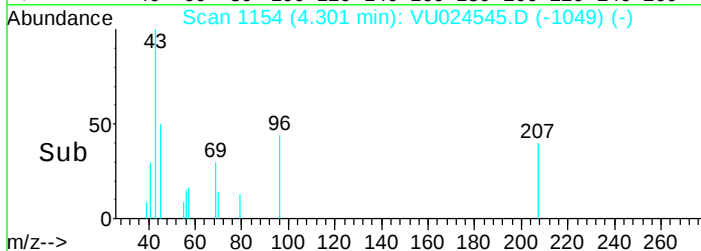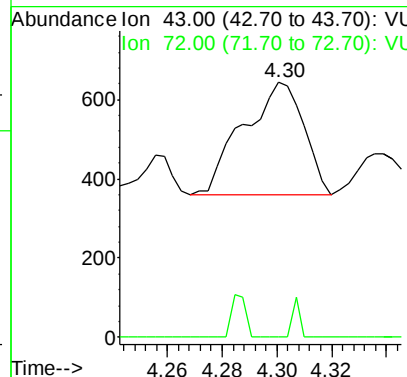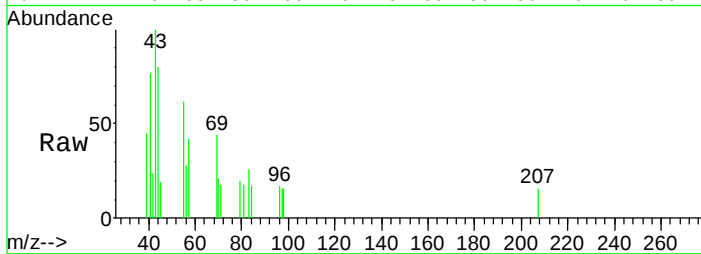

#31
Cyclohexane
Concen: 1.946 ug/l
RT: 5.00 min Scan# 1371
Delta R.T. -0.00 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16

Tgt Ion: 56 Resp: 14012
Ion Ratio Lower Upper
56 100


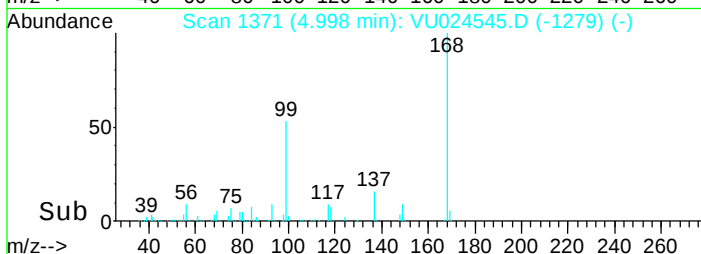
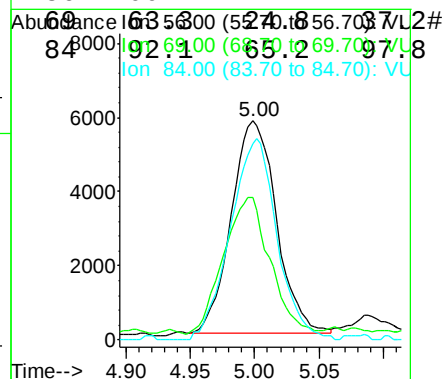
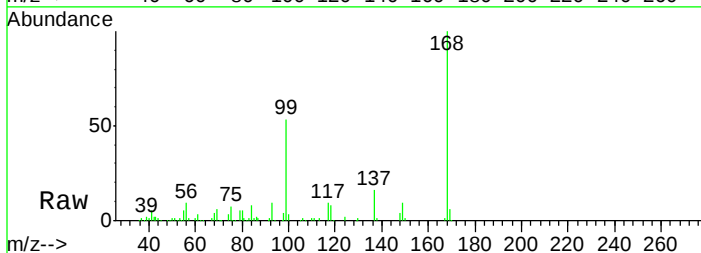


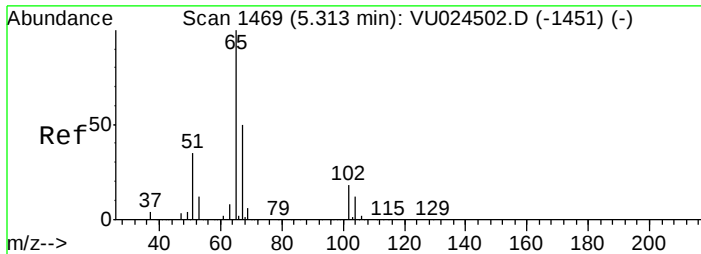

#33
 1,2-Dichloroethane-d4
 Concen: 47.647 ug/l
 RT: 5.31 min Scan# 1469
 Delta R.T. -0.00 min
 Lab File: VU024545.D
 Acq: 14 Jun 2018 17:16




Instrument :
 MSVOA_U
 ClientSampleId :


Tot Ion: 65 Resp: 132472
 Ion Ratio Lower Upper
 65 100
 67 53.2 0.0 107.0

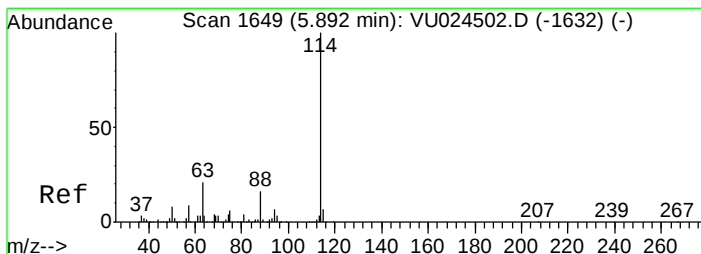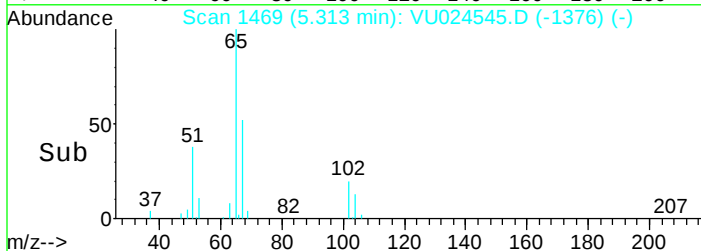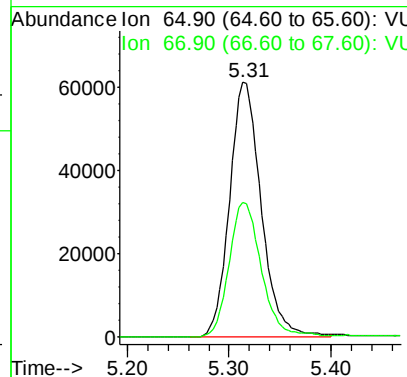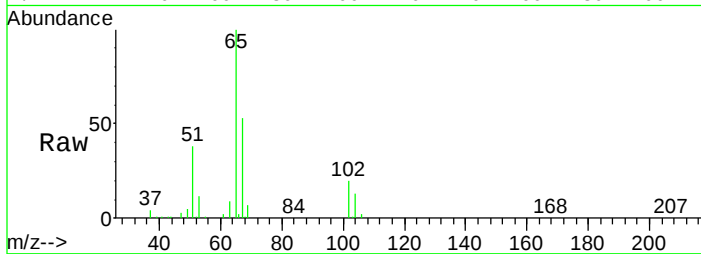

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.89 min Scan# 1649
 Delta R.T. -0.00 min
 Lab File: VU024545.D
 Acq: 14 Jun 2018 17:16

Tgt Ion:114 Resp: 289993
 Ion Ratio Lower Upper
 114 100


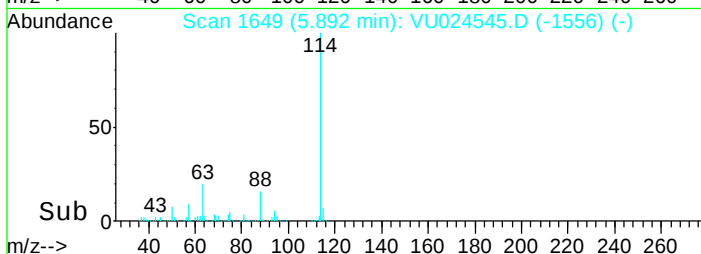
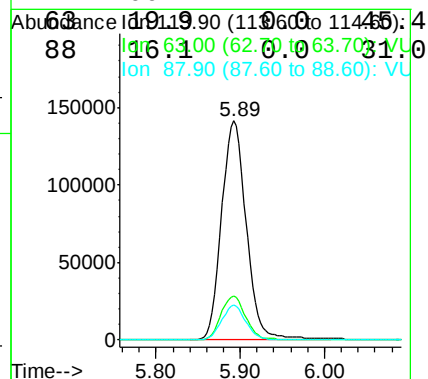
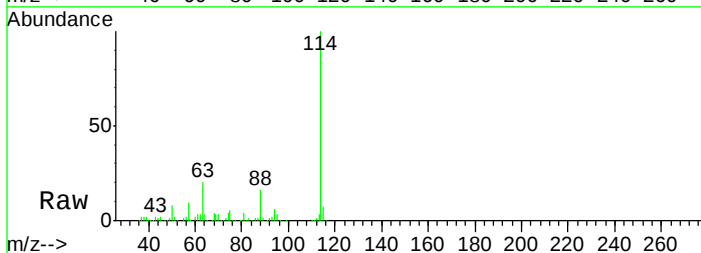




#35
 Dibromofluoromethane
 Concen: 49.169 ug/l
 RT: 4.89 min Scan# 1337
 Delta R.T. 0.00 min
 Lab File: VU024545.D
 Acq: 14 Jun 2018 17:16




Instrument :
 MSVOA_U
 ClientSampleId :


Tot Ion:113 Resp: 118337
 Ion Ratio Lower Upper
 113 100
 111 101.6 82.2 123.4
 192 21.2 16.2 24.4

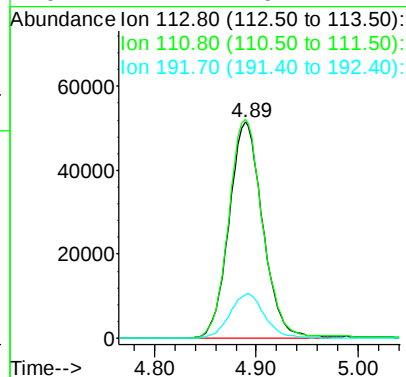

#36
 1,1-Dichloropropene
 Concen: 3.471 ug/l
 RT: 4.99 min Scan# 1368
 Delta R.T. -0.15 min
 Lab File: VU024545.D
 Acq: 14 Jun 2018 17:16

Tgt Ion: 75 Resp: 11828
 Ion Ratio Lower Upper
 75 100

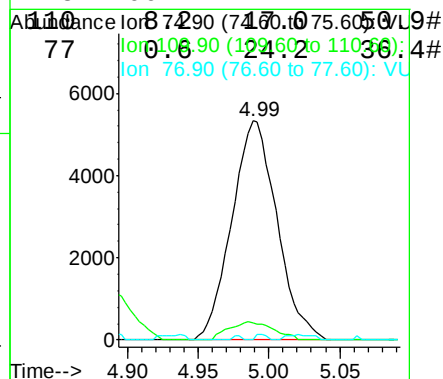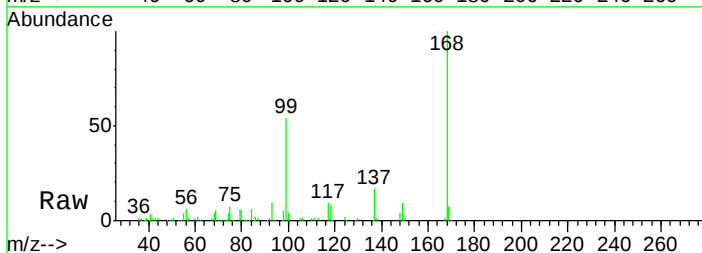







#38
Carbon Tetrachloride
Concen: 4.342 ug/l
RT: 4.99 min Scan# 1369
Delta R.T. -0.15 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16

Instrument :
MSVOA_U
ClientSampleId :

Tot Ion:117 Resp: 16269
Ion Ratio Lower Upper
117 100
119 4.9 76.1 114.1#
121 0.0 23.7 35.5#




Abundance Ion 116.80 (116.50 to 117.50):
Ion 118.80 (118.50 to 119.50):
Ion 120.80 (120.50 to 121.50):

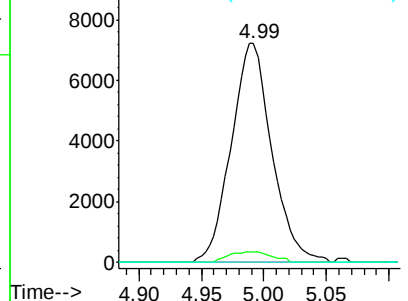




#39
Methylcyclohexane
Concen: 1.355 ug/l
RT: 6.42 min Scan# 1812
Delta R.T. -0.00 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16

Tgt Ion: 83 Resp: 5761
Ion Ratio Lower Upper
83 100



Abundance Ion 83.00 (82.70 to 83.30):
Ion 98.00 (97.70 to 98.30):



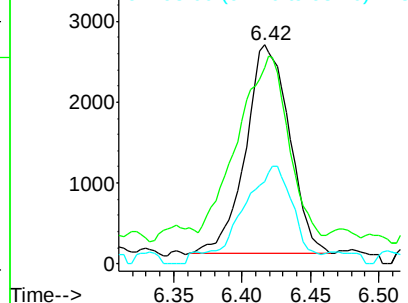





#50
Toluene-d8
Concen: 49.639 ug/l
RT: 7.57 min Scan# 2171
Delta R.T. -0.00 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16




Instrument :
MSVOA_U
ClientSampleId :


Tot Ion: 98 Resp: 435769
Ion Ratio Lower Upper
98 100
100 64.2 51.1 76.7

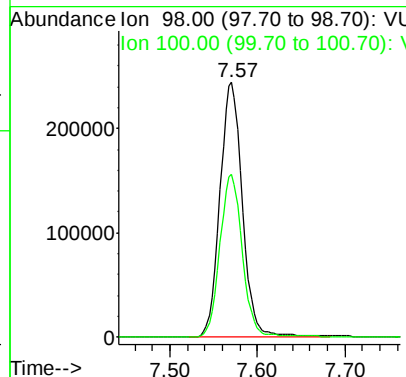

#52
Toluene
Concen: 0.394 ug/l
RT: 7.64 min Scan# 2194
Delta R.T. 0.00 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16

Tgt Ion: 92 Resp: 2464
Ion Ratio Lower Upper
92 100

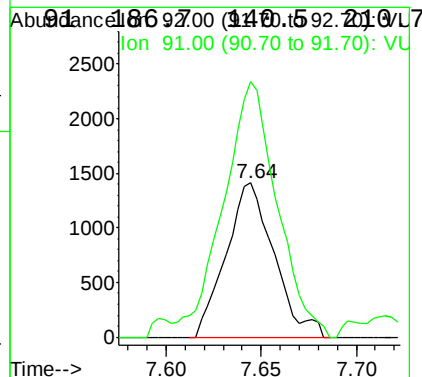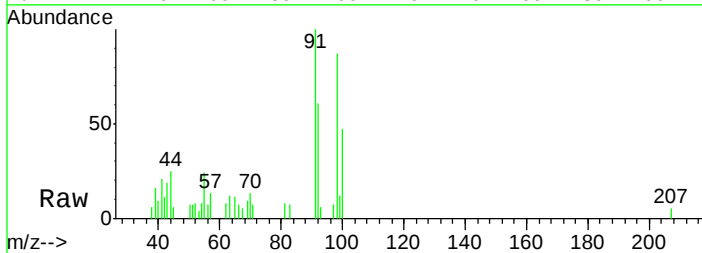


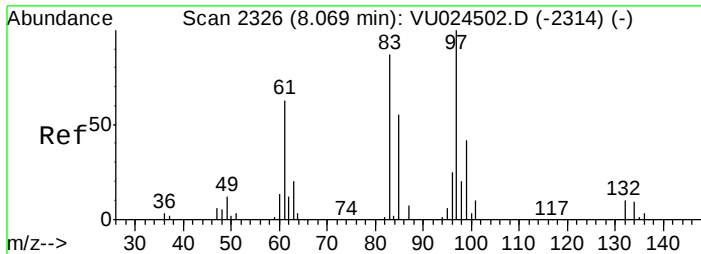




#55
1,1,2-Trichloroethane
Concen: 0.457 ug/l
RT: 8.05 min Scan# 2320
Delta R.T. -0.02 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16

Instrument :
MSVOA_U
ClientSampleId :

Tot Ion: 97 Resp: 1161
Ion Ratio Lower Upper
97 100
83 0.9 70.5 105.7#
85 0.0 46.4 69.6#

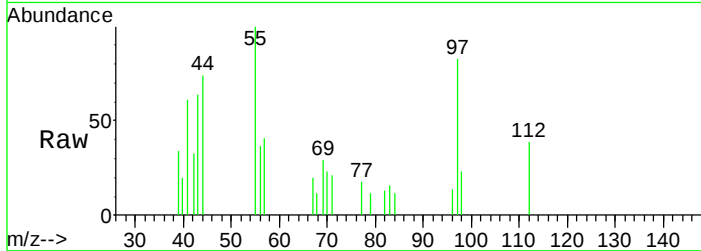


Abundance Ion 97.00 (95.60 to 98.40): VU024545.D (-2233) (-)

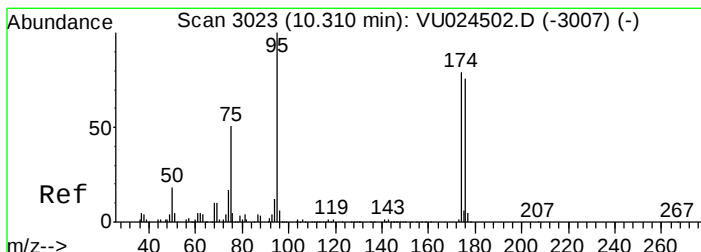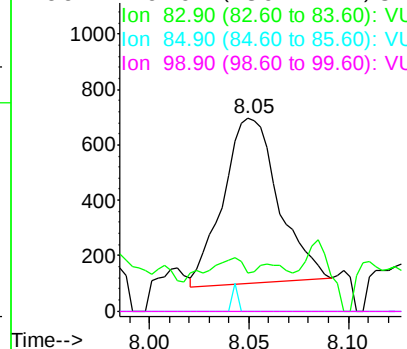
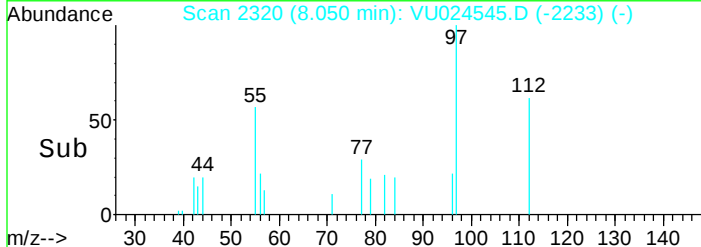



#62
4-Bromofluorobenzene
Concen: 48.741 ug/l
RT: 10.31 min Scan# 3023
Delta R.T. -0.00 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16

Tgt Ion: 95 Resp: 169887
Ion Ratio Lower Upper
95 100
174 83.2 94.0 165.8
176 81.7 175.5 159.4

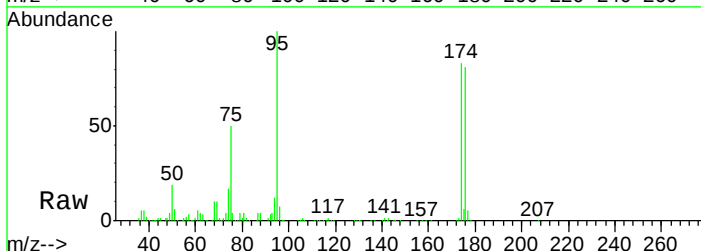

Abundance Ion 95.00 (94.00 to 96.00): VU024545.D (-2930) (-)

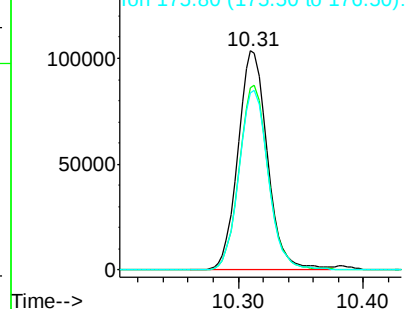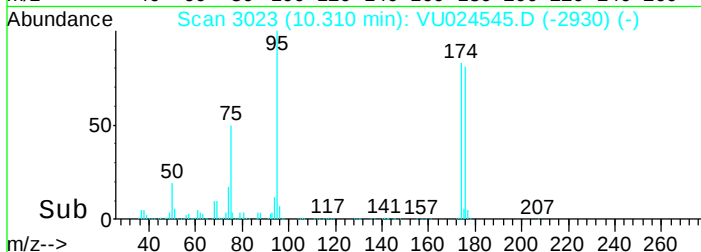







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.09 min Scan# 2645
Delta R.T. -0.00 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16

Instrument :
MSVOA_U
ClientSampleId :

Tot Ion:117 Resp: 286448
Ion Ratio Lower Upper
117 100
82 53.8 44.3 66.5
119 32.1 25.4 38.2

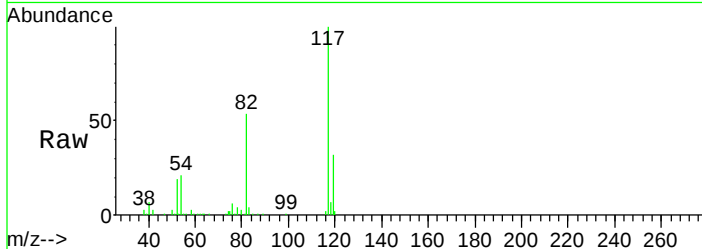


Abundance Ion 116.90 (116.60 to 117.60):
Ion 82.00 (81.70 to 82.70): VU
Ion 118.90 (118.60 to 119.60):

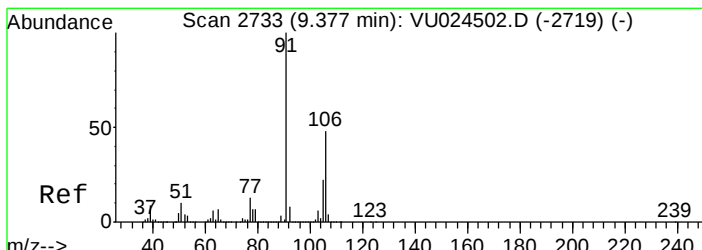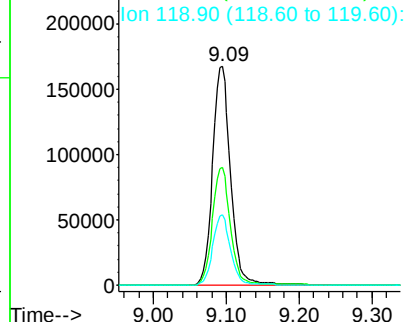
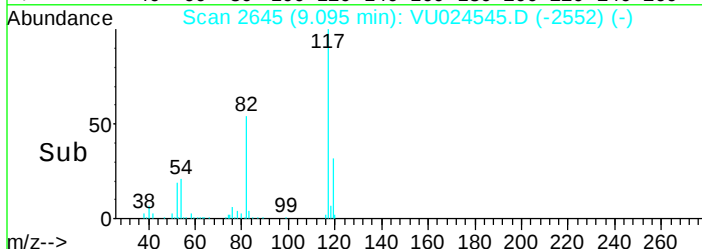



#68
m/p-Xylenes
Concen: 0.992 ug/l
RT: 9.38 min Scan# 2734
Delta R.T. 0.00 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16

Tgt Ion:106 Resp: 4887
Ion Ratio Lower Upper
106 100



Abundance Ion 106.00 (105.70 to 106.70): VU
Ion 91.00 (90.70 to 91.70): VU

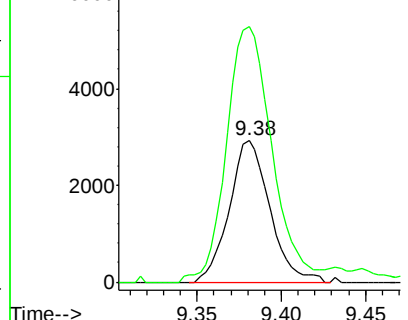







#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 11.49 min Scan# 3389
 Delta R.T. -0.00 min
 Lab File: VU024545.D
 Acq: 14 Jun 2018 17:16

Instrument :
 MSVOA_U
 ClientSampleId :

Tot Ion:152 Resp: 168449
 Ion Ratio Lower Upper
 152 100
 115 58.8 43.0 129.0
 150 157.2 0.0 354.0




Abundance Ion 151.90 (151.60 to 152.60):
 Ion 114.90 (114.60 to 115.60):
 Ion 149.90 (149.60 to 150.60):

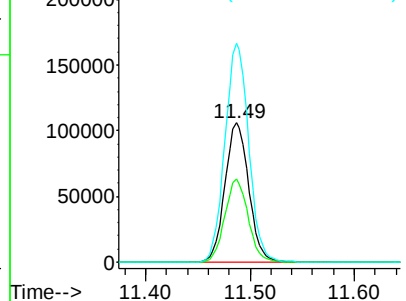




#73
 Isopropylbenzene
 Concen: 5.088 ug/l
 RT: 10.17 min Scan# 2979
 Delta R.T. -0.00 min
 Lab File: VU024545.D
 Acq: 14 Jun 2018 17:16

Tgt Ion:105 Resp: 65800
 Ion Ratio Lower Upper
 105 100



Abundance Ion 120.00 (119.70 to 120.70):
 Ion 105.00 (104.70 to 105.30):
 Ion 127.00 (126.70 to 127.30):
 Ion 137.00 (136.70 to 137.30):
 Ion 148.00 (147.70 to 148.30):
 Ion 159.00 (158.70 to 159.30):



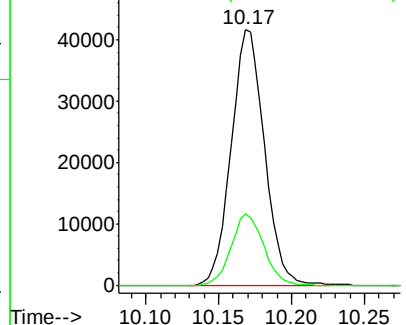





#76
1,2,3-Trichloropropane
Concen: 22.667 ug/l
RT: 10.31 min Scan# 3023
Delta R.T. -0.19 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16




Instrument :
MSVOA_U
ClientSampleId :


Tot Ion: 75 Resp: 84064
Ion Ratio Lower Upper
75 100
77 1.2 20.9 62.7#

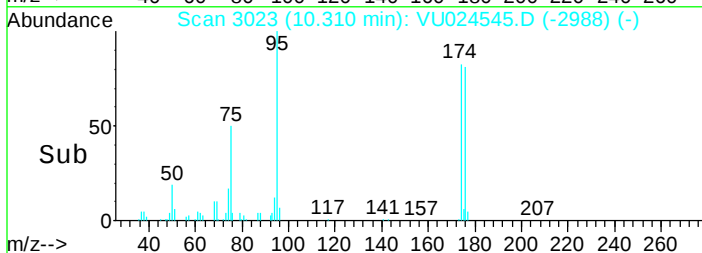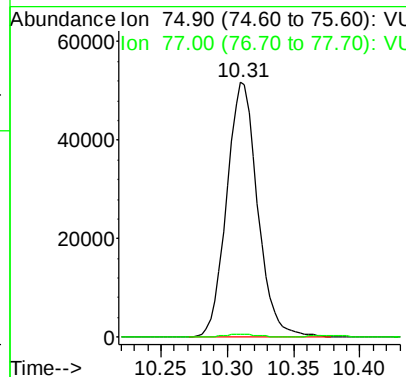

#78
n-propylbenzene
Concen: 2.155 ug/l
RT: 10.59 min Scan# 3111
Delta R.T. 0.00 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16

Tgt Ion: 91 Resp: 32828
Ion Ratio Lower Upper
91 100



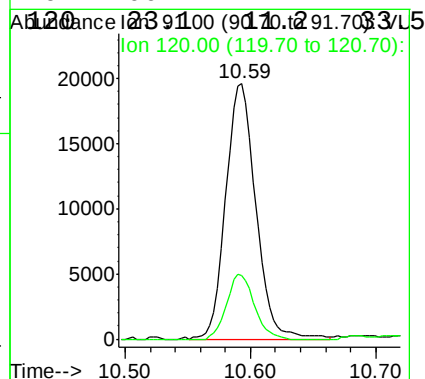
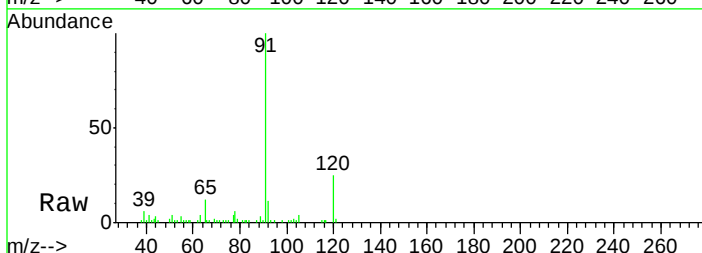




#79
 2-Chlorotoluene
 Concen: 3.654 ug/l
 RT: 10.59 min Scan# 3111
 Delta R.T. -0.07 min
 Lab File: VU024545.D
 Acq: 14 Jun 2018 17:16




Instrument :
 MSVOA_U
 ClientSampleId :


Tot Ion: 91 Resp: 32828
 Ion Ratio Lower Upper
 91 100
 126 0.0 16.9 50.7#

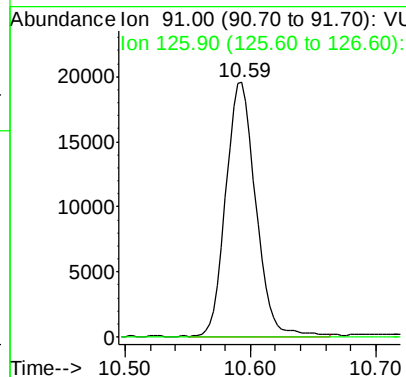

#81
 trans-1,4-Dichloro-2-butene
 Concen: 52.461 ug/l
 RT: 10.31 min Scan# 3023
 Delta R.T. -0.20 min
 Lab File: VU024545.D
 Acq: 14 Jun 2018 17:16

Tgt Ion: 75 Resp: 84064
 Ion Ratio Lower Upper
 75 100



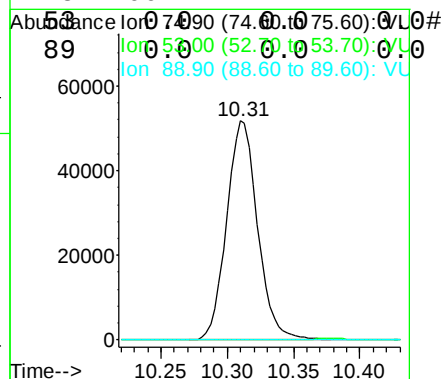





#82
4-Chlorotoluene
Concen: 3.139 ug/l
RT: 10.59 min Scan# 3111
Delta R.T. -0.18 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16




Instrument :
MSVOA_U
ClientSampleId :


Tot Ion: 91 Resp: 32828
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.9#

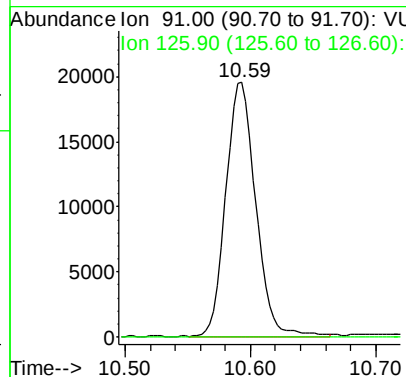

#83
tert-Butylbenzene
Concen: 1.753 ug/l
RT: 11.10 min Scan# 3270
Delta R.T. -0.00 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16

Tgt Ion: 119 Resp: 18905
Ion Ratio Lower Upper
119 100



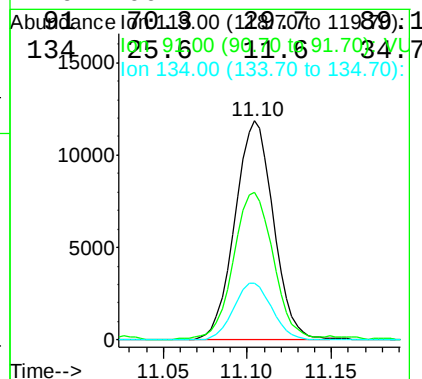
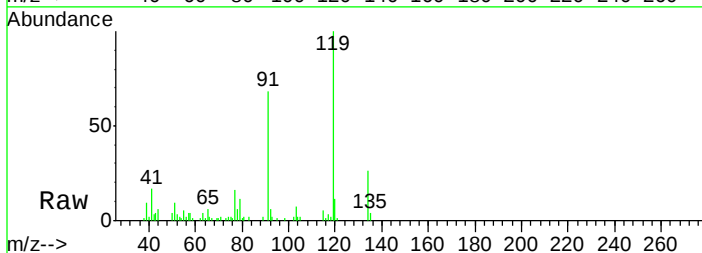




#84
 1,2,4-Trimethylbenzene
 Concen: 1.404 ug/l
 RT: 10.98 min Scan# 3230
 Delta R.T. -0.17 min
 Lab File: VU024545.D
 Acq: 14 Jun 2018 17:16




Instrument :
 MSVOA_U
 ClientSampleId :


Tgt Ion:105 Resp: 16042
 Ion Ratio Lower Upper
 105 100
 120 31.3 22.6 67.8

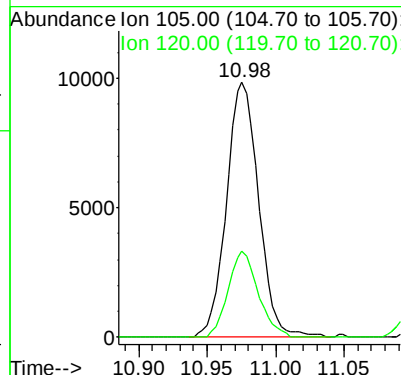

#85
 sec-Butylbenzene
 Concen: 4.262 ug/l
 RT: 11.33 min Scan# 3339
 Delta R.T. -0.00 min
 Lab File: VU024545.D
 Acq: 14 Jun 2018 17:16

Tgt Ion:105 Resp: 57518
 Ion Ratio Lower Upper
 105 100



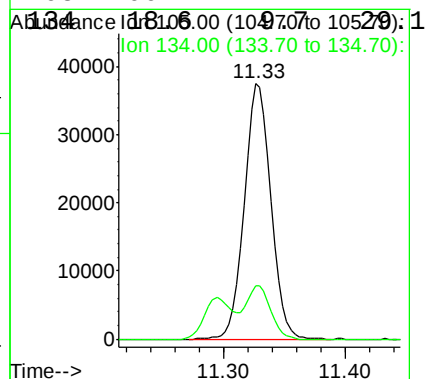
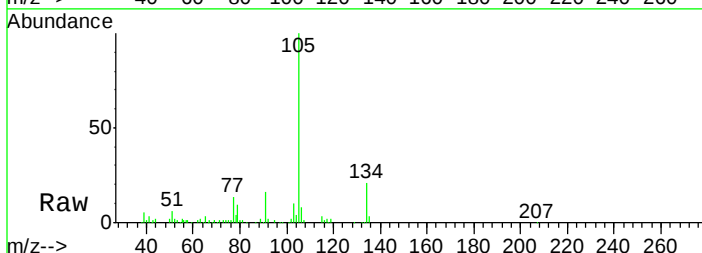




#86
p-Isopropyltoluene
Concen: 3.006 ug/l
RT: 11.69 min Scan# 3453
Delta R.T. 0.22 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16




Instrument :
MSVOA_U
ClientSampleId :


Tot Ion:119 Resp: 36331
Ion Ratio Lower Upper
119 100
134 29.2 12.9 38.6
91 27.1 12.0 36.1

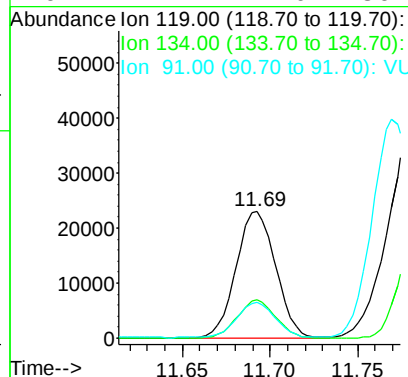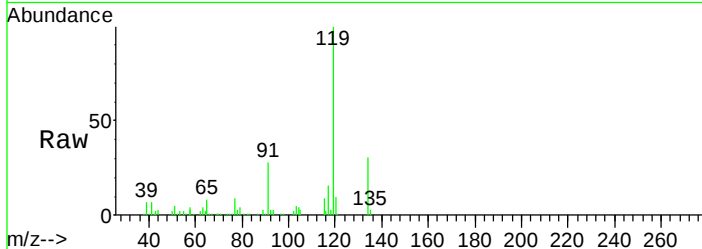

#89
n-Butylbenzene
Concen: 1.068 ug/l
RT: 11.90 min Scan# 3516
Delta R.T. 0.00 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16

Tgt Ion: 91 Resp: 11463
Ion Ratio Lower Upper
91 100



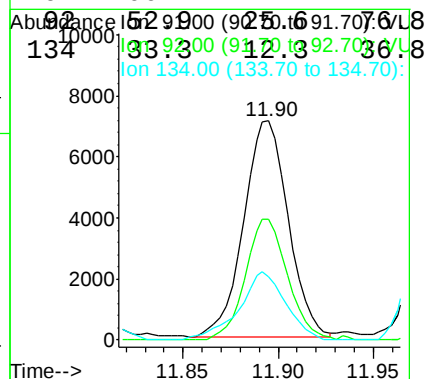
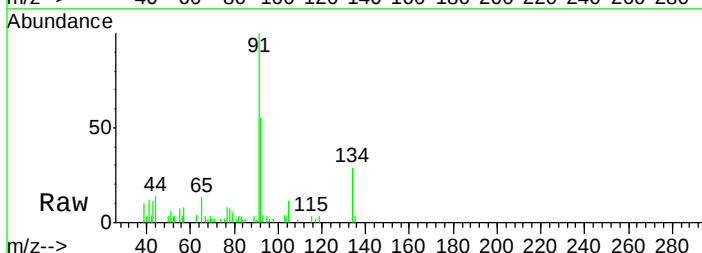




#90
Hexachloroethane
Concen: 4.002 ug/l
RT: 12.26 min Scan# 3628
Delta R.T. 0.11 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16




Instrument :
MSVOA_U
ClientSampleId :


Tot Ion:117 Resp: 9438
Ion Ratio Lower Upper
117 100
201 0.0 41.1 123.3#

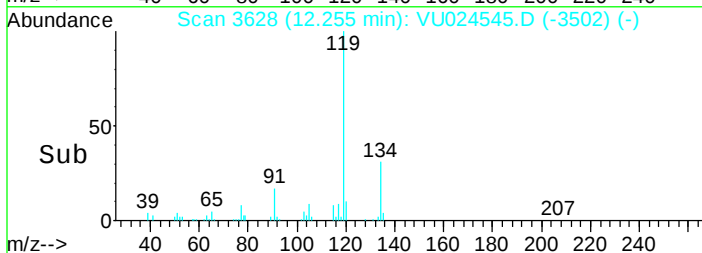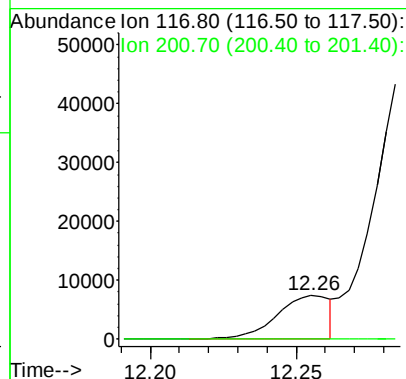

#92
1,2-Dibromo-3-Chloropropane
Concen: 1.272 ug/l
RT: 12.65 min Scan# 3751
Delta R.T. -0.01 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16


Tgt Ion: 75 Resp: 1521
Ion Ratio Lower Upper
75 100

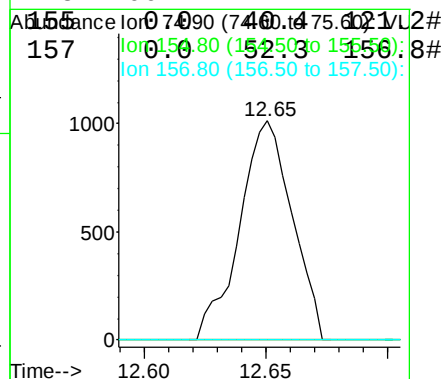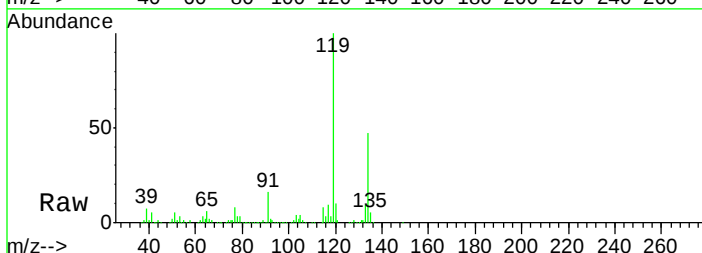



#95
Naphthalene
Concen: 0.958 ug/l
RT: 13.75 min Scan# 4093
Delta R.T. 0.01 min
Lab File: VU024545.D
Acq: 14 Jun 2018 17:16

Instrument :
MSVOA_U
ClientSampleId :



Tot Ion:128 Resp: 3495
Ion Ratio Lower Upper
128 100
127 18.5 10.6 16.0#
129 40.0 8.6 12.8#

