

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061418\
 Data File : VU024563.D
 Acq On : 15 Jun 2018 00:59
 Operator : MD/SY
 Sample : J3452-03
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 KY038PS033-180611

Quant Time: Jun 15 05:35:01 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 13 13:55:26 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.99	168	185731	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.89	114	304820	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	292401	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.49	152	170981	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.32	65	134150	44.24	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.48%	
35) Dibromofluoromethane	4.89	113	122920	48.59	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.18%	
50) Toluene-d8	7.57	98	447171	48.46	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.92%	
62) 4-Bromofluorobenzene	10.31	95	169630	46.30	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.60%	
Target Compounds						
16) Acetone	2.32	43	10418	6.395	ug/l #	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061418\
Data File : VU024563.D
Acq On : 15 Jun 2018 00:59
Operator : MD/SY
Sample : J3452-03
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
KY038PS033-180611

Quant Time: Jun 15 05:35:01 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 13 13:55:26 2018
Response via : Initial Calibration

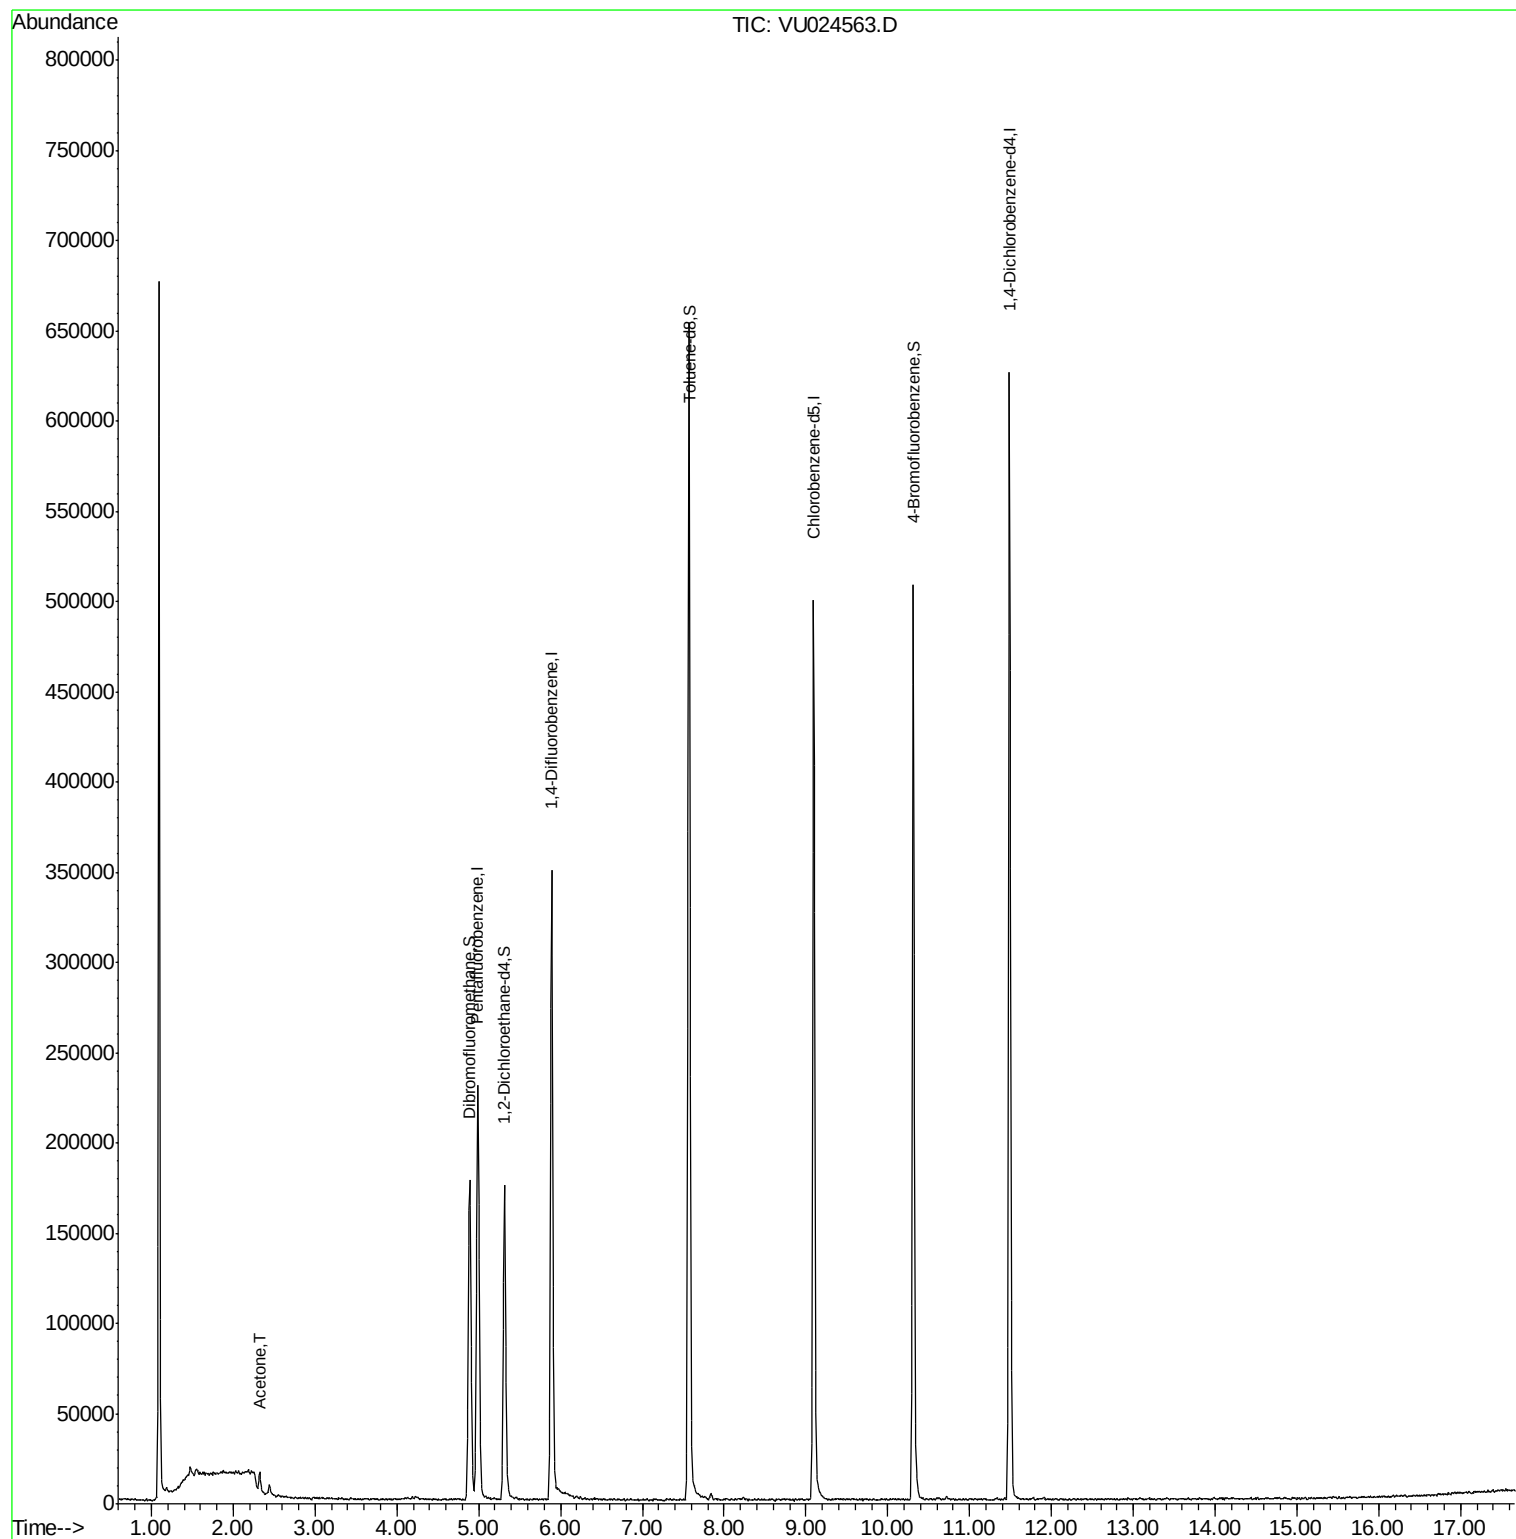

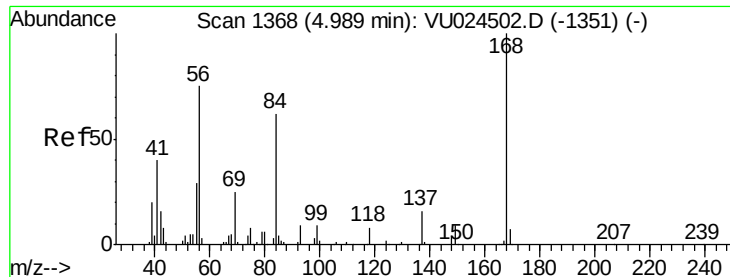

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.99 min Scan# 1369

Delta R.T. 0.00 min

Lab File: VU024563.D

Acq: 15 Jun 2018 00:59

Instrument :

MSVOA_U

ClientSampleId :


KY038PS033-180611

Tot Ion:168 Resp: 185731

Ion Ratio Lower Upper




168 100

99 51.9 43.2 64.8

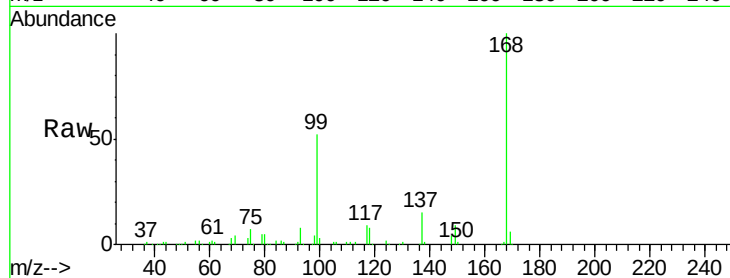

Abundance Ion 167.90 (167.60 to 168.60): VU024502.D (-1351) (-)

Ion 98.90 (98.60 to 99.60): VU024502.D (-1351) (-)

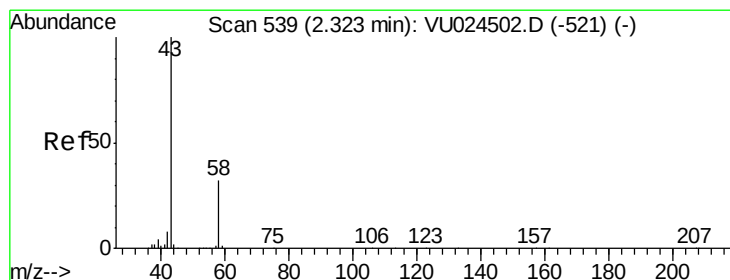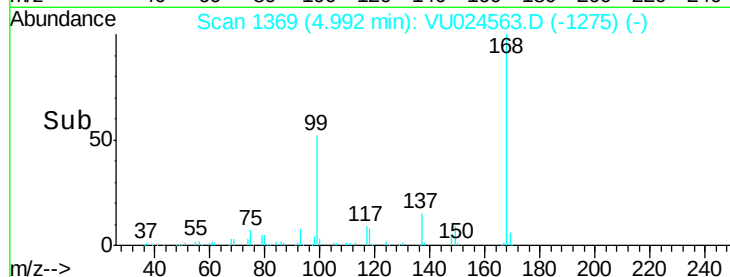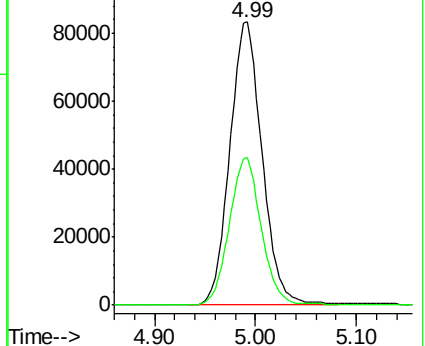

#16

Acetone

Concen: 6.395 ug/l

RT: 2.32 min Scan# 539

Delta R.T. -0.00 min

Lab File: VU024563.D


Acq: 15 Jun 2018 00:59

Tgt Ion: 43 Resp: 10418

Ion Ratio Lower Upper



43 100


58 36.7 24.4 36.6#

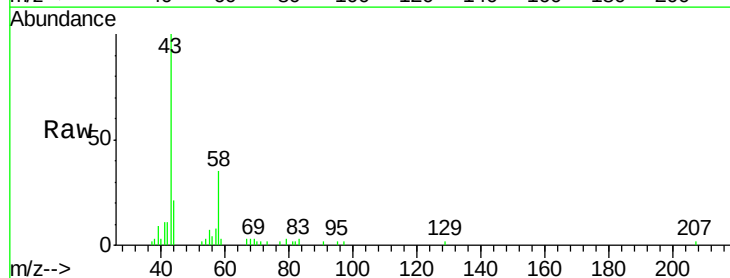

Abundance Ion 43.00 (42.70 to 43.70): VU024502.D (-521) (-)

Ion 58.00 (57.70 to 58.70): VU024502.D (-521) (-)



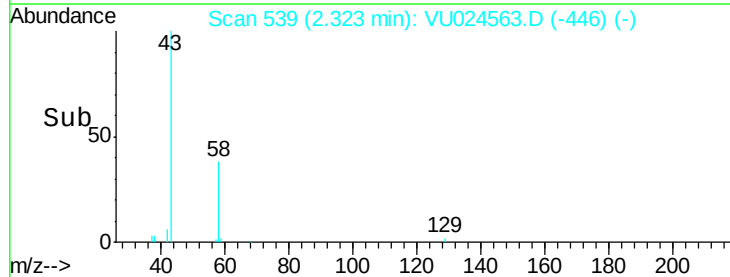
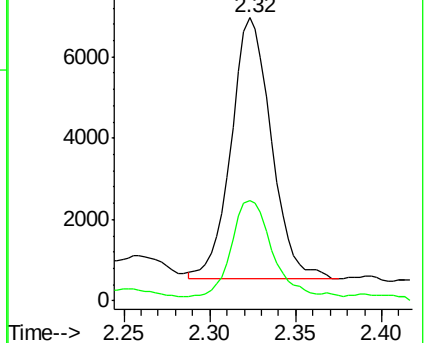


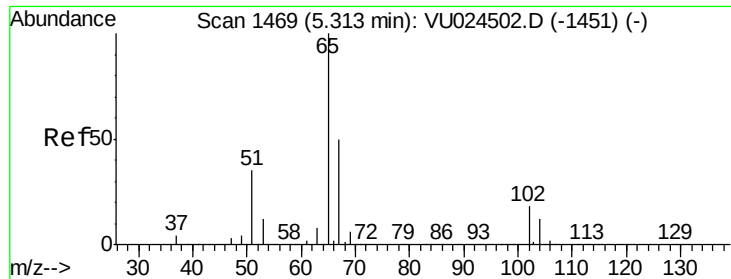

#33
 1,2-Dichloroethane-d4
 Concen: 44.243 ug/l
 RT: 5.32 min Scan# 1470
 Delta R.T. 0.00 min
 Lab File: VU024563.D
 Acq: 15 Jun 2018 00:59




Instrument :
 MSVOA_U
 ClientSampleId :
 KY038PS033-180611


Tot Ion: 65 Resp: 134150
 Ion Ratio Lower Upper
 65 100
 67 53.3 0.0 107.0

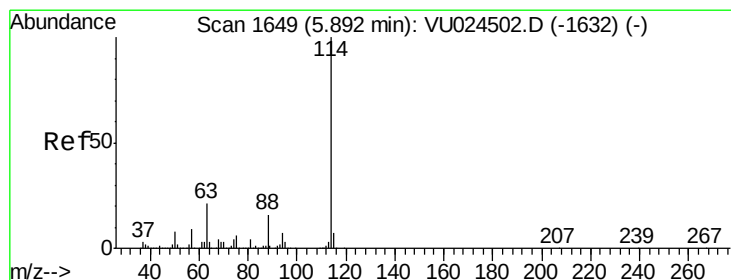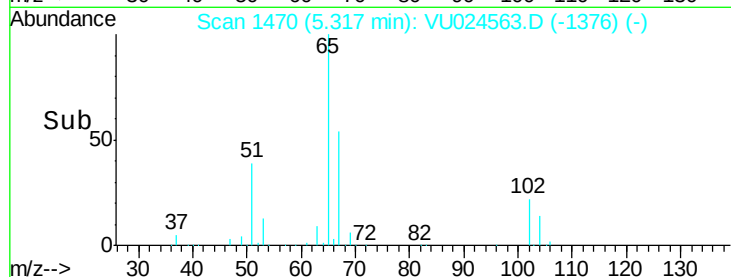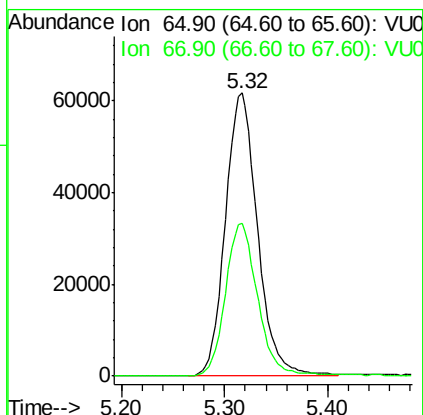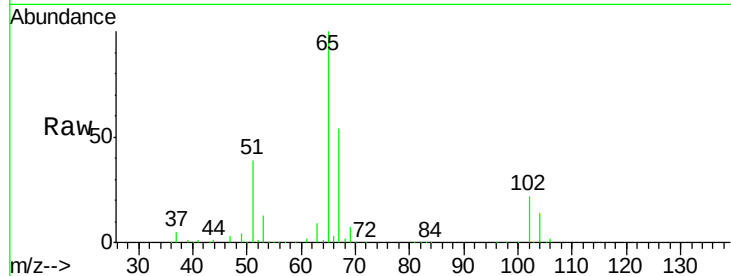

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.89 min Scan# 1649
 Delta R.T. -0.00 min
 Lab File: VU024563.D
 Acq: 15 Jun 2018 00:59

Tgt Ion: 114 Resp: 304820
 Ion Ratio Lower Upper
 114 100
 63 19.9 0.0 45.4
 88 16.1 0.0 31.0

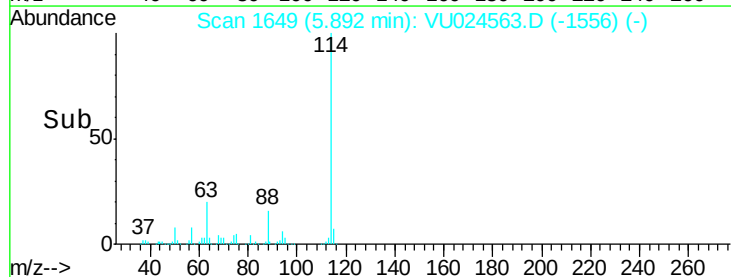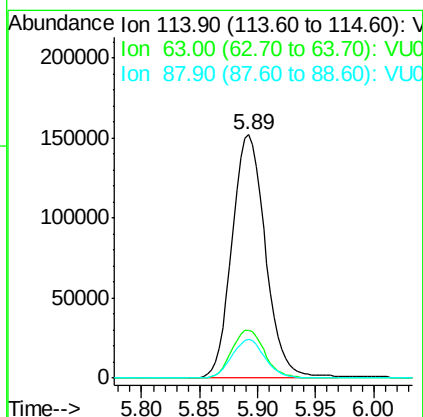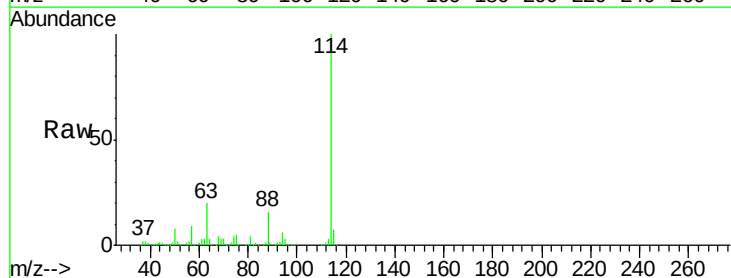


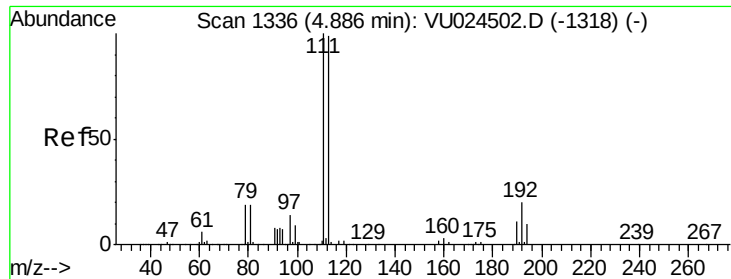




#35
 Dibromofluoromethane
 Concen: 48.589 ug/l
 RT: 4.89 min Scan# 1337
 Delta R.T. 0.00 min
 Lab File: VU024563.D
 Acq: 15 Jun 2018 00:59

Instrument :
 MSVOA_U
 ClientSampleId :
 KY038PS033-180611

Tot Ion	Ratio	Lower	Upper
113	100		
111	101.0	82.2	123.4
192	21.6	16.2	24.4

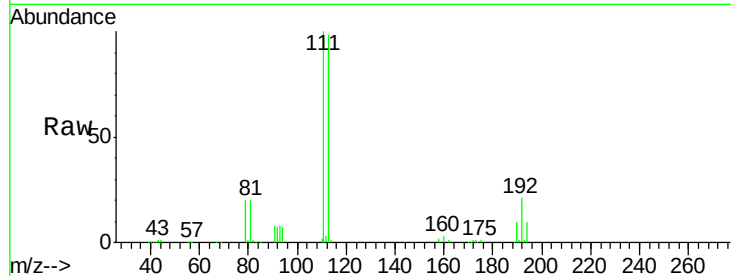


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

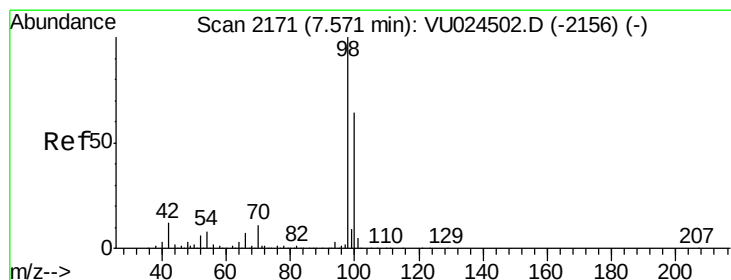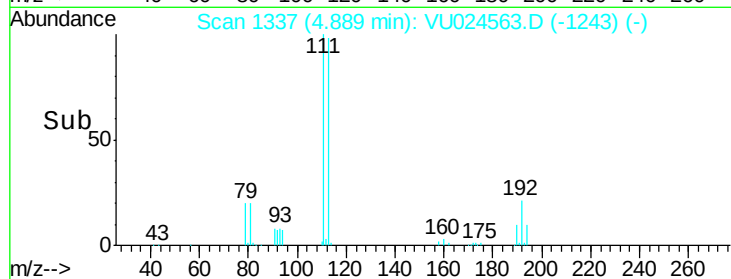
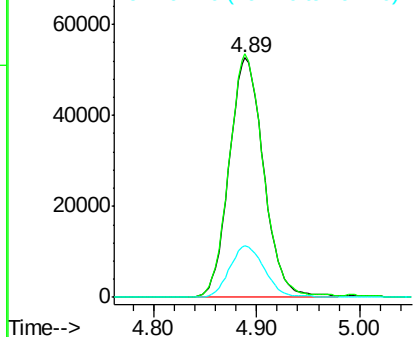



#50
 Toluene-d8
 Concen: 48.460 ug/l
 RT: 7.57 min Scan# 2171
 Delta R.T. -0.00 min
 Lab File: VU024563.D
 Acq: 15 Jun 2018 00:59

Tgt Ion	Ratio	Lower	Upper
98	100		
100	64.2	51.1	76.7

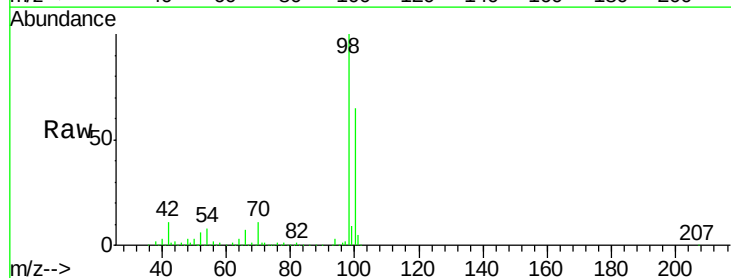

Abundance Ion 98.00 (97.70 to 98.70): VU0
 Ion 100.00 (99.70 to 100.70): VU



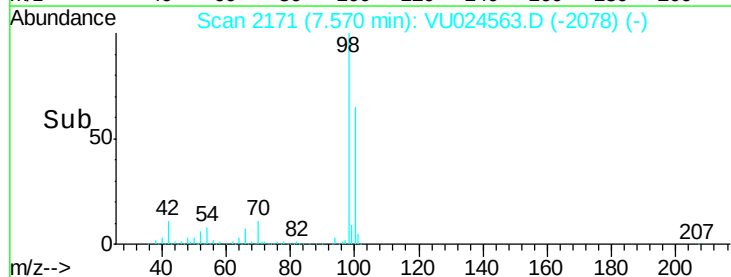
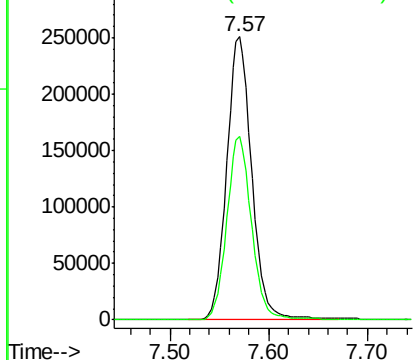


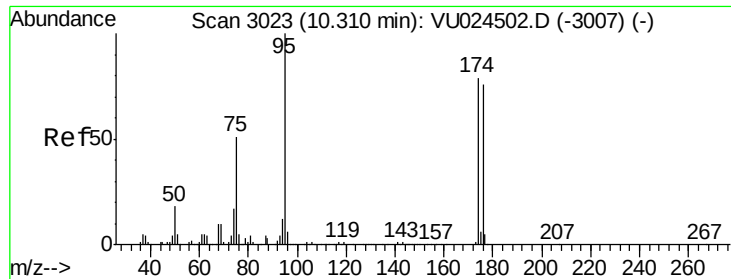

#62
4-Bromofluorobenzene
Concen: 46.300 ug/l
RT: 10.31 min Scan# 3024
Delta R.T. 0.00 min
Lab File: VU024563.D
Acq: 15 Jun 2018 00:59




Instrument :
MSVOA_U
ClientSampleId :
KY038PS033-180611


Tot Ion	95	Resp	169630
Ion Ratio	Lower	Upper	
95	100		
174	86.7	0.0	165.8
176	85.1	0.0	159.4

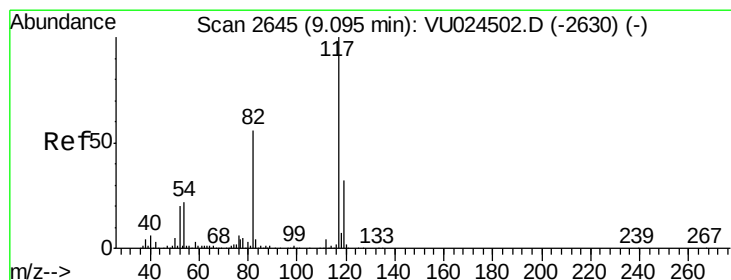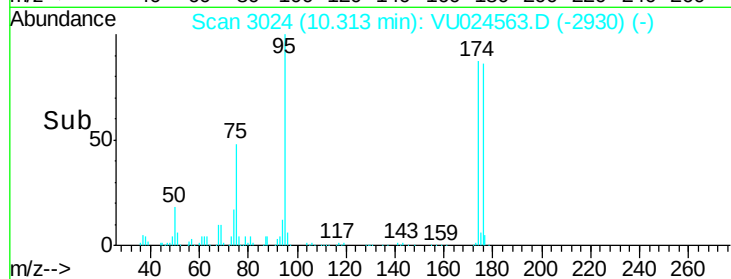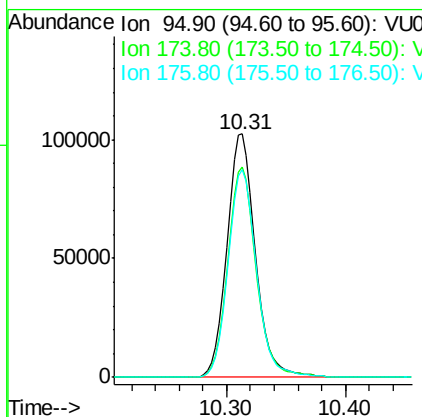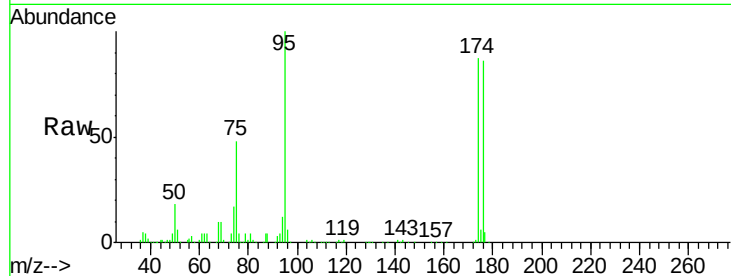

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.09 min Scan# 2645
Delta R.T. -0.00 min
Lab File: VU024563.D
Acq: 15 Jun 2018 00:59

Tgt Ion	117	Resp	292401
Ion Ratio	Lower	Upper	
117	100		
82	54.0	44.3	66.5
119	32.2	25.4	38.2

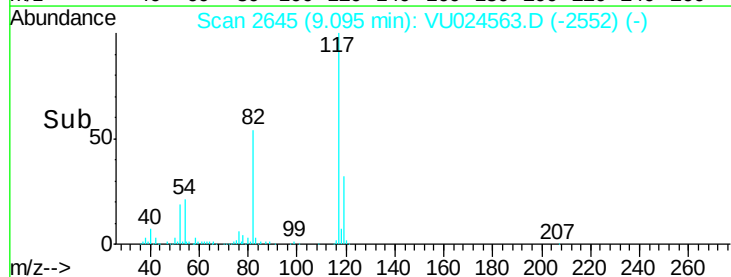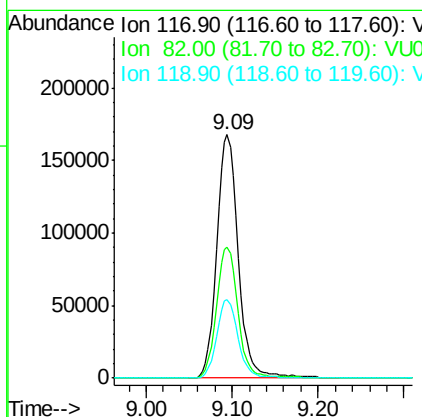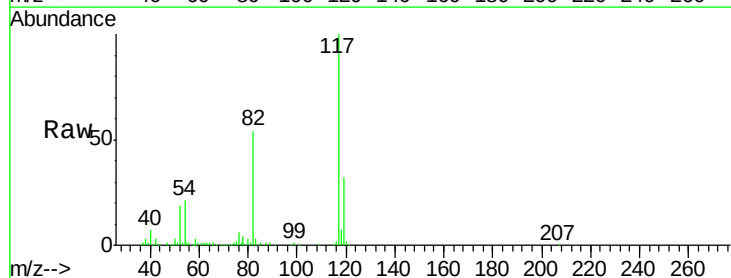

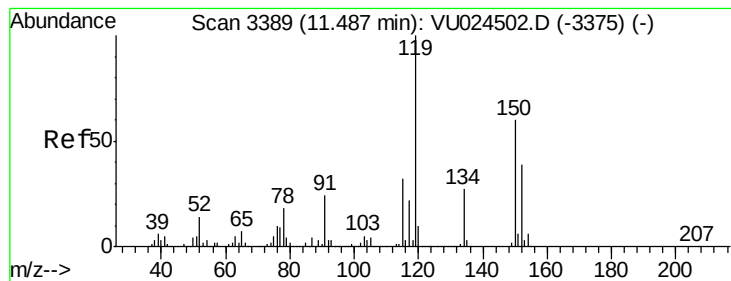

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.49 min Scan# 3389

Delta R.T. -0.00 min

Lab File: VU024563.D

Acq: 15 Jun 2018 00:59

Instrument :

MSVOA_U

ClientSampleId :

KY038PS033-180611


Tot Ion:152 Resp: 170981

Ion Ratio Lower Upper

152 100

115 57.4 43.0 129.0

150 155.6 0.0 354.0

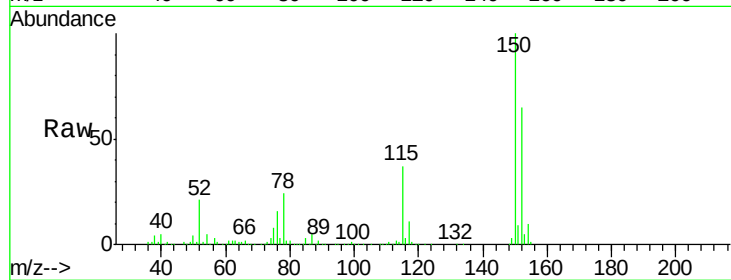

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

