

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061418\
 Data File : VU024548.D
 Acq On : 14 Jun 2018 18:26
 Operator : MD/SY
 Sample : J3451-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VB-25830-SLUDGEBOX

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.091	147	156	179	rBV	3603976	4155503	100.00%	38.618%
2	2.323	531	539	554	rVB	37311	60563	1.46%	0.563%
3	4.641	1244	1260	1285	rBV	104059	255268	6.14%	2.372%
4	4.889	1321	1337	1354	rBV	170284	386852	9.31%	3.595%
5	4.988	1354	1368	1386	rVB	213094	468829	11.28%	4.357%
6	5.313	1451	1469	1489	rBV	165128	359691	8.66%	3.343%
7	5.892	1634	1649	1670	rBV	333663	675435	16.25%	6.277%
8	7.570	2157	2171	2189	rBV	629405	1120274	26.96%	10.411%
9	9.094	2632	2645	2677	rBV	498149	850513	20.47%	7.904%
10	10.310	3011	3023	3051	rBV	508803	827004	19.90%	7.686%
11	11.152	3275	3285	3297	rVB	33539	52859	1.27%	0.491%
12	11.487	3378	3389	3406	rVB	634772	1011554	24.34%	9.401%
13	11.773	3463	3478	3487	rBV3	29800	61842	1.49%	0.575%
14	13.126	3879	3899	3909	rBV3	50830	89698	2.16%	0.834%
15	13.747	4080	4092	4102	rBV	45858	75279	1.81%	0.700%
16	14.351	4266	4280	4291	rBV6	29606	62599	1.51%	0.582%
17	14.882	4433	4445	4455	rBV3	26597	52631	1.27%	0.489%
18	15.065	4492	4502	4514	rBV2	92761	149642	3.60%	1.391%
19	16.065	4804	4813	4820	rBV3	26585	44441	1.07%	0.413%


Sum of corrected areas: 10760477

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061418\
Data File : VU024548.D
Acq On : 14 Jun 2018 18:26
Operator : MD/SY
Sample : J3451-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VB-25830-SLUDGEBOX

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

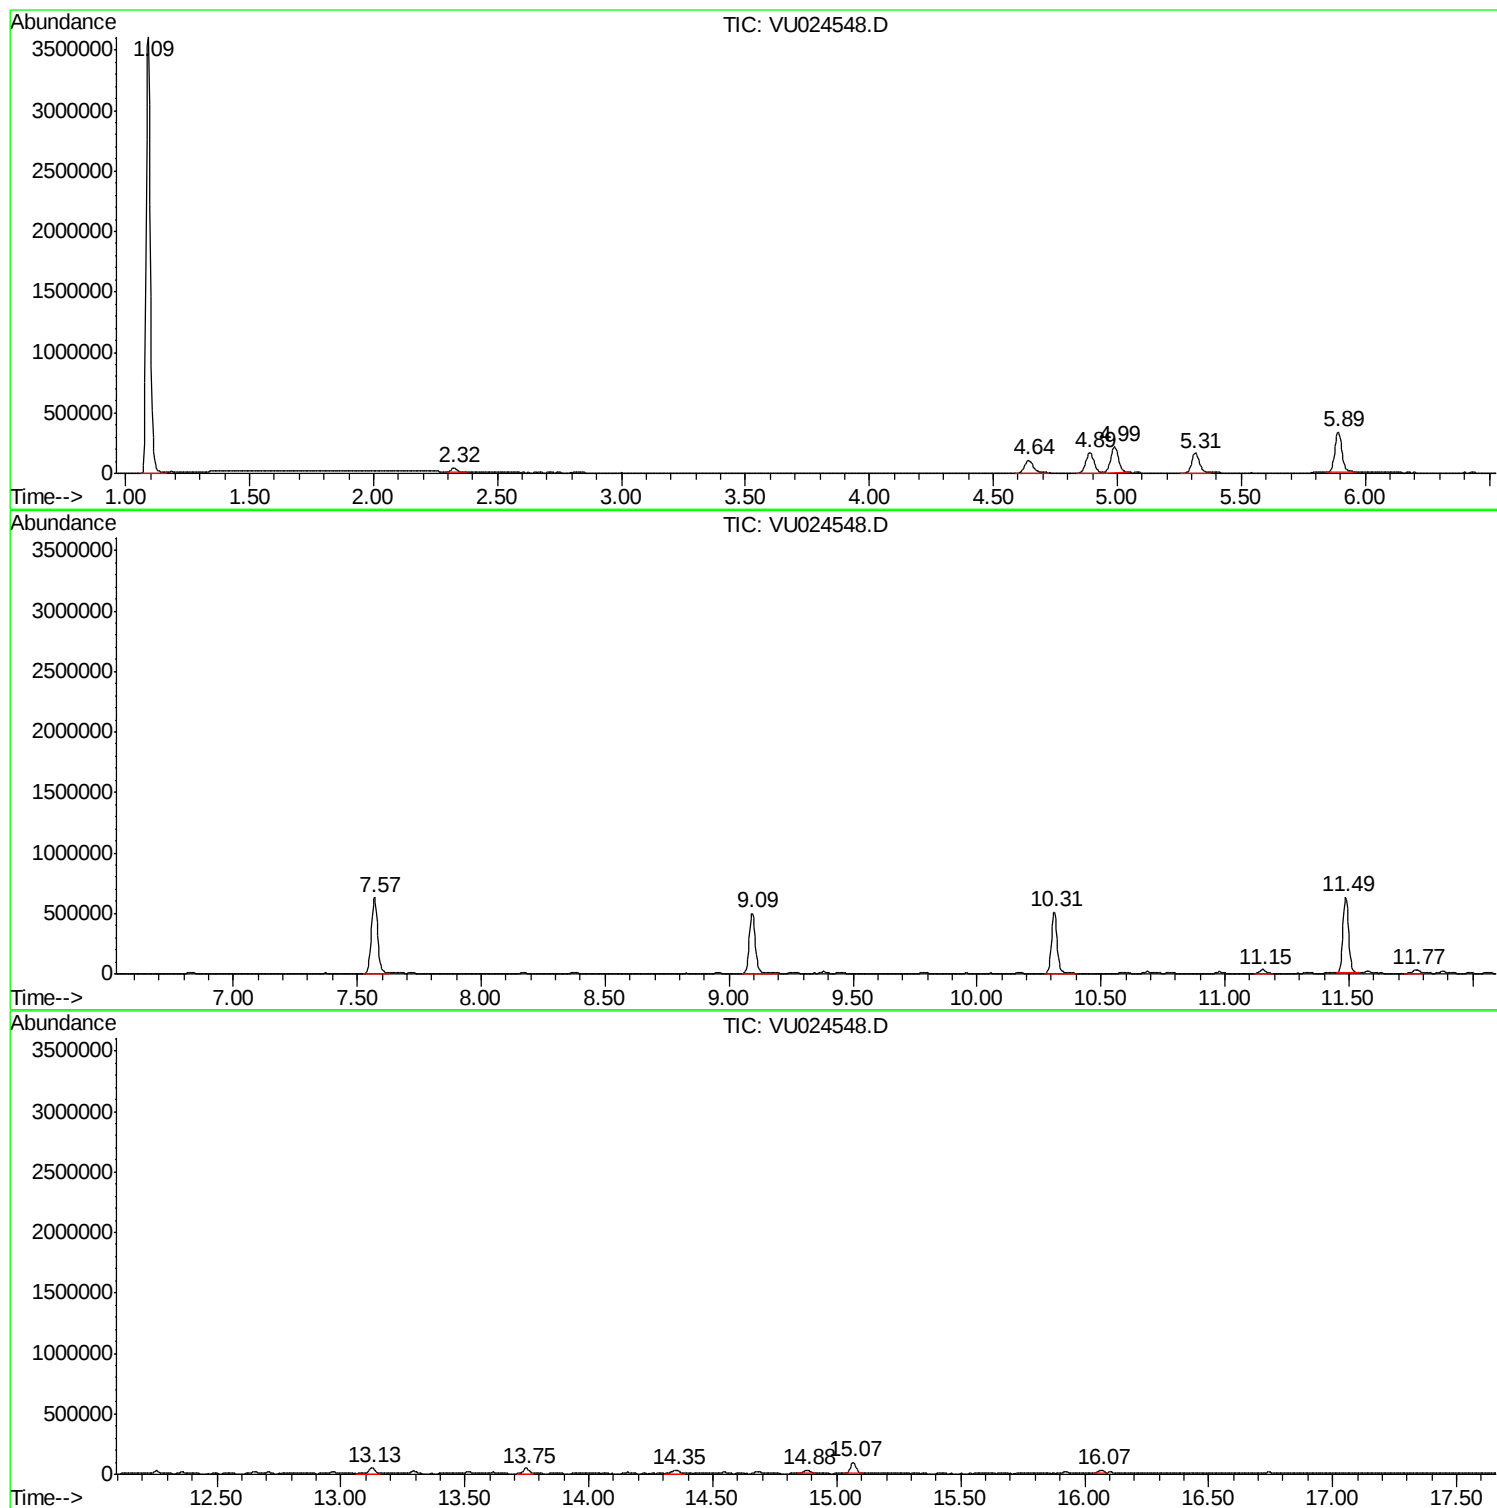

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061418\
Data File : VU024548.D
Acq On : 14 Jun 2018 18:26
Operator : MD/SY
Sample : J3451-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VB-25830-SLUDGEBOX

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Naphthalene, 1-methyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.07	7.40 ug/l	149642	1,4-Dichlorobenzene-d4	11.49

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Naphthalene, 2-methyl-	142	C11H10	000091-57-6	96
2			Naphthalene, 1-methyl-	142	C11H10	000090-12-0	96
3			1,4-Methanonaphthalene, 1,4-dihy...	142	C11H10	004453-90-1	94
4			Benzocycloheptatriene	142	C11H10	000264-09-5	91
5			1H-Indene, 1-ethylidene-	142	C11H10	002471-83-2	64

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061418\
Data File : VU024548.D
Acq On : 14 Jun 2018 18:26
Operator : MD/SY
Sample : J3451-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VB-25830-SLUDGEBOX

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Naphthalene, 1-me...	15.07	7.4	ug/l	149642	4	11.49	1011550	50.0