


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU061418\
Data File : VU024525.D
Acq On : 14 Jun 2018 09:20
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Title : SW846 8260
Last Update : Wed Jun 13 13:55:26 2018

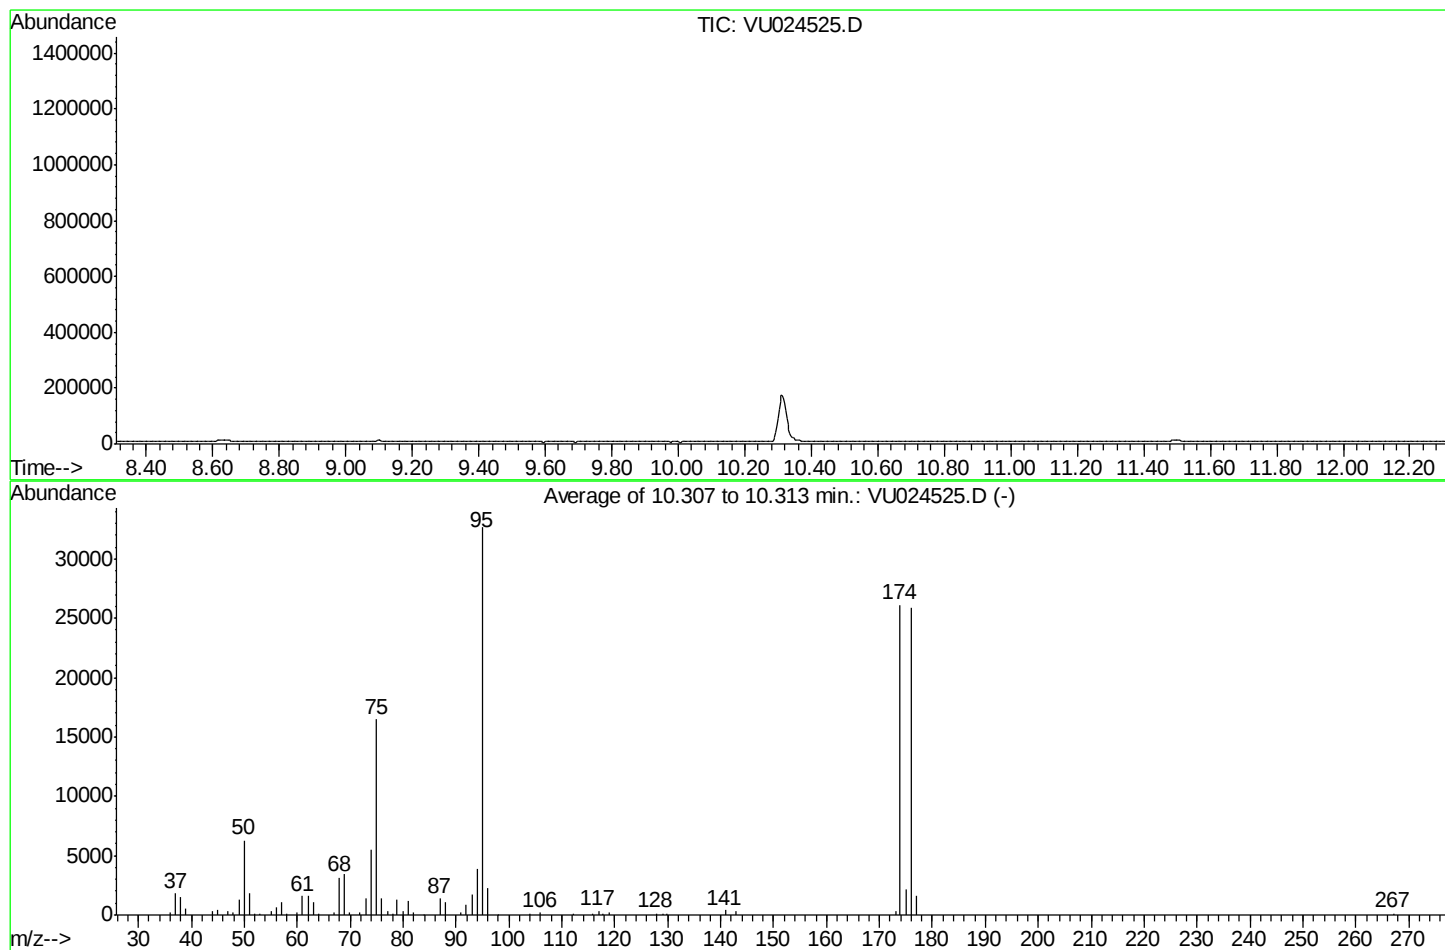

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3009

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	6304	PASS
75	95	30	60	50.5	16501	PASS
95	95	100	100	100.0	32663	PASS
96	95	5	9	6.9	2242	PASS
173	174	0.00	2	1.4	354	PASS
174	95	50	100	79.9	26114	PASS
175	174	5	9	8.2	2145	PASS
176	174	95	101	99.1	25882	PASS
177	176	5	9	6.5	1674	PASS