


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU061418\
Data File : VU024556.D
Acq On : 14 Jun 2018 21:54
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Title : SW846 8260
Last Update : Wed Jun 13 13:55:26 2018

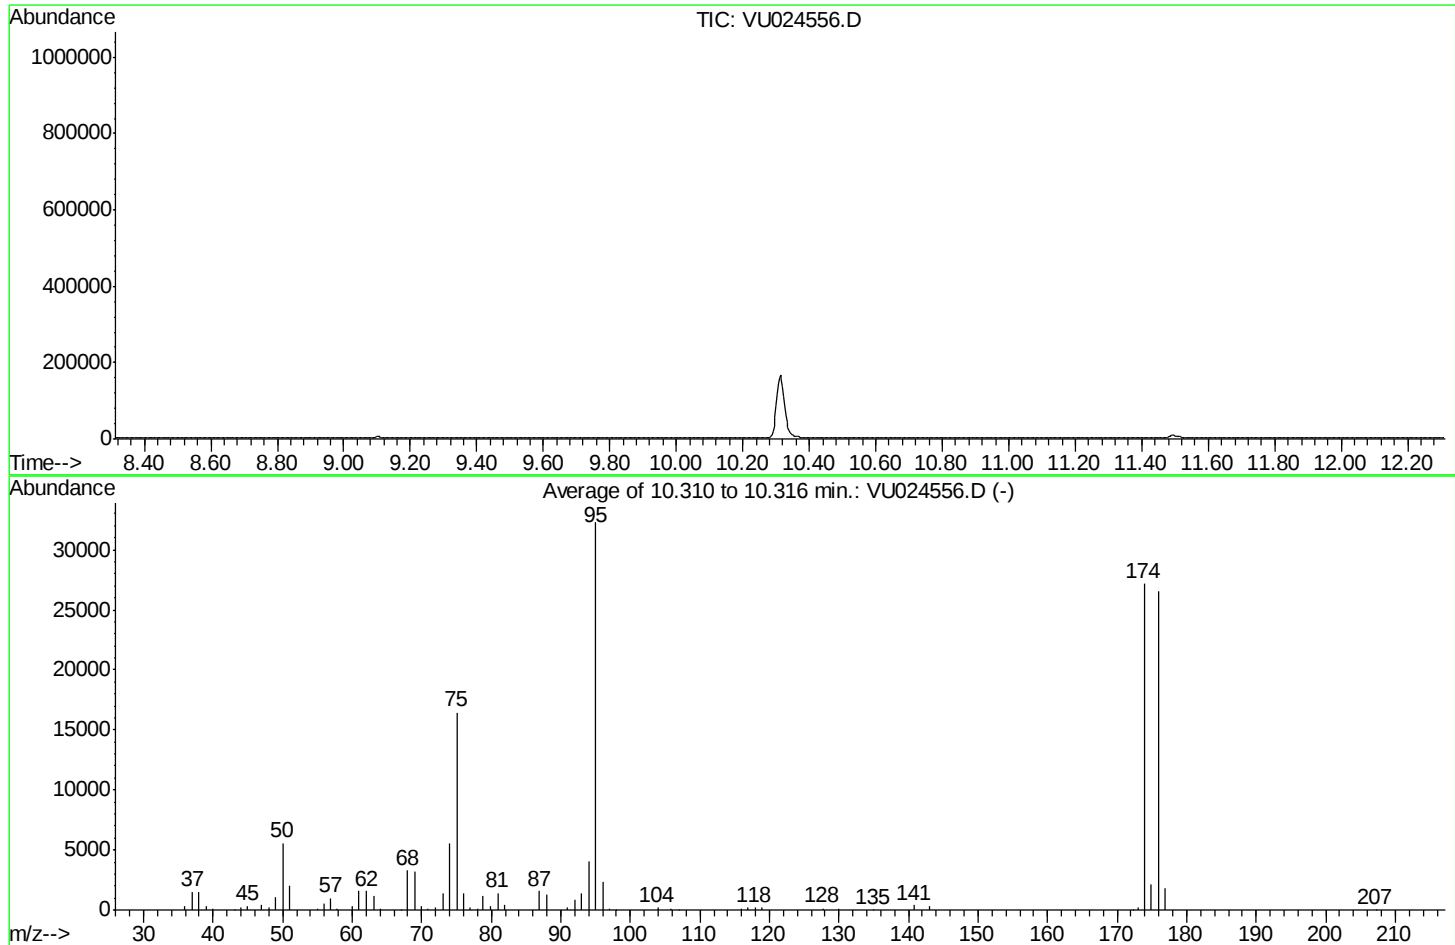

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	5597	PASS
75	95	30	60	51.0	16466	PASS
95	95	100	100	100.0	32288	PASS
96	95	5	9	7.2	2331	PASS
173	174	0.00	2	0.9	232	PASS
174	95	50	100	84.1	27146	PASS
175	174	5	9	8.0	2165	PASS
176	174	95	101	97.9	26581	PASS
177	176	5	9	6.8	1803	PASS