

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061522\
 Data File : VU049159.D
 Acq On : 15 Jun 2022 10:51
 Operator : SY/MD
 Sample : N3288-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGJB3

Quant Time: Jun 16 04:46:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 16 04:45:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	134194	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	123212	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	59262	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	54603	4.657	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.200%
7) Chloroethane-d5	1.912	69	39650	4.995	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.800%
11) 1,1-Dichloroethene-d2	2.568	65	21867	4.636	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	92.800%
20) 2-Butanone-d5	4.639	46	153521	49.035	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.080%
24) Chloroform-d	5.067	84	89336	4.856	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.200%
26) 1,2-Dichloroethane-d4	5.703	65	49645	4.919	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.400%
32) Benzene-d6	5.729	84	183721	4.950	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.000%
36) 1,2-Dichloropropane-d6	6.693	67	62667	4.974	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.400%
41) Toluene-d8	7.899	98	165421	4.949	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.000%
43) trans-1,3-Dichloroprop...	8.182	79	23494	4.198	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.000%
46) 2-Hexanone-d5	8.636	63	99613	44.121	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.240%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	47056	4.665	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.400%
66) 1,2-Dichlorobenzene-d4	12.195	152	59167	5.203	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.000%
Target Compounds						
					Qvalue	
13) Acetone	2.652	43	22677	14.635	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061522\
Data File : VU049159.D
Acq On : 15 Jun 2022 10:51
Operator : SY/MD
Sample : N3288-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGJB3

Quant Time: Jun 16 04:46:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 16 04:45:30 2022
Response via : Initial Calibration

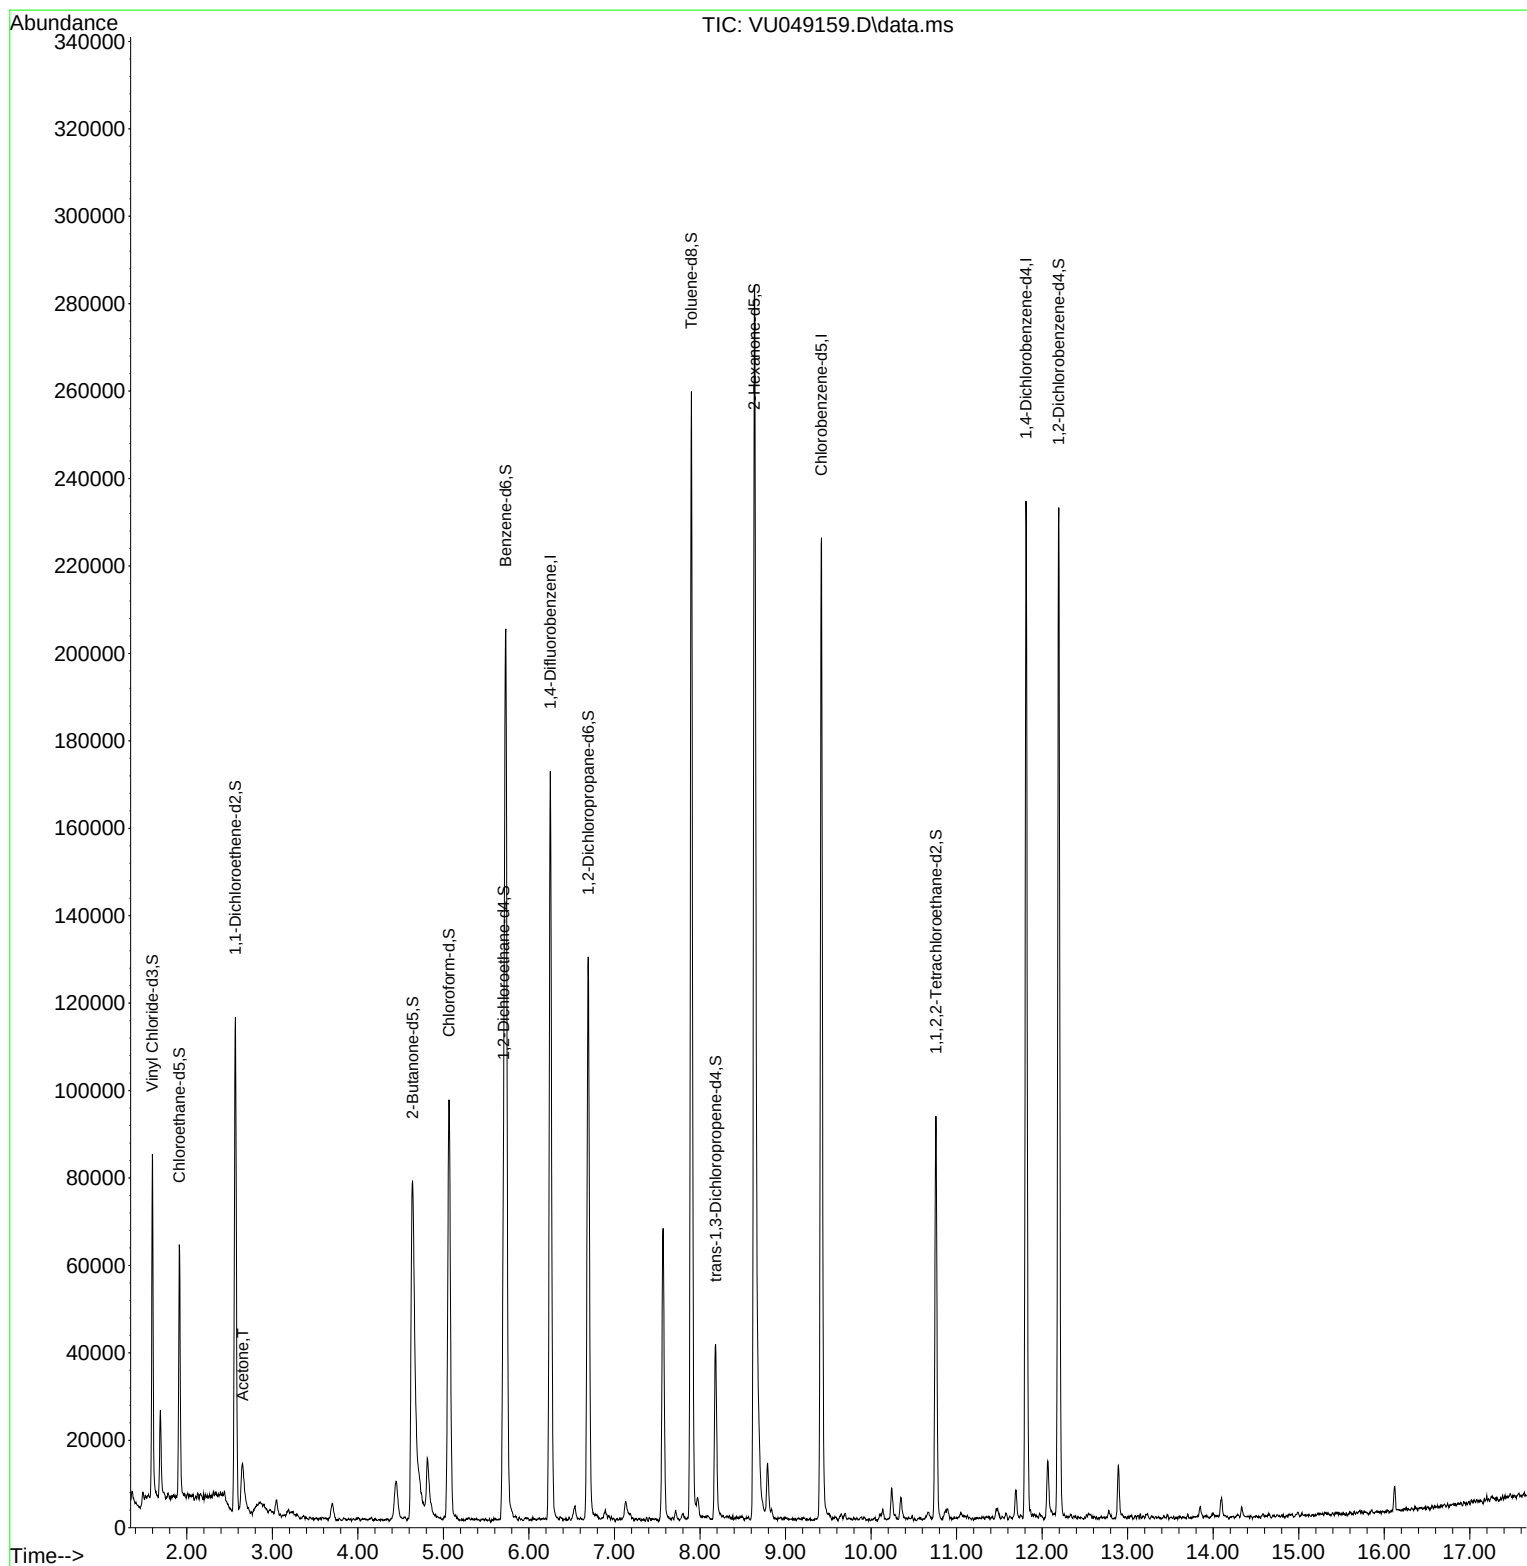

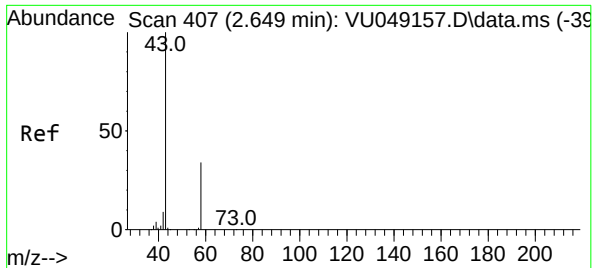

#13
 Acetone
 Concen: 14.635 ug/L
 RT: 2.652 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU049159.D
 Acq: 15 Jun 2022 10:51

Instrument :
 MSVOA_U
 ClientSampleId :
 BGJB3

Tgt Ion: 43 Resp: 22677
 Ion Ratio Lower Upper
 43 100
 58 31.7 0.0 65.8

