

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061522\
 Data File : VU049171.D
 Acq On : 15 Jun 2022 15:35
 Operator : SY/MD
 Sample : VIBLK017
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK017

Quant Time: Jun 16 04:49:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 16 04:45:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	134169	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	123564	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	61599	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	48385	4.127	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.600%
7) Chloroethane-d5	1.912	69	36170	4.557	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.200%
11) 1,1-Dichloroethene-d2	2.565	65	19734	4.185	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.600%
20) 2-Butanone-d5	4.633	46	176716	56.454	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.900%
24) Chloroform-d	5.063	84	89861	4.885	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
26) 1,2-Dichloroethane-d4	5.703	65	50621	5.017	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.400%
32) Benzene-d6	5.729	84	177768	4.776	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
36) 1,2-Dichloropropane-d6	6.690	67	62540	4.950	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.000%
41) Toluene-d8	7.899	98	158792	4.737	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%
43) trans-1,3-Dichloroprop...	8.179	79	24721	4.404	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.000%
46) 2-Hexanone-d5	8.636	63	129700	57.284	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	114.560%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	50840	5.026	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.600%
66) 1,2-Dichlorobenzene-d4	12.195	152	59591	5.041	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.800%
Target Compounds						Qvalue
34) Trichloroethene	6.546	95	2985	0.318	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061522\
Data File : VU049171.D
Acq On : 15 Jun 2022 15:35
Operator : SY/MD
Sample : VIBLK017
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK017

Quant Time: Jun 16 04:49:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 16 04:45:30 2022
Response via : Initial Calibration

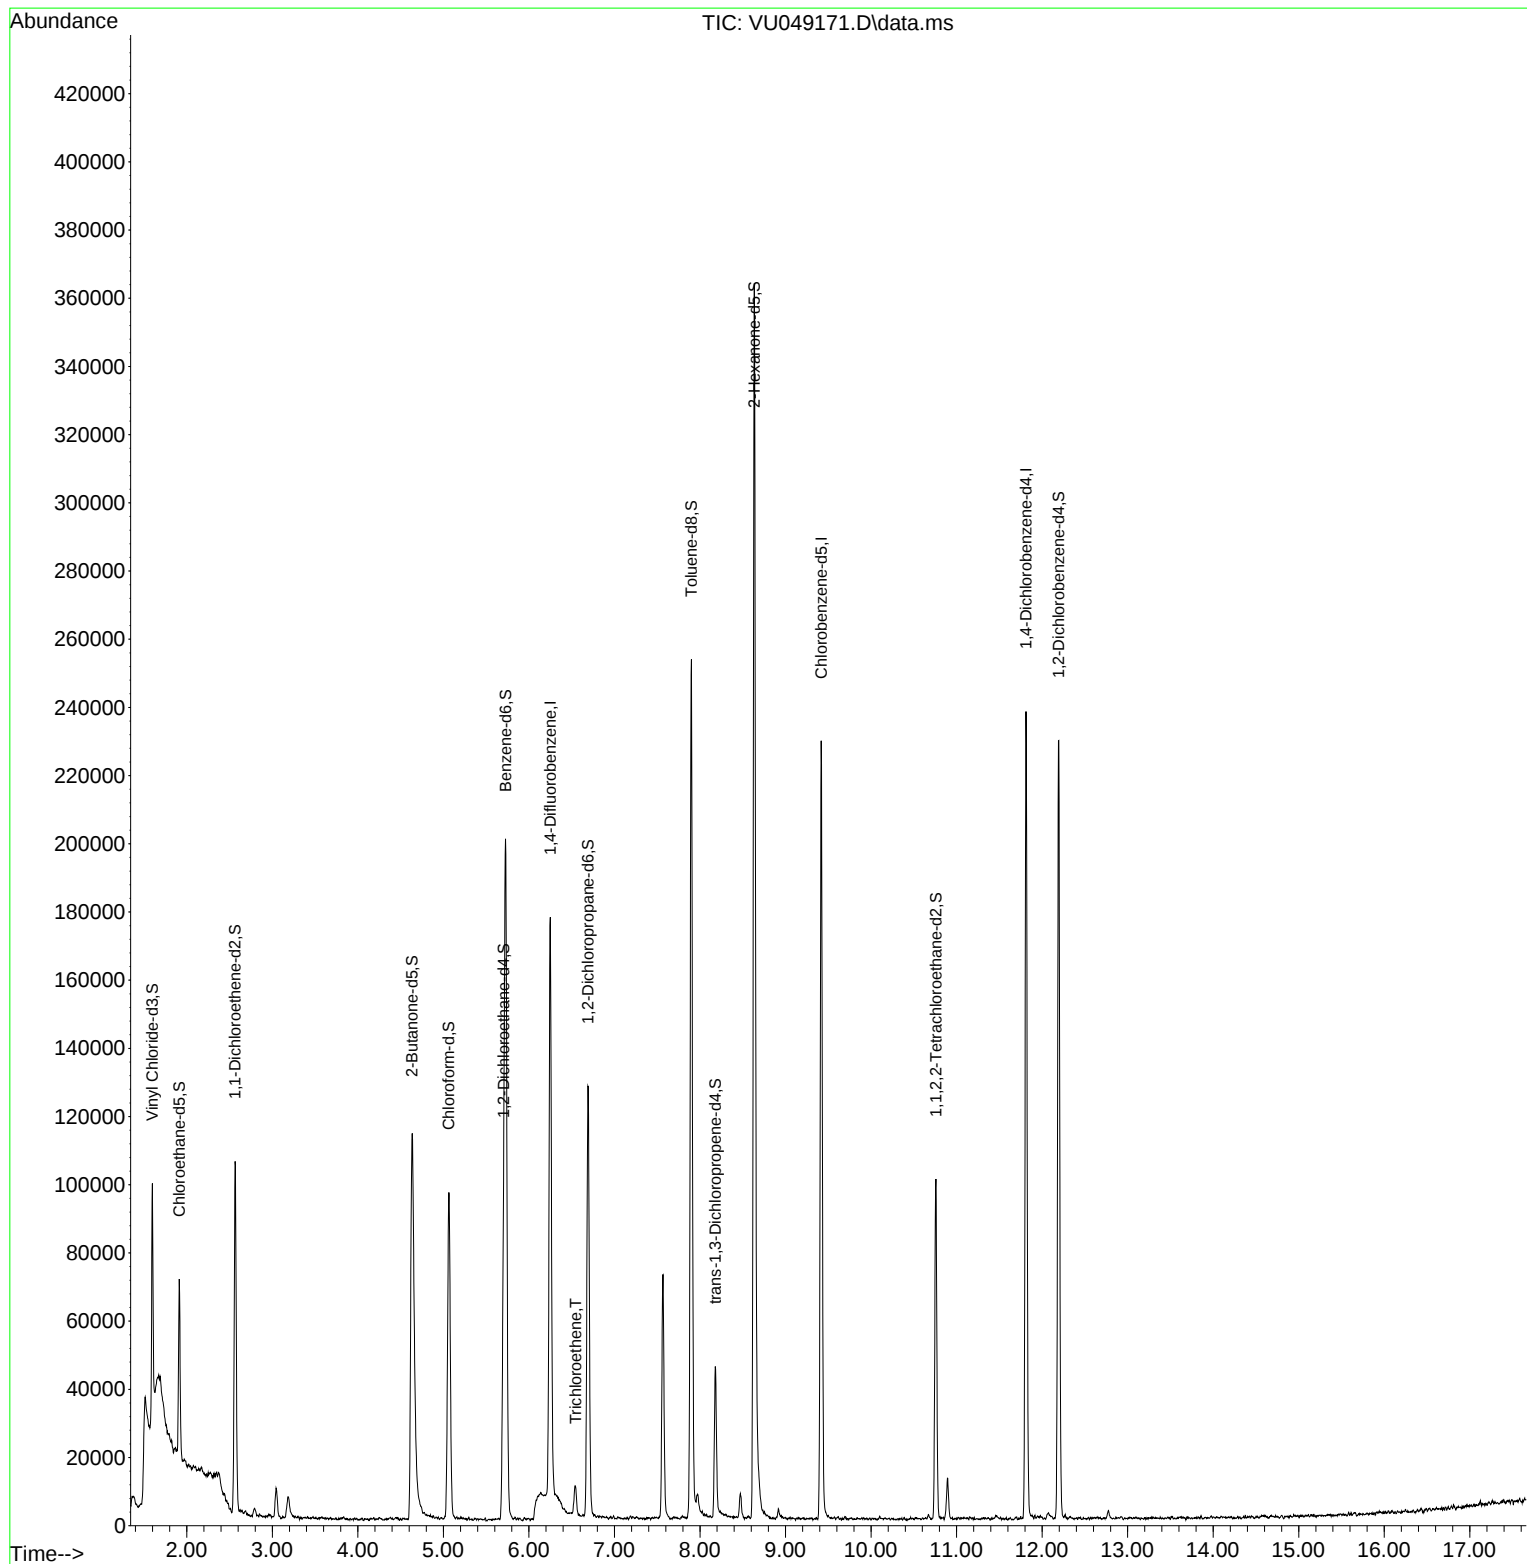

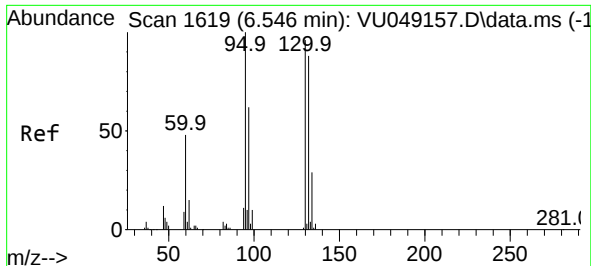

#34
 Trichloroethene
 Concen: 0.318 ug/L
 RT: 6.546 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU049171.D
 Acq: 15 Jun 2022 15:35

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK017

Tgt Ion:	95	Resp:	2985
Ion	Ratio	Lower	Upper
95	100		
97	56.9	45.3	84.1
132	76.9	61.5	114.3
130	86.8	65.6	121.8

