

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061522\
 Data File : VU049158.D
 Acq On : 15 Jun 2022 10:20
 Operator : SY/MD
 Sample : VU0615WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK087

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049158.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rVB	76360	84539	13.55%	1.883%
2	1.916	170	179	189	rBV	57170	71572	11.47%	1.594%
3	2.568	371	382	398	rVB	109136	179395	28.76%	3.997%
4	3.047	522	531	540	rBV4	4349	7576	1.21%	0.169%
5	4.639	1012	1026	1066	rBV	86133	270329	43.34%	6.022%
6	5.066	1143	1159	1181	rBV	96605	212118	34.00%	4.726%
7	5.726	1344	1364	1390	rBV2	198613	522730	83.80%	11.645%
8	6.250	1513	1527	1545	rBV	167696	319686	51.25%	7.122%
9	6.693	1649	1665	1683	rBV	124468	249158	39.94%	5.551%
10	7.568	1924	1937	1955	rBV	69672	126961	20.35%	2.828%
11	7.899	2025	2040	2057	rBV	247949	436246	69.93%	9.719%
12	7.970	2057	2062	2072	rVB6	4898	7444	1.19%	0.166%
13	8.182	2116	2128	2144	rBV	43456	76233	12.22%	1.698%
14	8.635	2257	2269	2302	rBV2	302444	623810	100.00%	13.897%
15	9.417	2500	2512	2532	rBV	221709	379438	60.83%	8.453%
16	10.758	2918	2929	2947	rBV	94464	154126	24.71%	3.434%
17	11.812	3246	3257	3275	rBV	235282	381937	61.23%	8.509%
18	12.192	3362	3375	3394	rBV	223874	366013	58.67%	8.154%
19	13.847	3880	3890	3900	rVB6	4588	6753	1.08%	0.150%
20	14.092	3955	3966	3977	rBV	7461	12636	2.03%	0.282%




Sum of corrected areas: 4488700

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061522\
Data File : VU049158.D
Acq On : 15 Jun 2022 10:20
Operator : SY/MD
Sample : VU0615WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK087

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

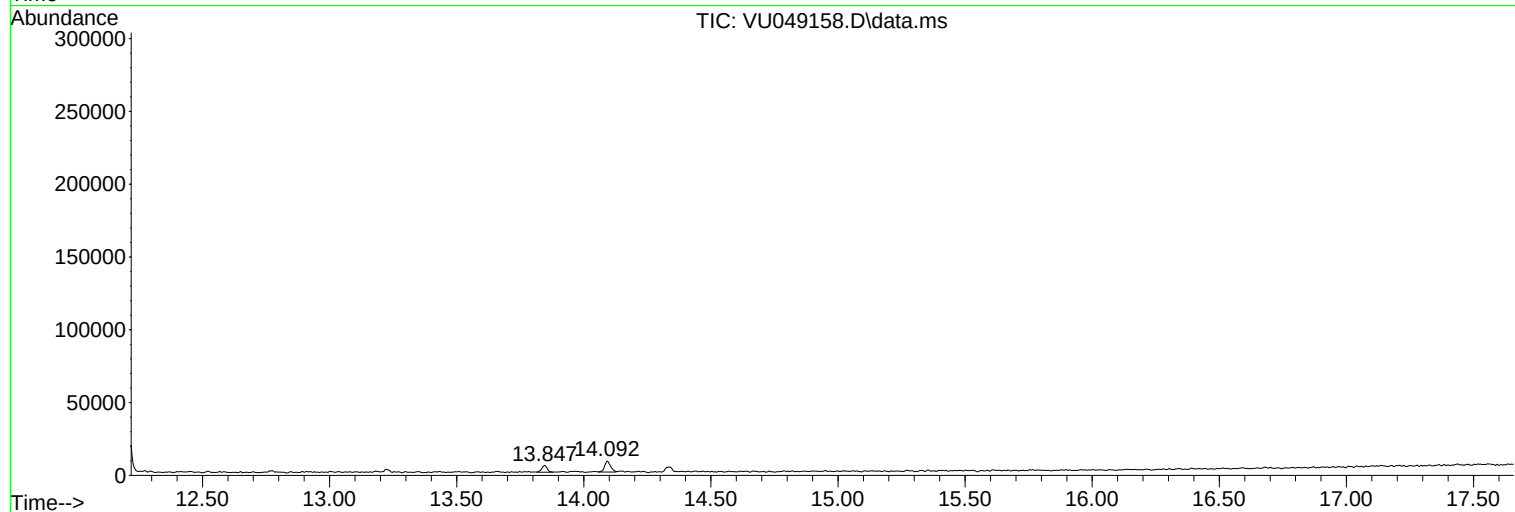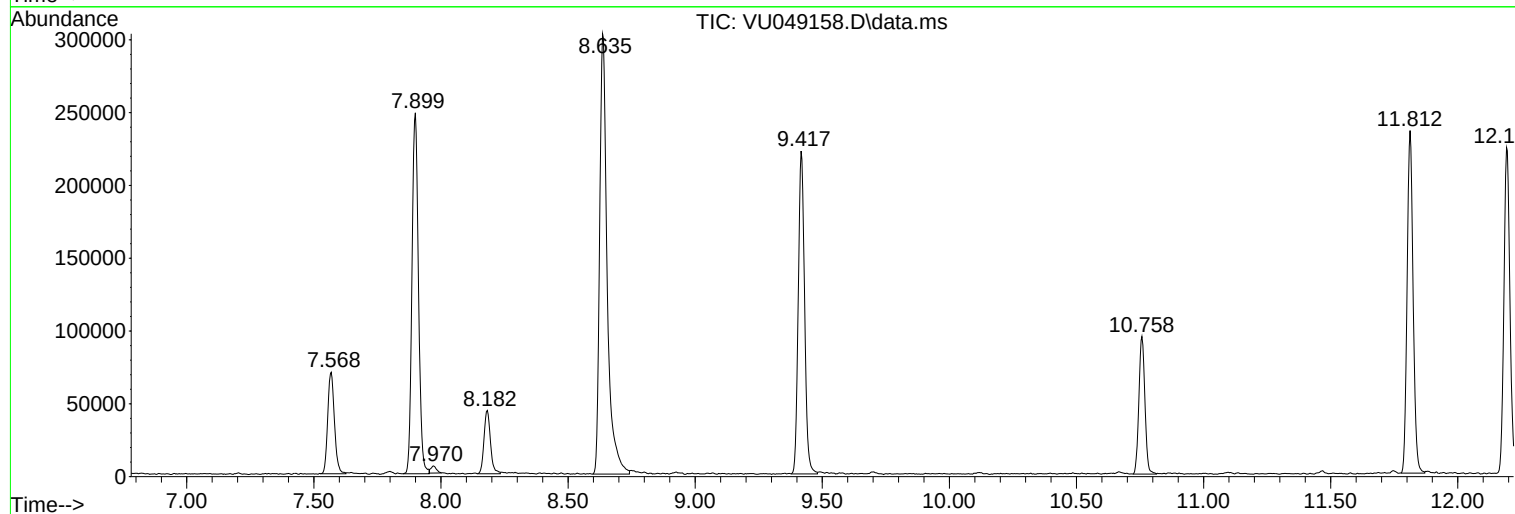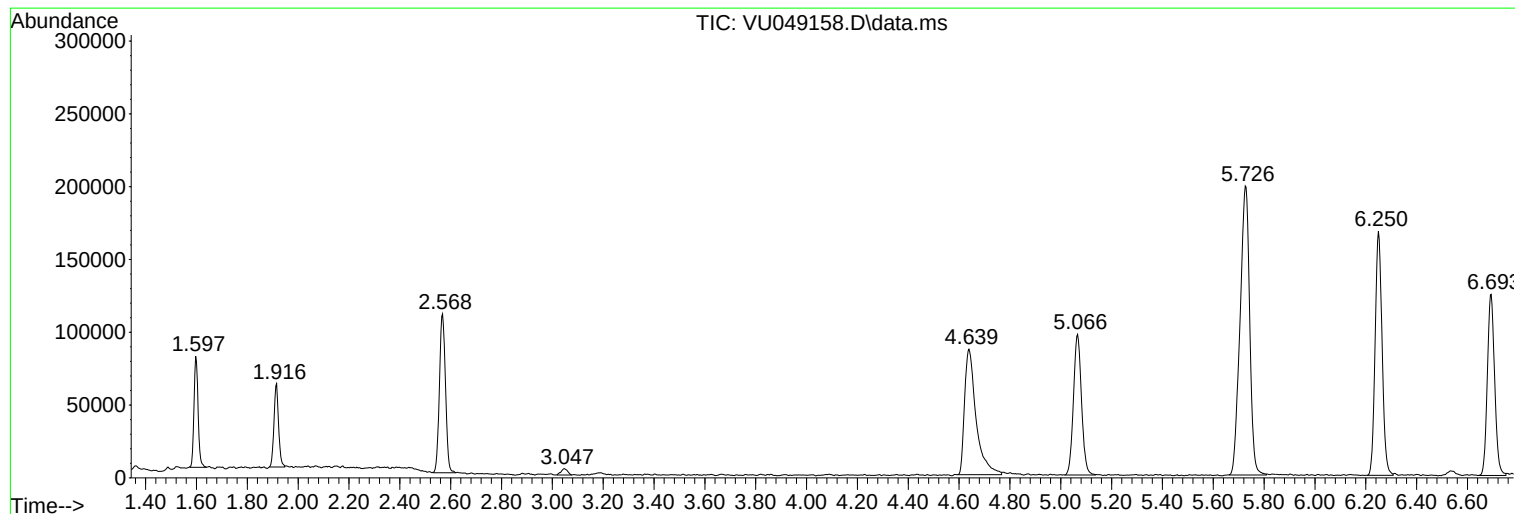

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061522\
Data File : VU049158.D
Acq On : 15 Jun 2022 10:20
Operator : SY/MD
Sample : VU0615WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK087

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061522\
Data File : VU049158.D
Acq On : 15 Jun 2022 10:20
Operator : SY/MD
Sample : VU0615WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK087

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc