
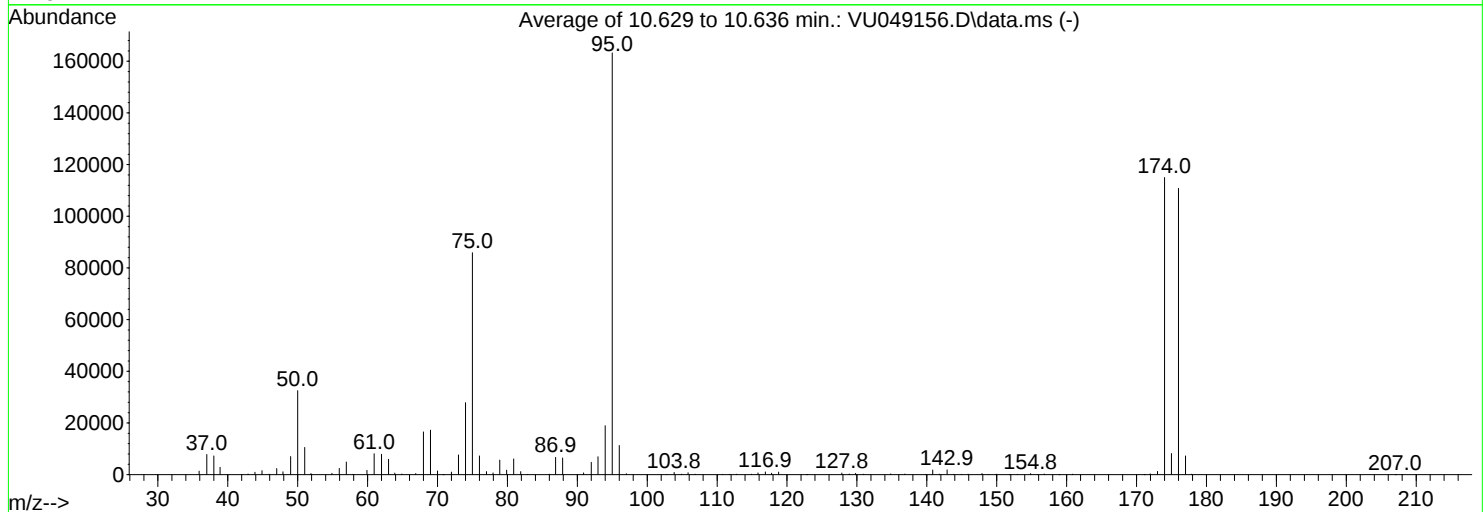


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061522\
Data File : VU049156.D
Acq On : 15 Jun 2022 08:53
Operator : SY/MD
Sample : BFB083
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB083

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Jun 18 05:20:12 2022

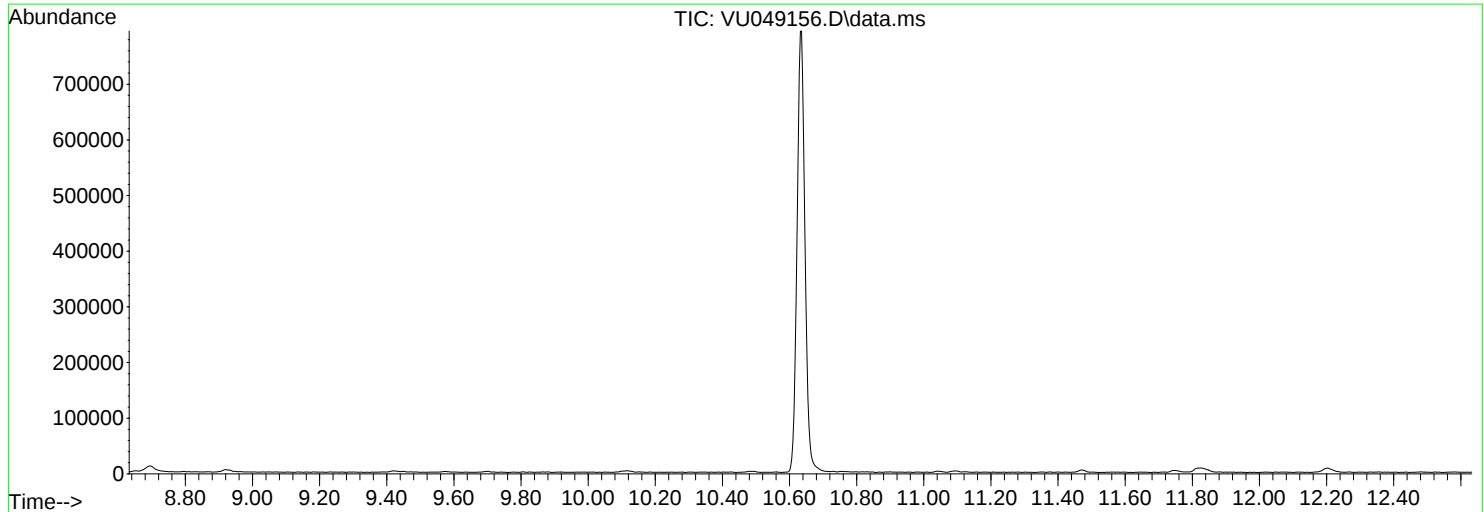

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	32504	PASS
75	95	30	80	52.6	85880	PASS
95	95	100	100	100.0	163264	PASS
96	95	5	9	6.9	11263	PASS
173	174	0.00	2	1.1	1239	PASS
174	95	50	120	70.5	115029	PASS
175	174	5	9	7.1	8177	PASS
176	174	95	101	96.3	110781	PASS
177	176	5	9	6.6	7279	PASS

m/z	Abundance
39.90	1468.0
43.90	745.0
207.00	630.0
207.90	120.0
281.10	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

m/z	Abundance
35.90	1301.0
37.00	7553.0
38.00	6786.0
38.90	2762.0
39.90	1354.0
42.90	176.0
43.90	1673.0
44.90	1438.0
45.90	149.0
47.00	2204.0
47.90	981.0
49.00	6815.0
50.00	31096.0
51.00	10091.0
51.90	417.0
54.90	534.0
55.90	2362.0
57.00	4682.0
57.90	170.0
59.90	1611.0
61.00	7688.0
62.00	7235.0
63.00	5639.0
63.90	530.0
64.90	221.0
66.90	394.0
68.00	15797.0
69.00	16287.0
70.00	1310.0
72.00	867.0
73.00	7053.0
74.00	26792.0
75.00	81120.0
76.00	7043.0
77.00	1124.0
77.90	600.0
78.90	5345.0
79.90	1571.0
80.90	5732.0
81.90	1082.0
82.90	162.0
86.10	202.0
86.90	6527.0
87.90	6097.0
90.90	624.0
92.00	4517.0
92.90	6414.0
94.00	17712.0
95.00	153600.0
96.00	10610.0
97.00	334.0
102.80	124.0
103.90	879.0
104.90	219.0
105.80	671.0
106.80	154.0
110.80	113.0
111.80	134.0
112.80	171.0
114.90	172.0
115.80	612.0
116.90	1025.0
117.80	550.0
118.80	909.0
127.90	582.0
128.90	227.0
129.80	419.0
130.90	211.0
134.90	283.0
136.90	279.0
139.80	107.0
140.80	1681.0
141.80	155.0
142.90	1816.0
143.90	114.0
145.00	113.0
145.90	214.0
147.90	378.0
149.90	162.0
152.90	130.0
154.90	436.0
156.80	276.0
158.90	117.0
160.90	198.0
171.90	283.0
173.00	1097.0
174.00	105320.0
175.00	7790.0
176.00	101688.0
177.00	6864.0
177.90	190.0
207.00	686.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

208.10

135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

m/z	Abundance
35.90	1406.0
37.00	7965.0
38.00	7525.0
38.90	2945.0
39.90	1348.0
42.90	236.0
43.90	1769.0
44.90	1596.0
45.90	172.0
47.00	2490.0
47.90	1115.0
49.00	7314.0
50.00	33624.0
51.00	10947.0
51.90	465.0
54.90	539.0
56.00	2493.0
56.90	5039.0
57.90	148.0
59.90	1766.0
60.90	8400.0
62.00	8119.0
63.00	6188.0
63.90	631.0
64.90	251.0
66.90	427.0
68.00	17048.0
69.00	17816.0
70.00	1531.0
72.00	1067.0
73.00	7816.0
74.00	28592.0
75.00	88496.0
76.00	7452.0
77.00	1209.0
78.00	707.0
78.90	5856.0
79.90	1813.0
80.90	6328.0
81.90	1243.0
82.90	160.0
86.00	229.0
86.90	6877.0
87.90	6666.0
90.90	685.0
92.00	4908.0
92.90	7074.0
94.00	19568.0
95.00	168448.0
96.00	11673.0
97.00	422.0
102.80	160.0
103.90	871.0
104.90	220.0
105.90	773.0
106.80	173.0
110.80	167.0
111.80	156.0
112.80	166.0
114.90	210.0
115.90	700.0
116.90	1106.0
117.80	580.0
118.80	1022.0
122.80	105.0
127.90	644.0
128.90	262.0
129.80	500.0
130.90	211.0
134.90	359.0
136.80	280.0
139.80	106.0
140.90	1841.0
141.80	160.0
142.90	1887.0
143.80	129.0
145.00	134.0
145.90	220.0
147.90	450.0
148.90	115.0
149.90	181.0
152.90	148.0
154.80	437.0
155.80	110.0
156.80	282.0
160.80	219.0
172.00	309.0
173.00	1287.0
174.00	118488.0
175.00	8383.0
176.00	114208.0
177.00	7482.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

177.90	203.0
207.00	674.0
208.00	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

m/z	Abundance
35.90	1433.0
37.00	7830.0
38.00	7451.0
38.90	2932.0
39.90	1356.0
42.90	259.0
43.90	1694.0
44.90	1621.0
45.90	181.0
47.00	2466.0
47.90	1197.0
49.00	6953.0
50.00	32792.0
51.00	10611.0
51.90	460.0
54.90	501.0
56.00	2464.0
57.00	4878.0
57.90	151.0
59.90	1729.0
60.90	8332.0
62.00	8339.0
63.00	6027.0
63.90	636.0
64.90	259.0
66.90	434.0
68.00	16728.0
69.00	17552.0
70.00	1525.0
70.80	104.0
72.00	1054.0
73.00	7940.0
74.00	28248.0
75.00	88024.0
76.00	7304.0
77.00	1196.0
77.90	733.0
78.90	5677.0
79.90	1808.0
80.90	6221.0
81.90	1275.0
82.90	149.0
85.90	231.0
86.90	6716.0
87.90	6617.0
90.90	712.0
92.00	4810.0
93.00	7249.0
94.00	19664.0
95.00	167744.0
96.00	11507.0
97.00	424.0
102.80	144.0
103.80	783.0
104.90	223.0
105.80	812.0
106.90	214.0
110.80	194.0
111.80	137.0
112.80	143.0
114.90	212.0
115.90	672.0
116.90	1075.0
117.80	591.0
118.80	1044.0
127.80	611.0
128.90	277.0
129.80	537.0
130.90	207.0
134.80	386.0
136.80	267.0
140.90	1785.0
141.80	183.0
142.90	1881.0
143.80	175.0
144.90	152.0
145.90	191.0
147.90	440.0
148.80	140.0
149.90	166.0
151.80	105.0
153.00	135.0
154.80	424.0
155.80	141.0
156.80	302.0
160.80	218.0
171.10	118.0
172.00	355.0
173.00	1333.0
174.00	121280.0
175.00	8359.0
176.00	116448.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

177.00	7491.0
177.90	184.0
207.00	630.0
208.00	125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083