




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
Data File : VU059287.D
Acq On : 17 Jun 2024 18:02
Operator : MD/SY
Sample : P2898-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GC3

Manual IntegrationsAPPROVED

Quant Time: Jun 18 04:22:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 17 12:07:46 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/19/2024
Supervised By :Semsettin Yesilyurt 06/19/2024

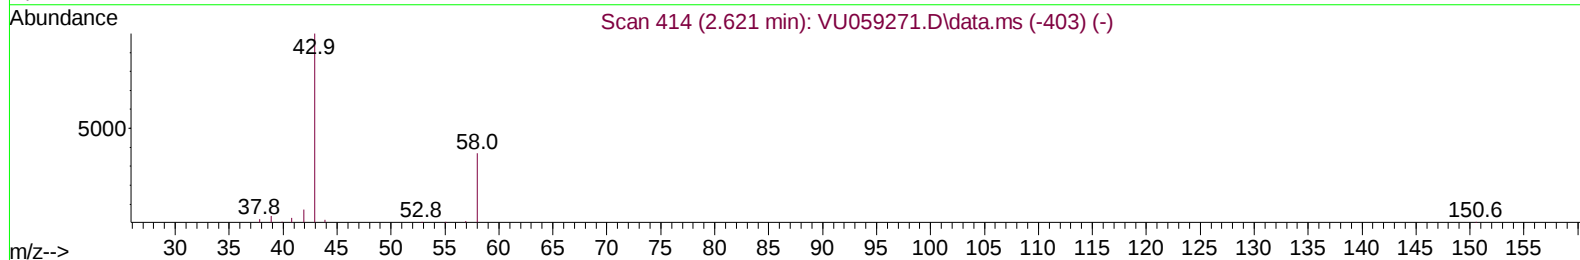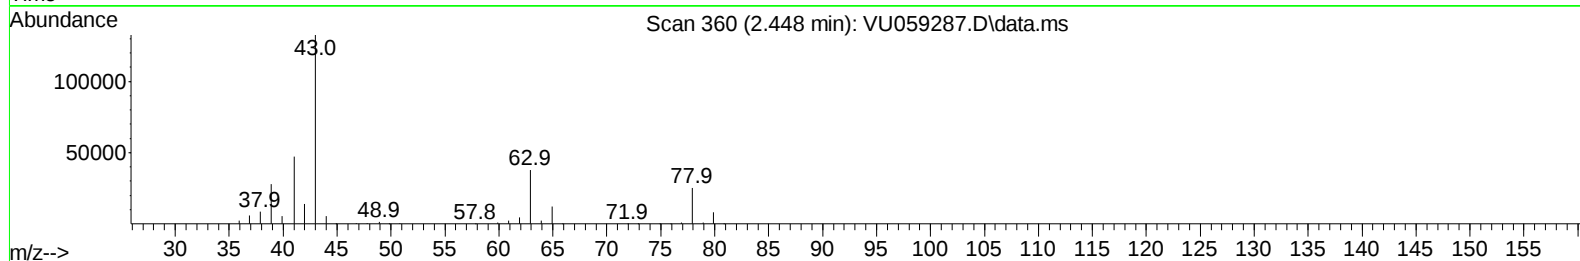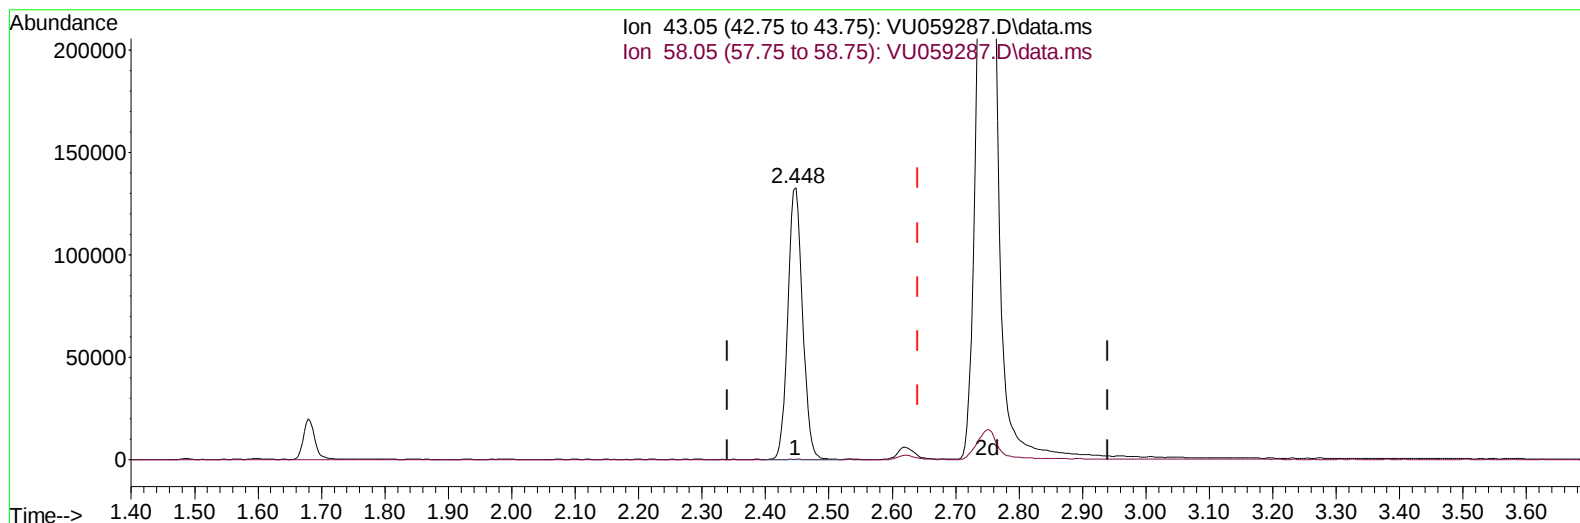

TIC: VU059287.D\data.ms

(13) Acetone (T)

2.448min (-0.193) 220.67 ug/L

response 213596

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	1.80
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
Data File : VU059287.D
Acq On : 17 Jun 2024 18:02
Operator : MD/SY
Sample : P2898-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GC3

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/19/2024
Supervised By :Semsettin Yesilyurt 06/19/2024

Quant Time: Jun 18 04:22:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 17 12:07:46 2024
Response via : Initial Calibration

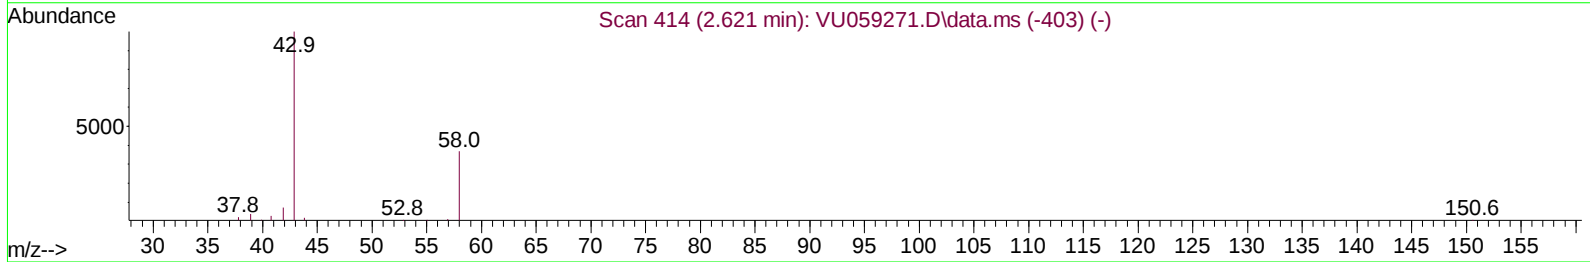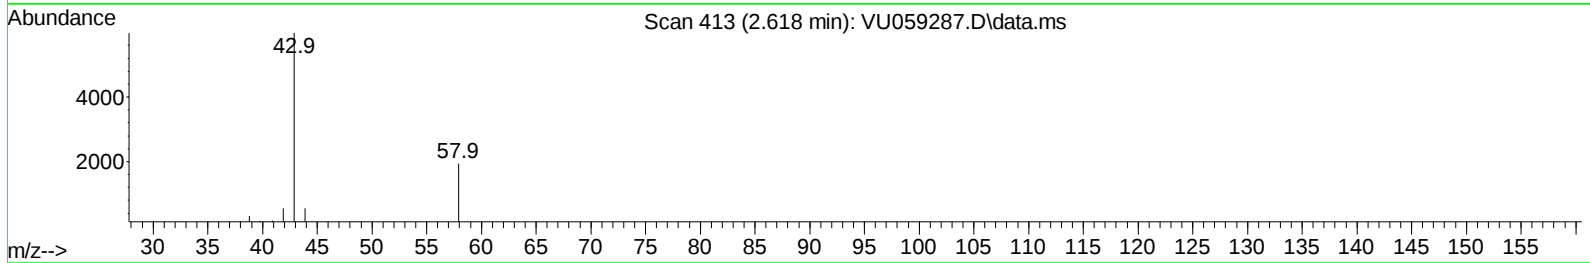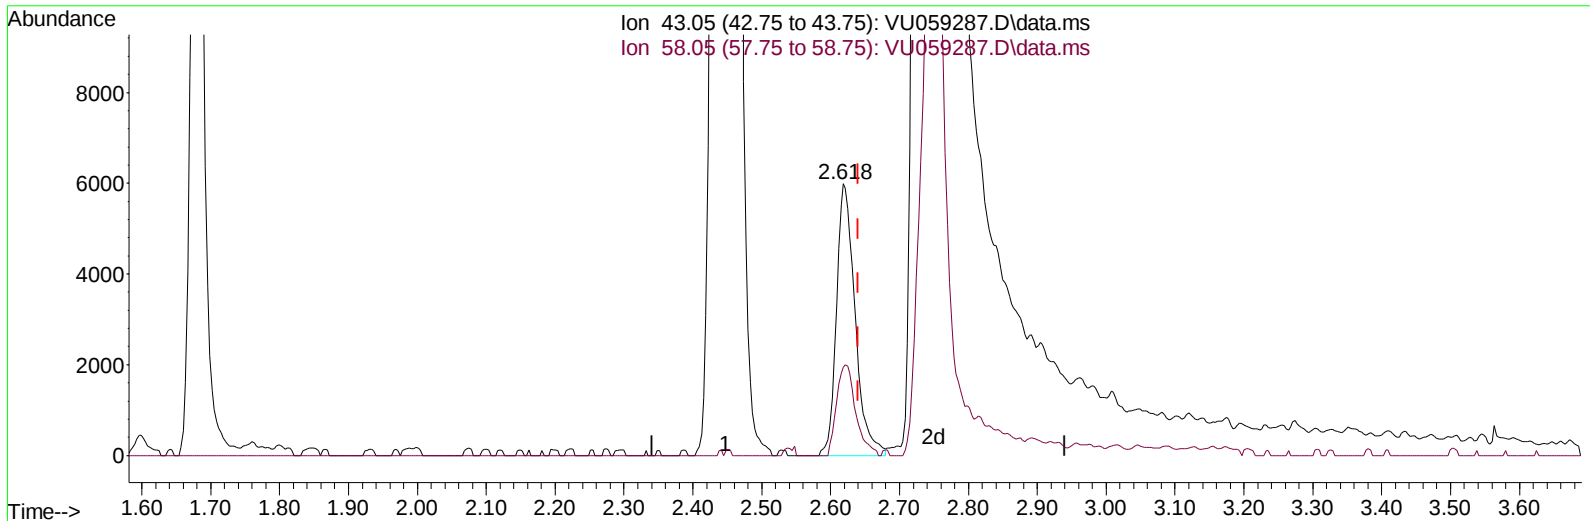

TIC: VU059287.D\data.ms

(13) Acetone (T)

2.618min (-0.022) 11.65 ug/L m

response 11272

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	34.19
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
 Data File : VU059287.D
 Acq On : 17 Jun 2024 18:02
 Operator : MD/SY
 Sample : P2898-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GC3

Manual IntegrationsAPPROVED

Quant Time: Jun 18 04:22:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 17 12:07:46 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/19/2024
 Supervised By :Semsettin Yesilyurt 06/19/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		104176	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117		109597	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152		49010	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		33534	4.629	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.600%	
7) Chloroethane-d5	1.908	69		33814	4.851	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.000%	
11) 1,1-Dichloroethene-d2	2.560	65		13562	4.513	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.200%	
20) 2-Butanone-d5	4.615	46		88650	59.411	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.820%	
24) Chloroform-d	5.059	84		71979	4.841	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.800%	
26) 1,2-Dichloroethane-d4	5.695	65		37577	5.247	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.000%	
32) Benzene-d6	5.721	84		138708	4.599	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.000%	
36) 1,2-Dichloropropane-d6	6.686	67		46155	4.994	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.800%	
41) Toluene-d8	7.895	98		112500	4.012	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.200%	
43) trans-1,3-Dichloroprop...	8.177	79		13462	4.651	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.000%	
46) 2-Hexanone-d5	8.628	63		63350	52.680	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.360%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84		39409	5.161	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.200%	
66) 1,2-Dichlorobenzene-d4	12.190	152		44268	5.075	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.400%	
Target Compounds							
13) Acetone	2.618	43		11272m	11.645	ug/L	
16) Methylene chloride	3.036	84		3311	0.378	ug/L	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
Data File : VU059287.D
Acq On : 17 Jun 2024 18:02
Operator : MD/SY
Sample : P2898-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GC3

Manual IntegrationsAPPROVED

Quant Time: Jun 18 04:22:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 17 12:07:46 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/19/2024
Supervised By :Semsettin Yesilyurt 06/19/2024

