




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
Data File : VU059289.D
Acq On : 17 Jun 2024 18:50
Operator : MD/SY
Sample : P2898-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GD7

Manual IntegrationsAPPROVED

Quant Time: Jun 18 04:23:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 17 12:07:46 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/19/2024
Supervised By :Semsettin Yesilyurt 06/19/2024

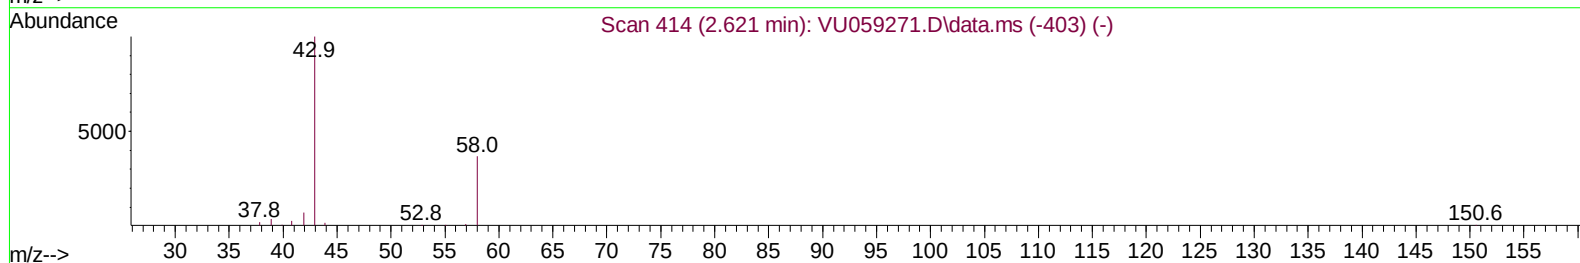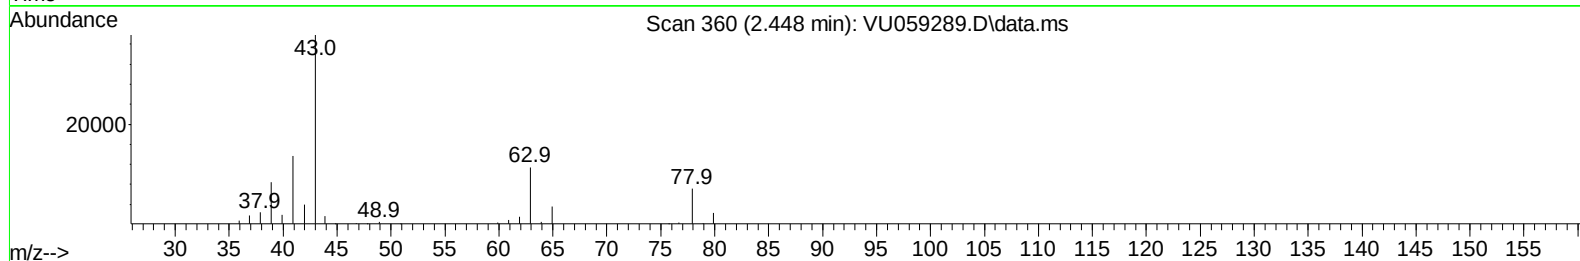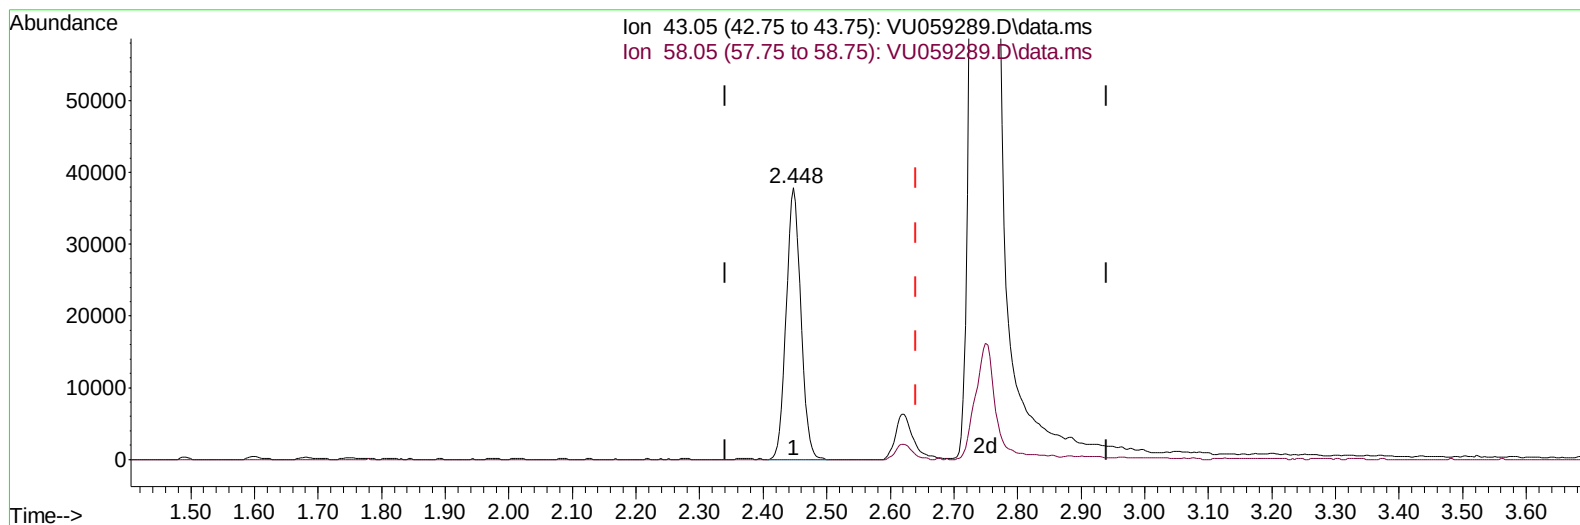

TIC: VU059289.D\data.ms

(13) Acetone (T)

2.448min (-0.193) 63.34 ug/L

response 60764

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	6.44
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
Data File : VU059289.D
Acq On : 17 Jun 2024 18:50
Operator : MD/SY
Sample : P2898-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GD7

Manual IntegrationsAPPROVED

Quant Time: Jun 18 04:23:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 17 12:07:46 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/19/2024
Supervised By :Semsettin Yesilyurt 06/19/2024

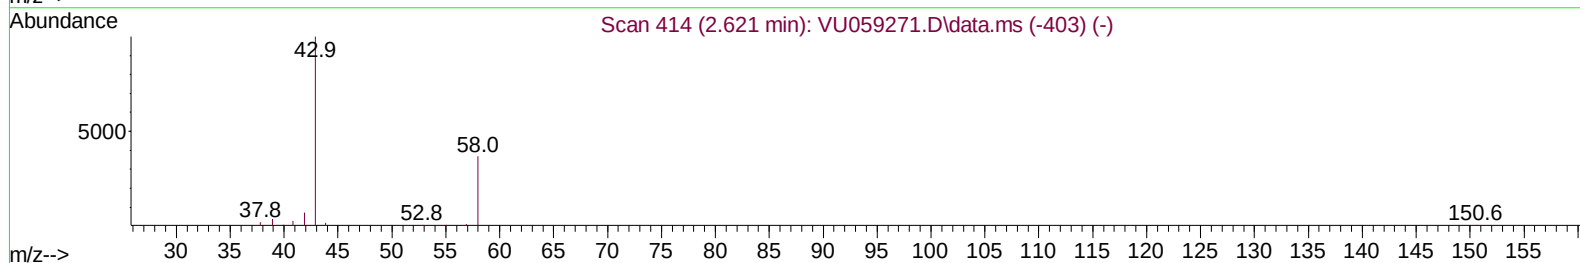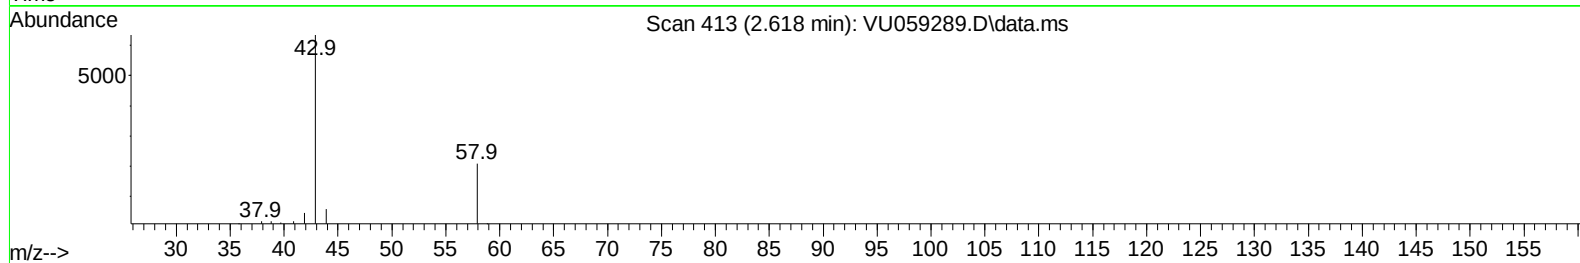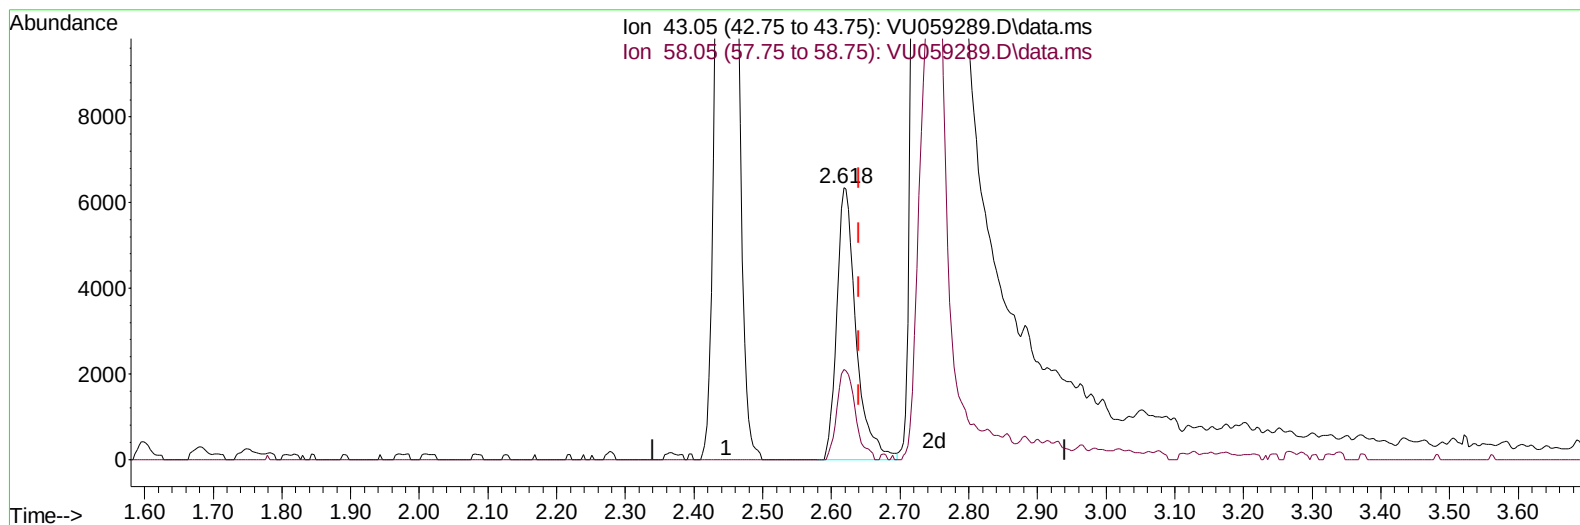

TIC: VU059289.D\data.ms

(13) Acetone (T)

2.618min (-0.022) 12.88 ug/L m

response 12356

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	31.69
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
 Data File : VU059289.D
 Acq On : 17 Jun 2024 18:50
 Operator : MD/SY
 Sample : P2898-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GD7

Manual IntegrationsAPPROVED

Quant Time: Jun 18 04:23:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 17 12:07:46 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/19/2024
 Supervised By :Semsettin Yesilyurt 06/19/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		103244	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117		107073	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152		46138	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		31632	4.406	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	88.200%	
7) Chloroethane-d5	1.907	69		33593	4.863	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	97.200%	
11) 1,1-Dichloroethene-d2	2.560	65		13424	4.507	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	90.200%	
20) 2-Butanone-d5	4.612	46		87702	59.307	ug/L	-0.02
Spiked Amount 50.000	Range 40	- 130		Recovery	=	118.620%	
24) Chloroform-d	5.055	84		69883	4.742	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	94.800%	
26) 1,2-Dichloroethane-d4	5.698	65		36570	5.152	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	103.000%	
32) Benzene-d6	5.721	84		134952	4.580	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	91.600%	
36) 1,2-Dichloropropane-d6	6.685	67		45271	5.014	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	100.200%	
41) Toluene-d8	7.894	98		109763	4.007	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	80.200%	
43) trans-1,3-Dichloroprop...	8.181	79		12834	4.539	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	90.800%	
46) 2-Hexanone-d5	8.627	63		61518	52.363	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	104.720%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84		37817	5.069	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	101.400%	
66) 1,2-Dichlorobenzene-d4	12.190	152		42243	5.144	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	102.800%	
Target Compounds							
13) Acetone	2.618	43		12356m	12.881	ug/L	
16) Methylene chloride	3.039	84		2313	0.267	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
Data File : VU059289.D
Acq On : 17 Jun 2024 18:50
Operator : MD/SY
Sample : P2898-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GD7

Manual IntegrationsAPPROVED

Quant Time: Jun 18 04:23:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 17 12:07:46 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/19/2024
Supervised By :Semsettin Yesilyurt 06/19/2024

