

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
 Data File : VU059275.D
 Acq On : 17 Jun 2024 13:03
 Operator : MD/SY
 Sample : VU0617WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK195

Quant Time: Jun 17 14:03:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 17 12:07:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	116017	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	113935	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	49287	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.593	65	39660	4.916	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.400%
7) Chloroethane-d5	1.908	69	38500	4.960	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.200%
11) 1,1-Dichloroethene-d2	2.560	65	16282	4.865	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	97.200%
20) 2-Butanone-d5	4.615	46	91987	55.356	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.720%
24) Chloroform-d	5.055	84	79703	4.813	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.200%
26) 1,2-Dichloroethane-d4	5.695	65	40139	5.032	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.600%
32) Benzene-d6	5.721	84	160942	5.133	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.600%
36) 1,2-Dichloropropane-d6	6.682	67	50692	5.276	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.600%
41) Toluene-d8	7.895	98	134268	4.606	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.200%
43) trans-1,3-Dichloroprop...	8.178	79	15154	5.037	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	100.800%
46) 2-Hexanone-d5	8.628	63	69703	55.756	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.520%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	41517	5.230	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.600%
66) 1,2-Dichlorobenzene-d4	12.190	152	47421	5.406	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.200%
Target Compounds						
16) Methylene chloride	3.039	84	1448	0.149	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
Data File : VU059275.D
Acq On : 17 Jun 2024 13:03
Operator : MD/SY
Sample : VU0617WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK195


Quant Time: Jun 17 14:03:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 17 12:07:46 2024
Response via : Initial Calibration

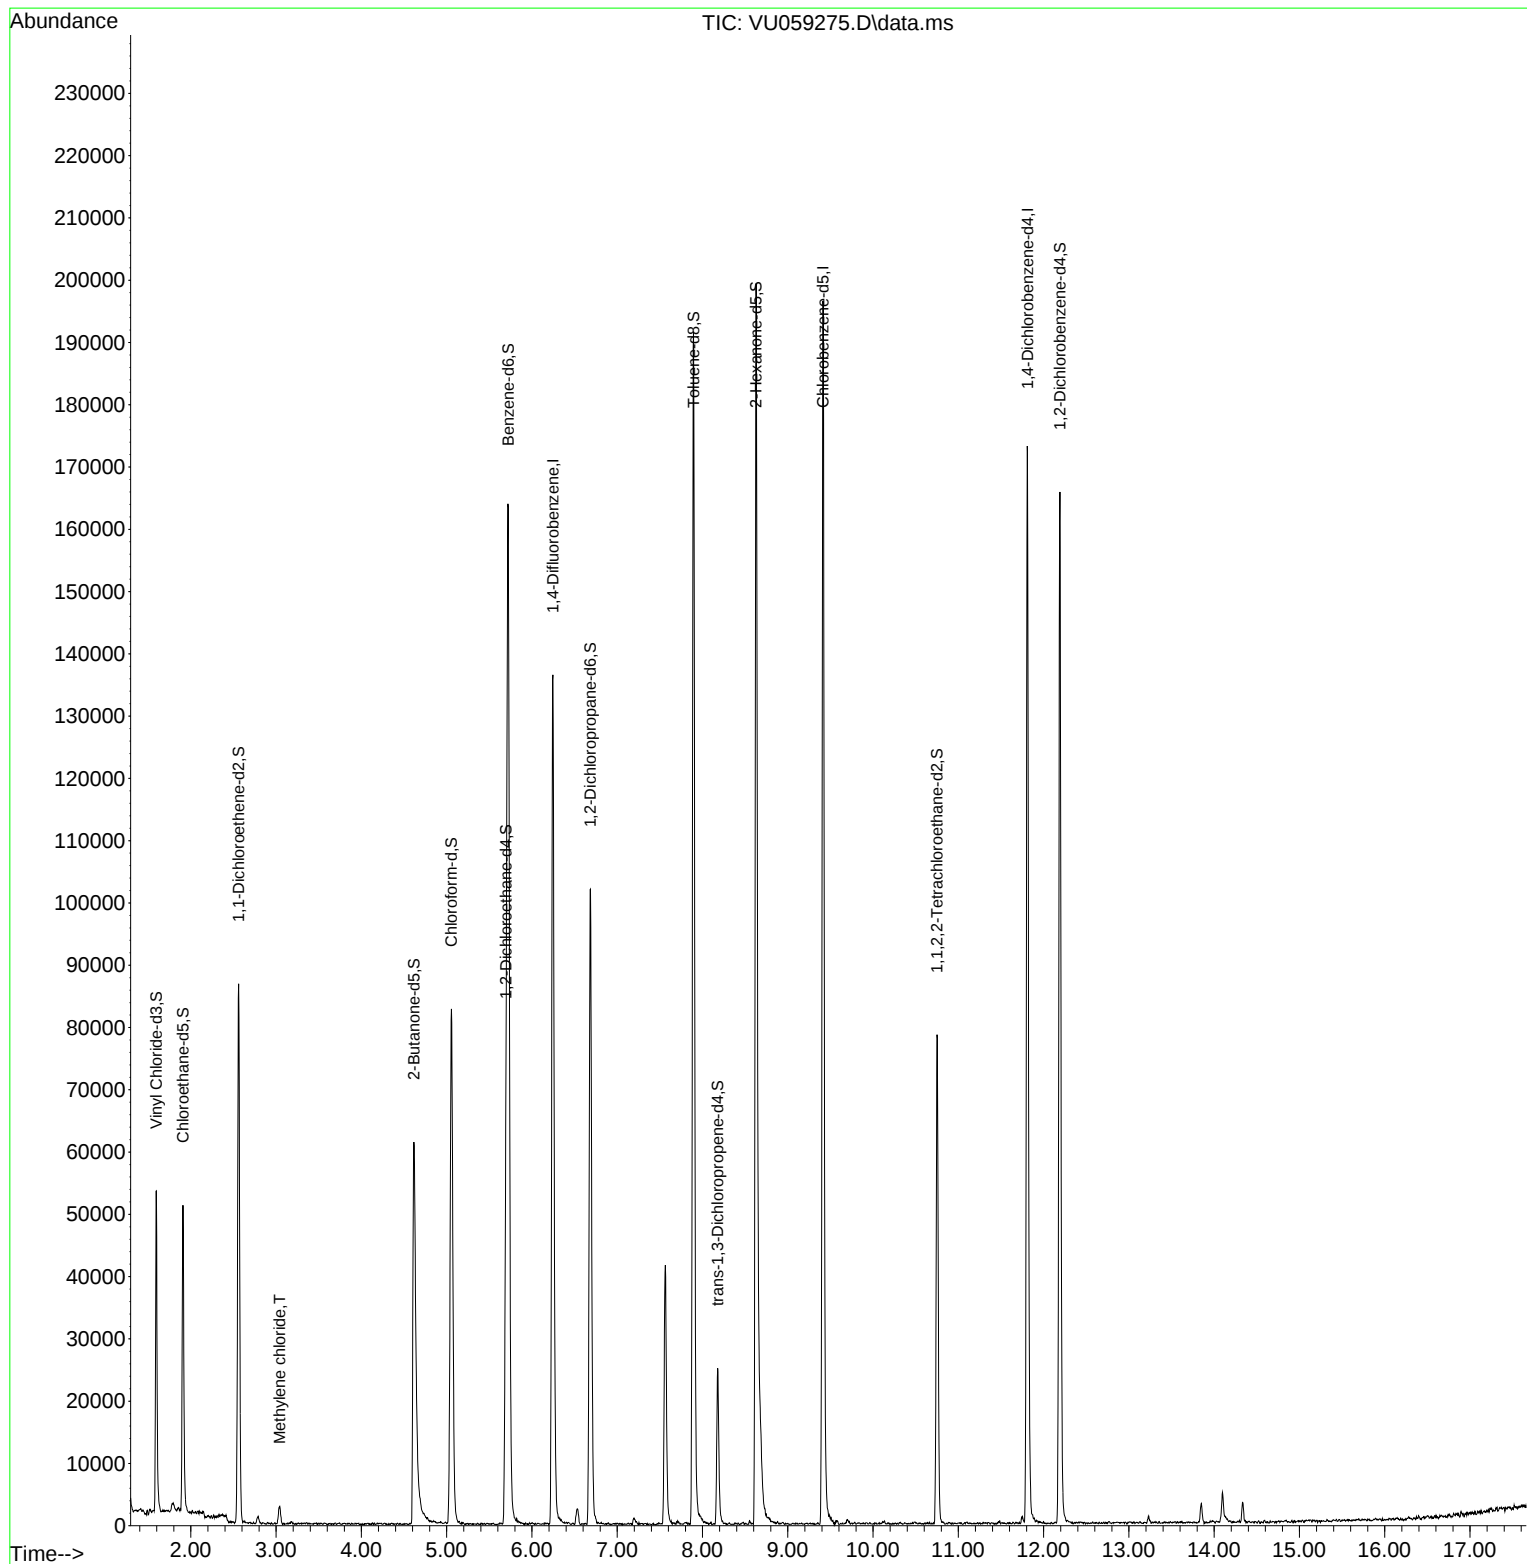

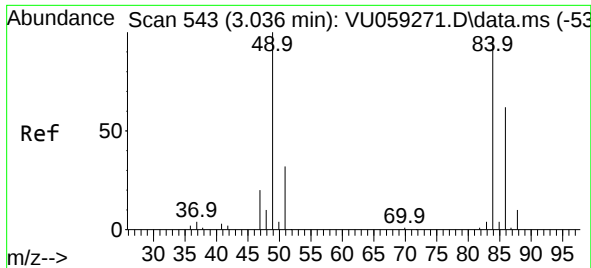

#16
Methylene chloride
Concen: 0.149 ug/L
RT: 3.039 min Scan# 54
Delta R.T. 0.000 min
Lab File: VU059275.D
Acq: 17 Jun 2024 13:03

Instrument :
MSVOA_U
ClientSampleId :
VBLK195

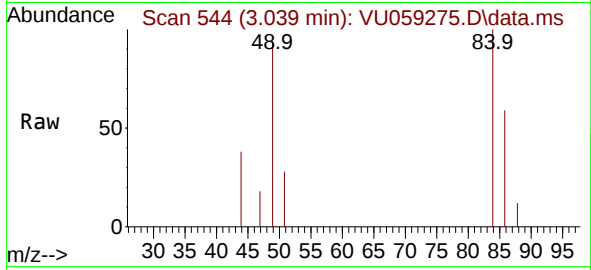

Tgt Ion: 84 Resp: 1448

Ion	Ratio	Lower	Upper
84	100		
86	59.0	42.1	78.1
49	93.8	80.6	149.8

