

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
 Data File : VU059276.D
 Acq On : 17 Jun 2024 13:35
 Operator : MD/SY
 Sample : P2895-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHAZ2

Quant Time: Jun 17 14:03:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 17 12:07:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	111103	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	112439	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	48744	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	38182	4.942	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.800%
7) Chloroethane-d5	1.908	69	37611	5.060	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.200%
11) 1,1-Dichloroethene-d2	2.560	65	15722	4.905	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	98.200%
20) 2-Butanone-d5	4.615	46	90992	57.179	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.360%
24) Chloroform-d	5.055	84	77507	4.888	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
26) 1,2-Dichloroethane-d4	5.695	65	39296	5.144	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.800%
32) Benzene-d6	5.721	84	157289	5.083	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.600%
36) 1,2-Dichloropropane-d6	6.685	67	49628	5.234	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.600%
41) Toluene-d8	7.894	98	131678	4.577	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.600%
43) trans-1,3-Dichloroprop...	8.177	79	15263	5.140	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	102.800%
46) 2-Hexanone-d5	8.627	63	65122	52.785	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.580%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	41024	5.236	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.800%
66) 1,2-Dichlorobenzene-d4	12.190	152	48267	5.564	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.200%
Target Compounds						
					Qvalue	
13) Acetone	2.625	43	9481	9.184	ug/L	95
16) Methylene chloride	3.043	84	1582	0.169	ug/L	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061724\
Data File : VU059276.D
Acq On : 17 Jun 2024 13:35
Operator : MD/SY
Sample : P2895-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAZ2

Quant Time: Jun 17 14:03:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 17 12:07:46 2024
Response via : Initial Calibration

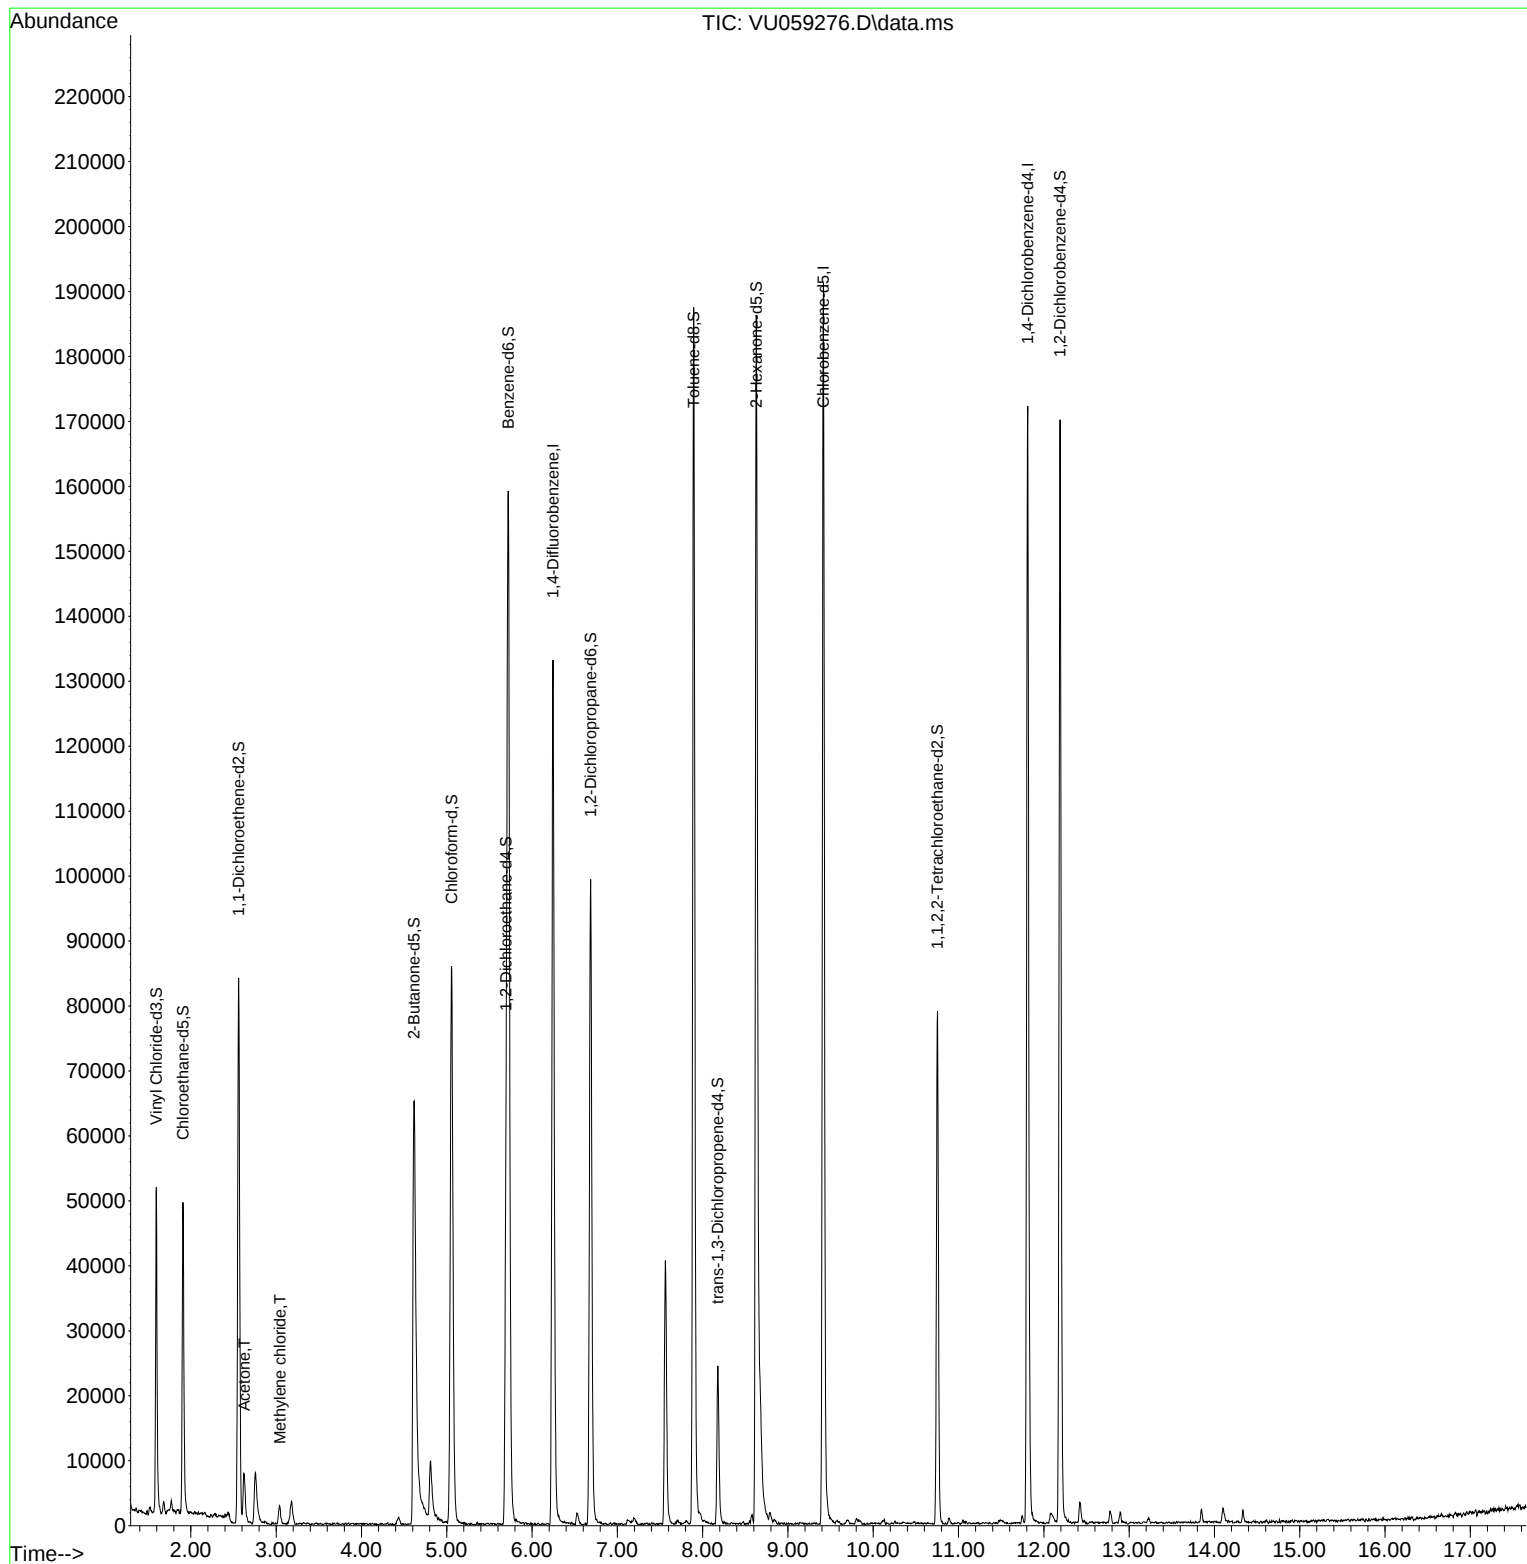

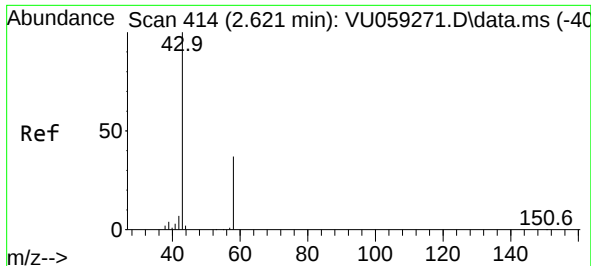

#13

Acetone

Concen: 9.184 ug/L

RT: 2.625 min Scan# 41

Delta R.T. -0.016 min

Lab File: VU059276.D

Acq: 17 Jun 2024 13:35

Instrument :

MSVOA_U

ClientSampleId :





BHAZ2

Tgt Ion: 43 Resp: 9481

Ion Ratio Lower Upper

43 100

58 36.6 0.0 68.0

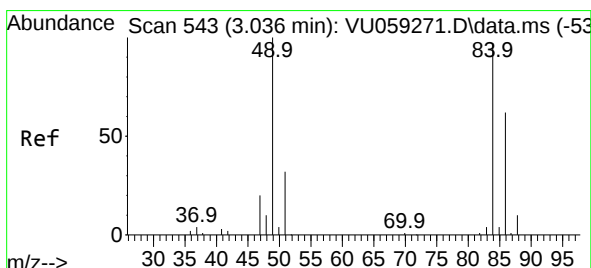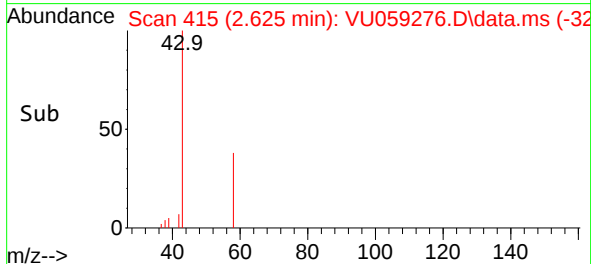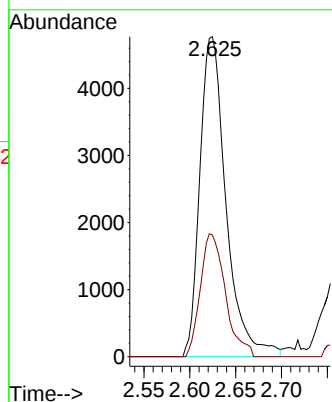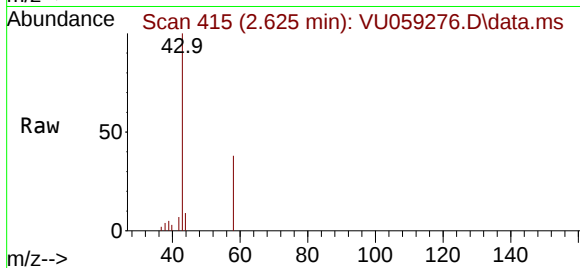

#16

Methylene chloride

Concen: 0.169 ug/L

RT: 3.043 min Scan# 545

Delta R.T. 0.003 min

Lab File: VU059276.D

Acq: 17 Jun 2024 13:35

Tgt Ion: 84 Resp: 1582

Ion Ratio Lower Upper

84 100

86 54.4 42.1 78.1

49 82.1 80.6 149.8

